


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP092419\
 Data File : BP000381.D
 Acq On : 24 Sep 2019 11:30
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 19 14:44:51 2019

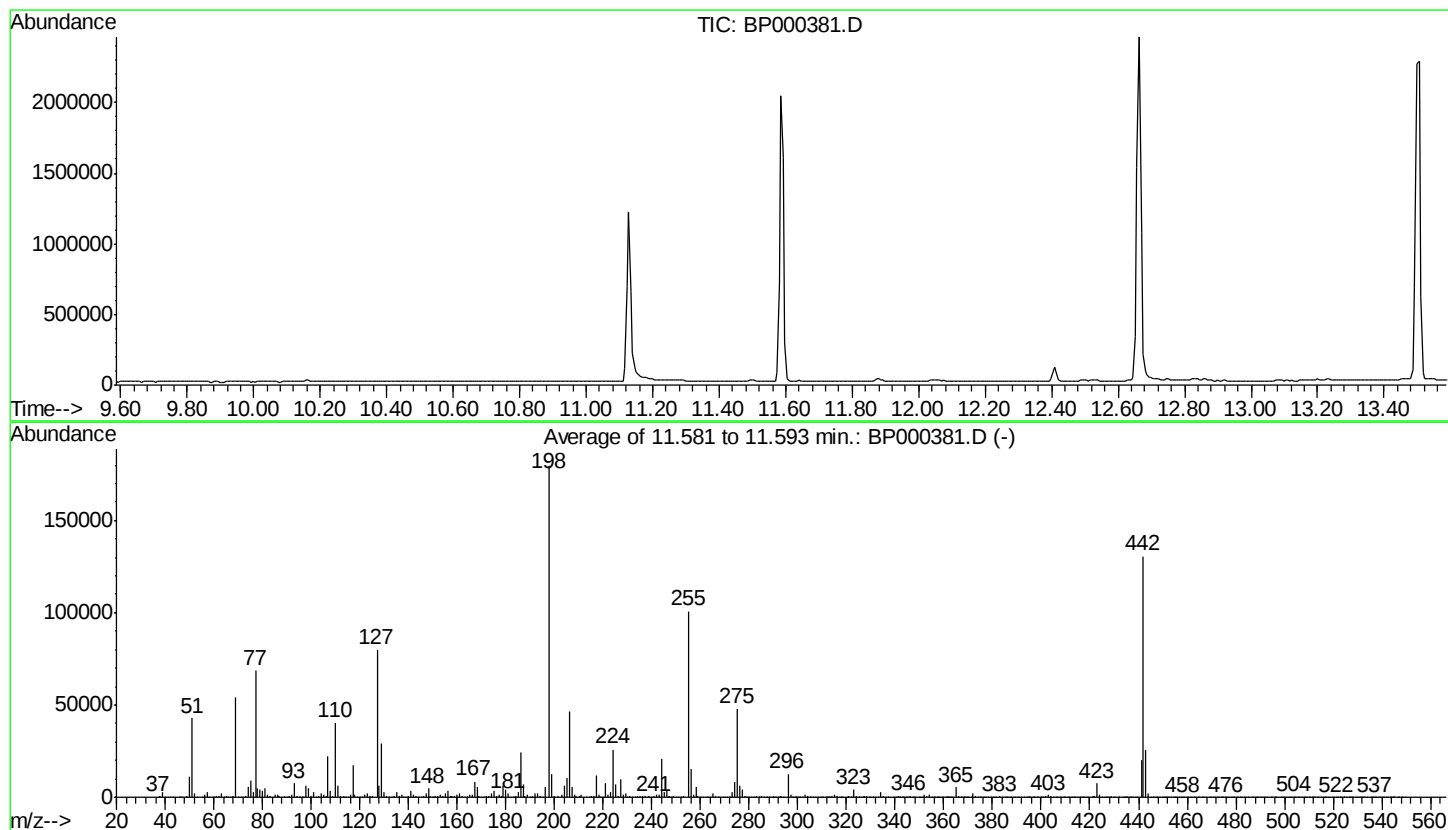

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.9	43000	PASS
68	69	0.00	2	1.9	1037	PASS
69	198	0.00	100	30.0	53905	PASS
70	69	0.00	2	0.6	335	PASS
127	198	10	80	44.5	79984	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	179720	PASS
199	198	5	9	7.1	12718	PASS
275	198	10	60	26.8	48111	PASS
365	198	1	100	3.0	5428	PASS
441	198	0.01	100	11.3	20305	PASS
442	198	50	100	72.8	130784	PASS
443	442	15	24	19.5	25469	PASS