
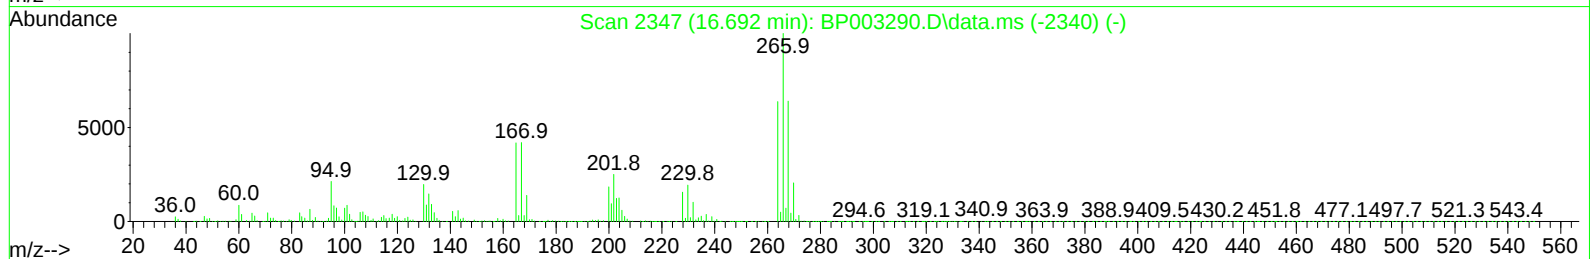
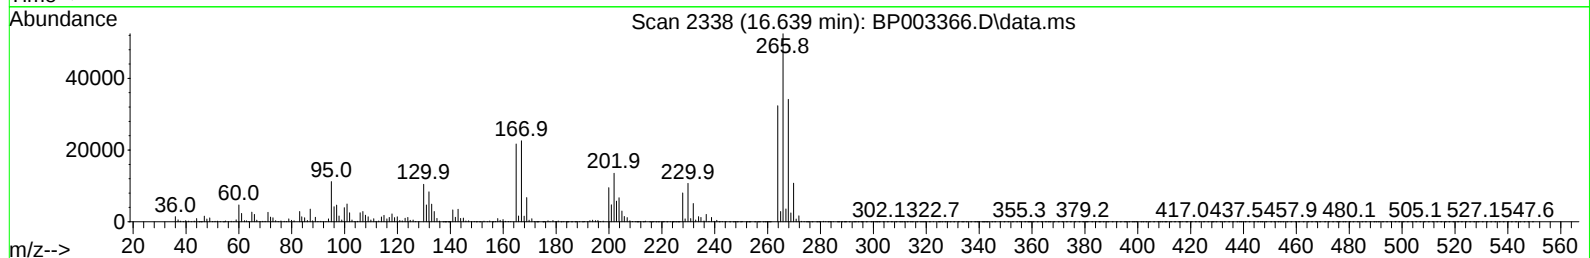


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092420\
 Data File : BP003366.D
 Acq On : 24 Sep 2020 11:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 05:05:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 22 12:48:08 2020
 Response via : Initial Calibration

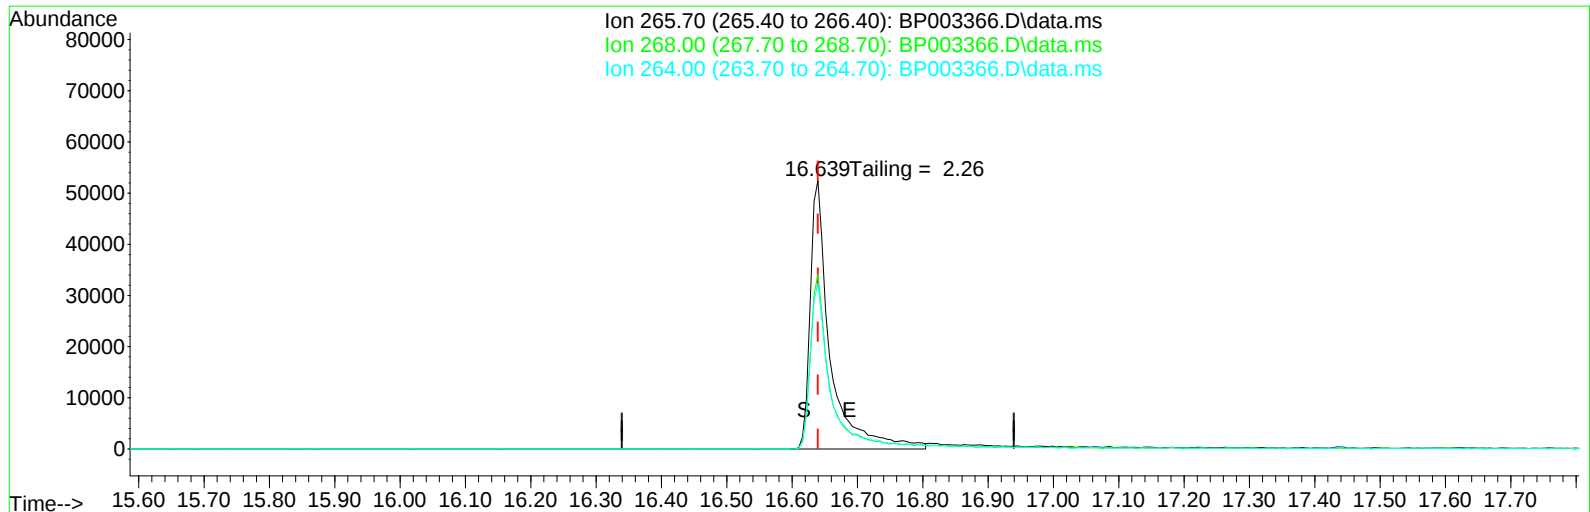

TIC: BP003366.D\data.ms

(70) Pentachlorophenol (C)




16.639min (+ 0.000) 25531.59 ng

response 111206

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.10
264.00	63.30	61.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092420\
 Data File : BP003366.D
 Acq On : 24 Sep 2020 11:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 05:05:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 22 12:48:08 2020
 Response via : Initial Calibration

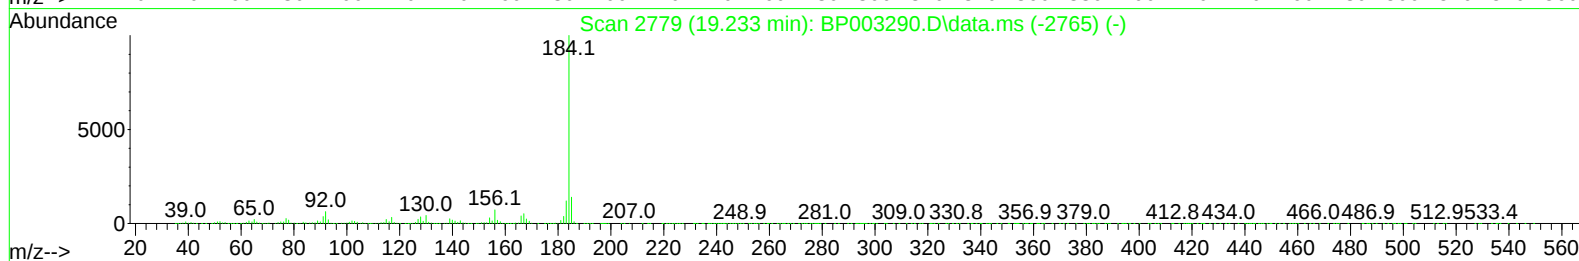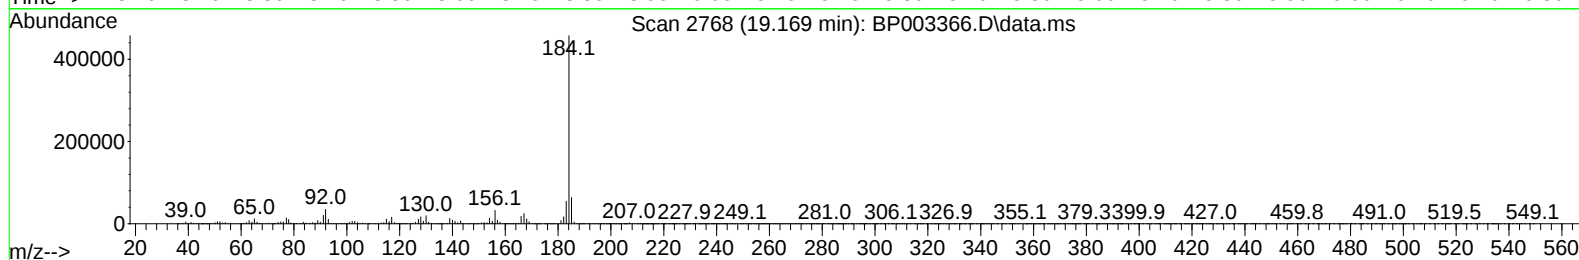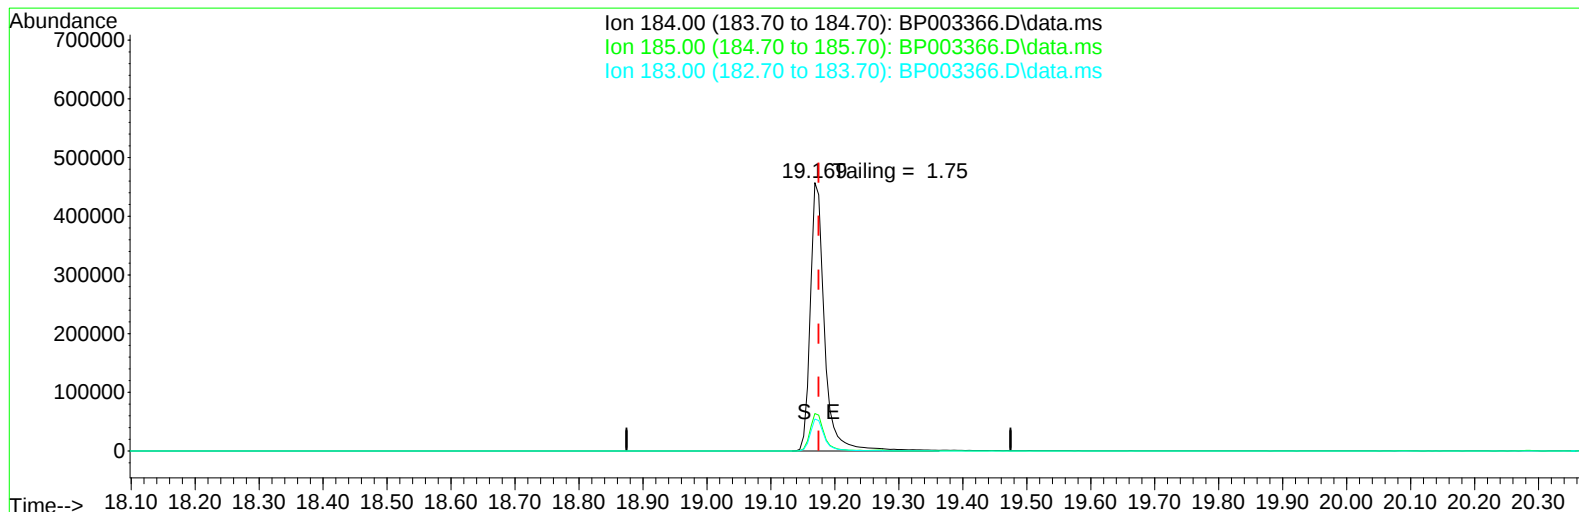

TIC: BP003366.D\data.ms

(77) Benzidine**19.169min (-0.006) 14132.27 ng****response 711239**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.94
183.00	12.00	11.91
0.00	0.00	0.00