
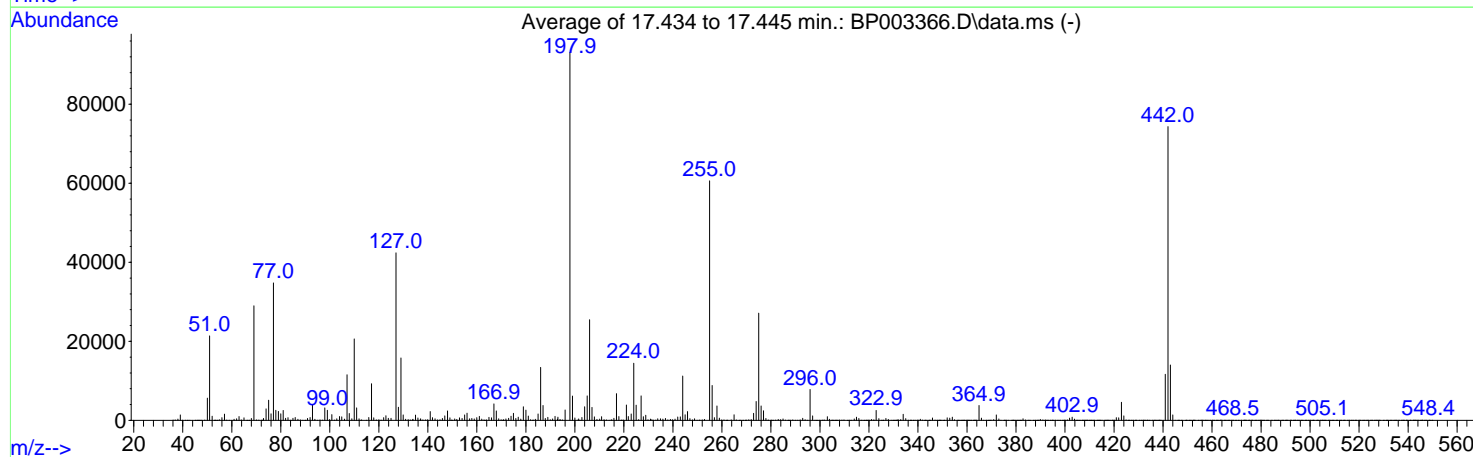


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092420\
 Data File : BP003366.D
 Acq On : 24 Sep 2020 11:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 22 12:48:08 2020

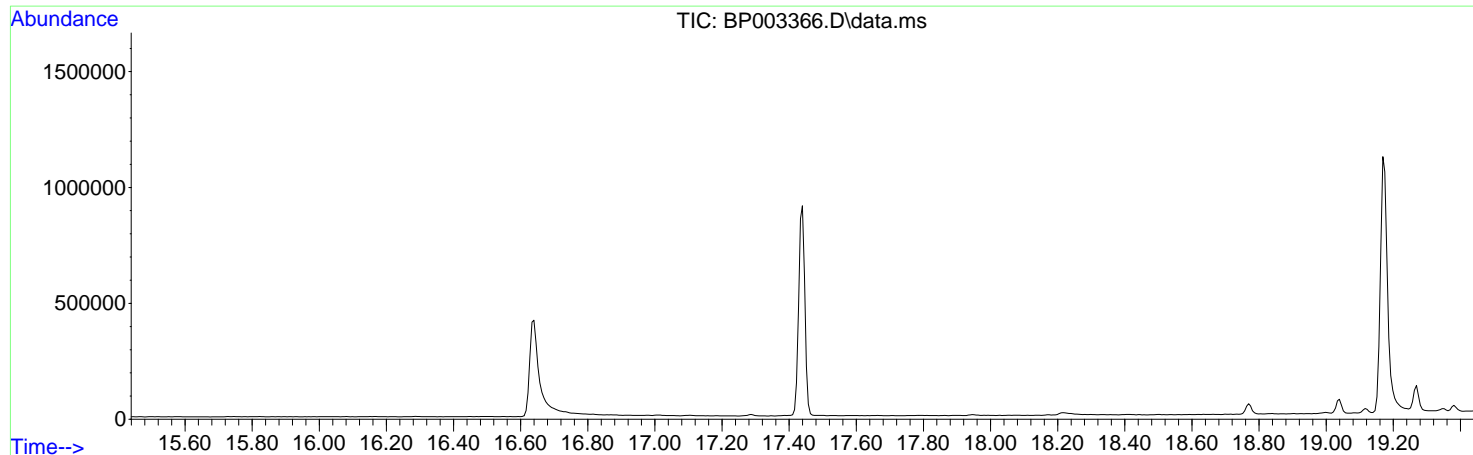

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	21372	PASS
68	69	0.00	2	1.7	498	PASS
69	198	0.00	100	31.1	28980	PASS
70	69	0.00	2	0.4	116	PASS
127	198	10	80	45.5	42401	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93088	PASS
199	198	5	9	6.6	6158	PASS
275	198	10	60	29.2	27139	PASS
365	198	1	100	4.0	3755	PASS
441	198	0.01	100	12.5	11649	PASS
442	198	50	100	79.8	74323	PASS
443	442	15	24	18.9	14024	PASS