

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092421\
 Data File : BP007159.D
 Acq On : 24 Sep 2021 15:10
 Operator : CG/JU
 Sample : M3911-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SW-RR-01-(2.0)

Quant Time: Sep 24 17:06:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	242125	20.000	ng	0.00
21) Naphthalene-d8	10.687	136	927962	20.000	ng	# 0.00
39) Acenaphthene-d10	14.516	164	578639	20.000	ng	-0.01
64) Phenanthrene-d10	17.269	188	1219601	20.000	ng	# 0.00
76) Chrysene-d12	21.357	240	1264590	20.000	ng	# 0.00
86) Perylene-d12	23.768	264	1364581	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.463	112	923250	63.829	ng	0.00
7) Phenol-d6	7.057	99	681251	34.460	ng	0.00
23) Nitrobenzene-d5	9.051	82	1393589	87.458	ng	0.00
42) 2,4,6-Tribromophenol	16.010	330	1059569	141.243	ng	0.00
45) 2-Fluorobiphenyl	13.145	172	3440567	85.183	ng	0.00
79) Terphenyl-d14	19.827	244	5319571	80.609	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092421\
Data File : BP007159.D
Acq On : 24 Sep 2021 15:10
Operator : CG/JU
Sample : M3911-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SW-RR-01-(2.0)

Quant Time: Sep 24 17:06:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 23 11:17:25 2021
Response via : Initial Calibration




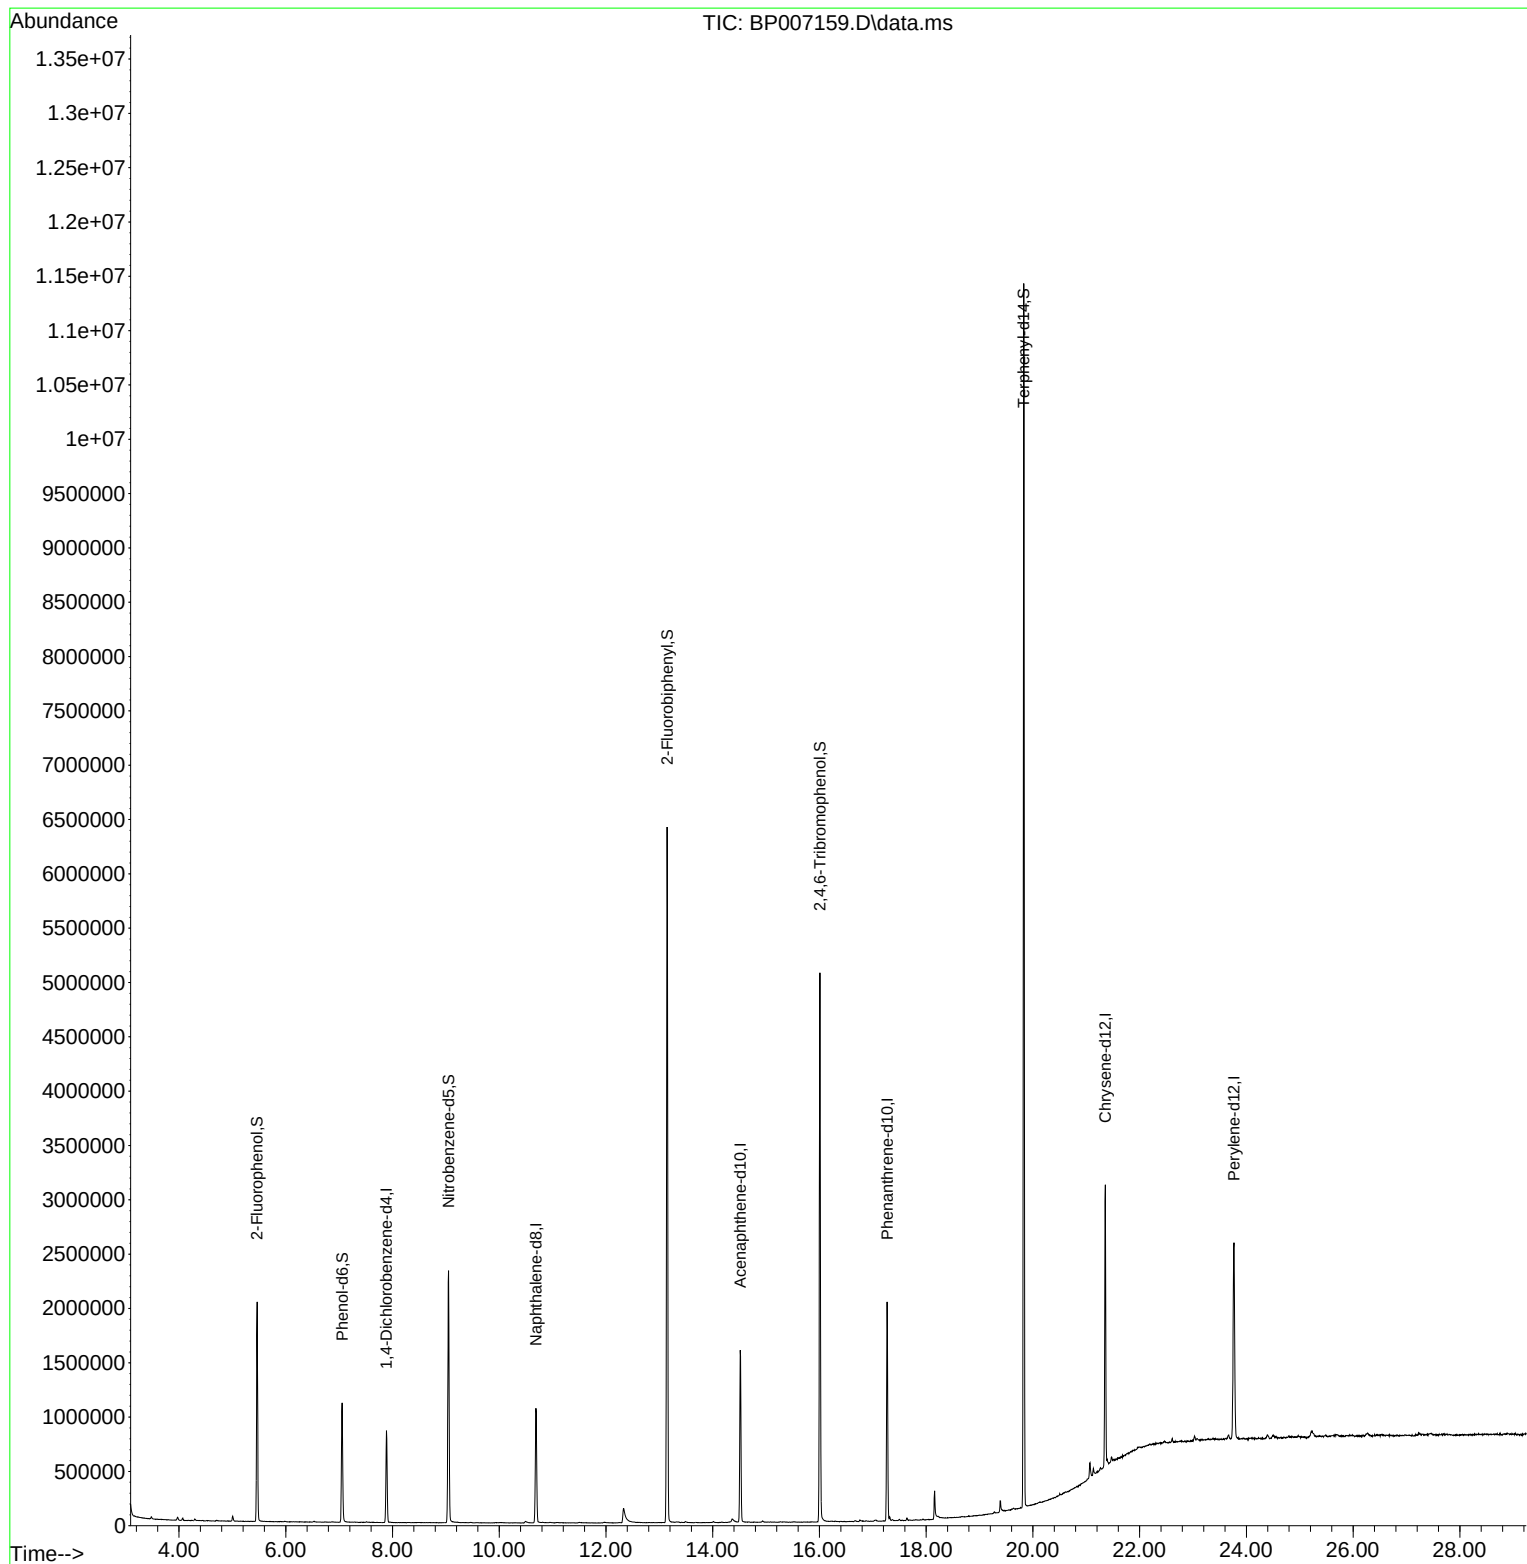




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.887 min Scan# 816
Delta R.T. -0.006 min
Lab File: BP007159.D
Acq: 24 Sep 2021 15:10




Instrument :
BNA_P
ClientSampleId :
SW-RR-01-(2.0)


Tgt Ion:152 Resp: 242125
Ion Ratio Lower Upper
152 100
150 157.9 125.6 188.4
115 56.7 48.5 72.7

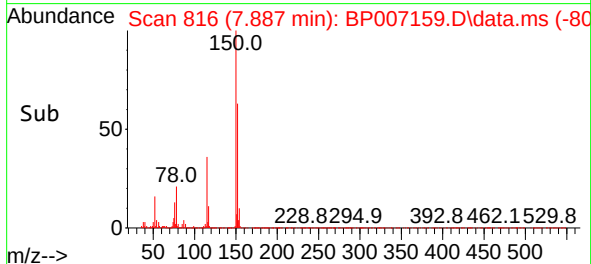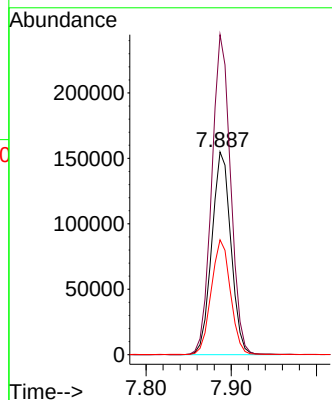

#5
2-Fluorophenol
Concen: 63.829 ng
RT: 5.463 min Scan# 404
Delta R.T. -0.000 min
Lab File: BP007159.D
Acq: 24 Sep 2021 15:10

Tgt Ion:112 Resp: 923250
Ion Ratio Lower Upper
112 100
64 52.7 41.4 62.2
63 26.7 23.8 35.8


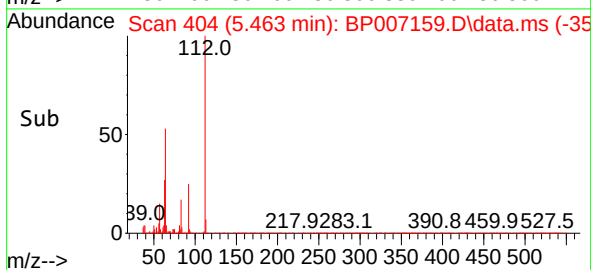
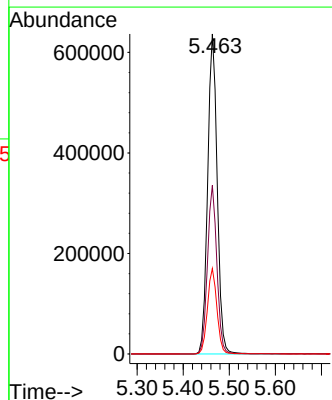
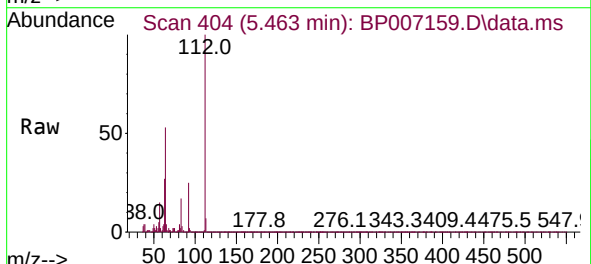




#7
Phenol-d6
Concen: 34.460 ng
RT: 7.057 min Scan# 675
Delta R.T. -0.006 min
Lab File: BP007159.D
Acq: 24 Sep 2021 15:10




Instrument :
BNA_P
ClientSampleId :
SW-RR-01-(2.0)


Tgt Ion: 99 Resp: 681251
Ion Ratio Lower Upper
99 100
42 14.2 13.4 20.0
71 30.4 30.6 46.0#

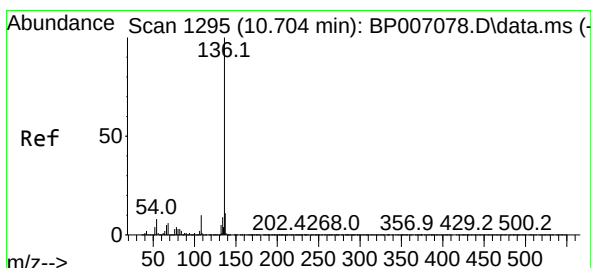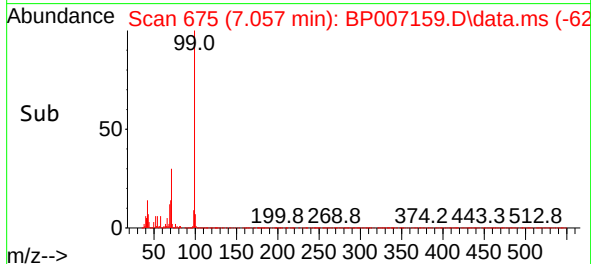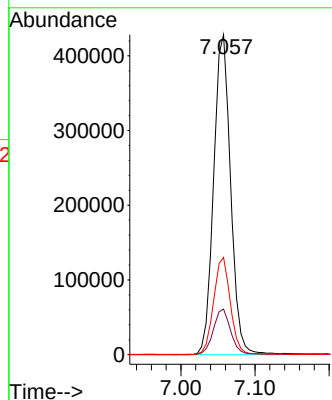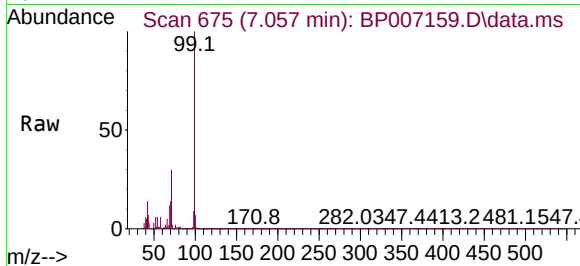

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.687 min Scan# 1292
Delta R.T. -0.006 min
Lab File: BP007159.D
Acq: 24 Sep 2021 15:10

Tgt Ion: 136 Resp: 927962
Ion Ratio Lower Upper
136 100
137 11.0 8.6 12.8
54 7.0 4.6 6.8#
68 5.7 3.6 5.4#

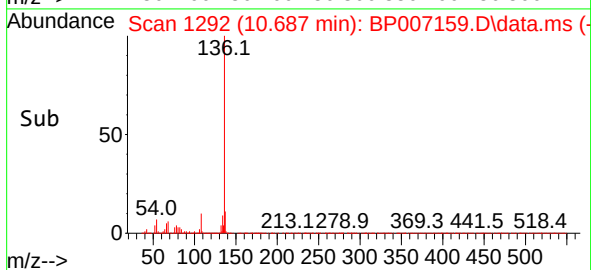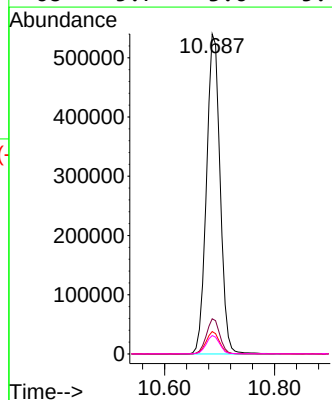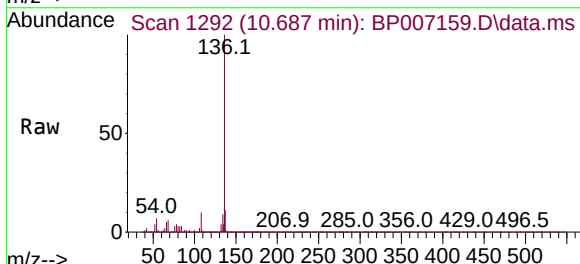







#23
Nitrobenzene-d5
Concen: 87.458 ng
RT: 9.051 min Scan# 1014
Delta R.T. -0.006 min
Lab File: BP007159.D
Acq: 24 Sep 2021 15:10

Instrument :
BNA_P
ClientSampleId :
SW-RR-01-(2.0)

Tgt Ion: 82 Resp: 1393589




Ion	Ratio	Lower	Upper
82	100		
128	48.2	35.7	53.5
54	44.3	35.0	52.4

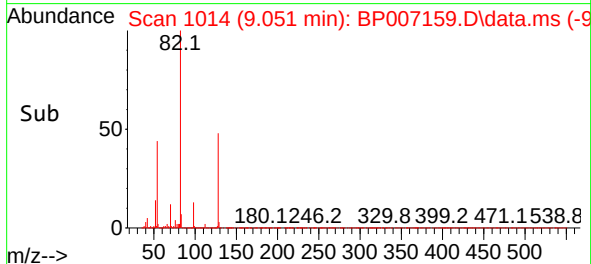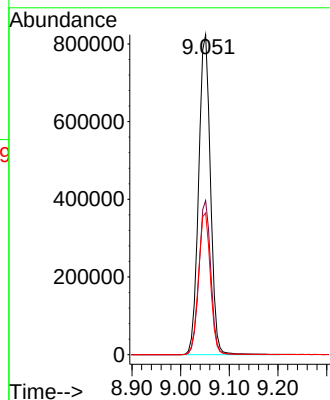


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.516 min Scan# 1943
Delta R.T. -0.012 min
Lab File: BP007159.D
Acq: 24 Sep 2021 15:10

Tgt Ion: 164 Resp: 578639

Ion	Ratio	Lower	Upper
164	100		
162	101.6	80.2	120.2
160	45.0	34.5	51.7


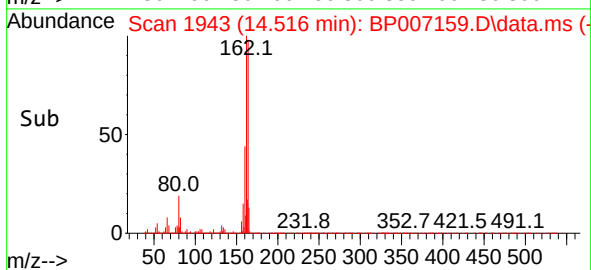
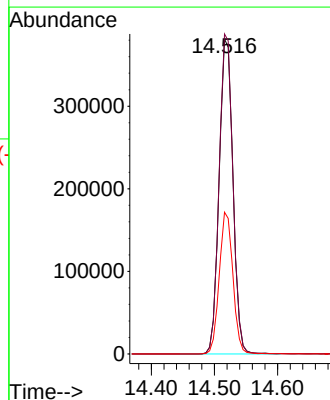
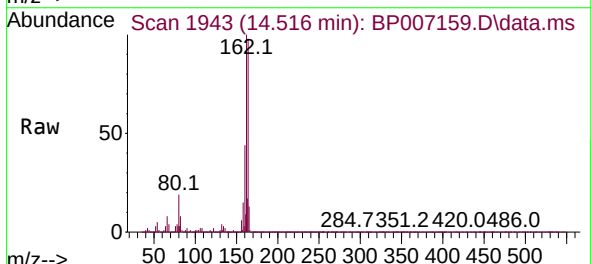




#42
2,4,6-Tribromophenol
Concen: 141.243 ng
RT: 16.010 min Scan# 2197
Delta R.T. -0.006 min
Lab File: BP007159.D
Acq: 24 Sep 2021 15:10




Instrument :
BNA_P
ClientSampleId :
SW-RR-01-(2.0)


Tgt Ion:330 Resp: 1059569
Ion Ratio Lower Upper
330 100
332 96.8 77.8 116.8
141 29.2 25.4 38.2

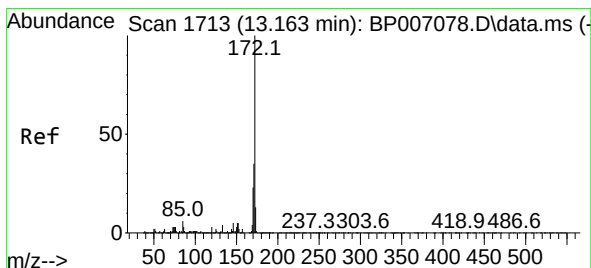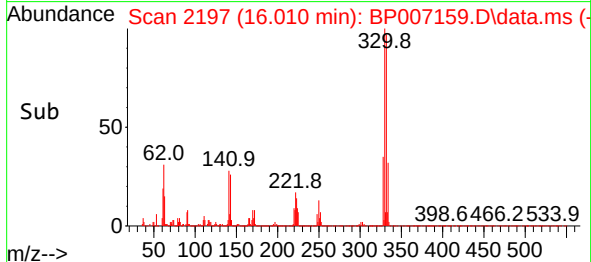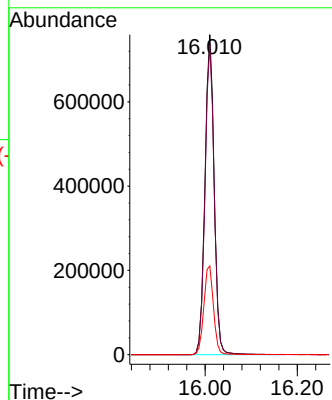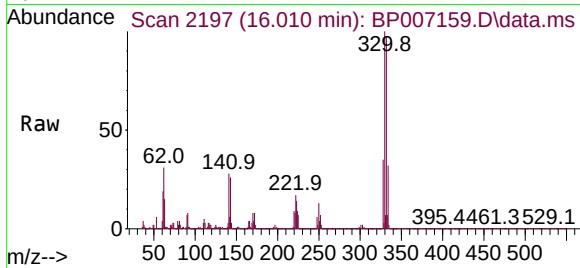

#45
2-Fluorobiphenyl
Concen: 85.183 ng
RT: 13.145 min Scan# 1710
Delta R.T. -0.006 min
Lab File: BP007159.D
Acq: 24 Sep 2021 15:10

Tgt Ion:172 Resp: 3440567
Ion Ratio Lower Upper
172 100
171 35.2 27.9 41.9
170 23.3 18.6 27.8


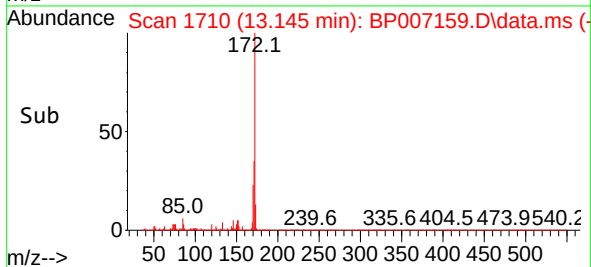
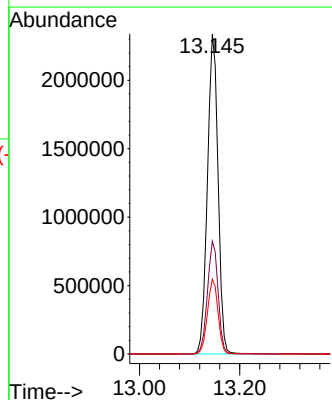
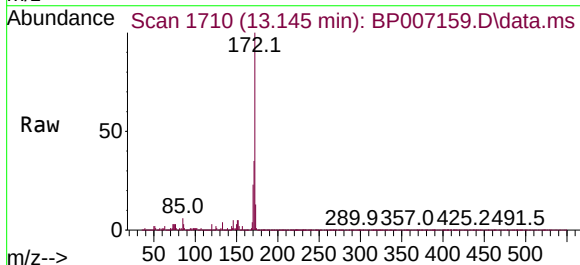




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.269 min Scan# 2411
Delta R.T. -0.006 min
Lab File: BP007159.D
Acq: 24 Sep 2021 15:10




Instrument :
BNA_P
ClientSampleId :
SW-RR-01-(2.0)


Tgt Ion:188 Resp: 1219601
Ion Ratio Lower Upper
188 100
94 9.0 5.6 8.4#
80 9.0 6.3 9.5

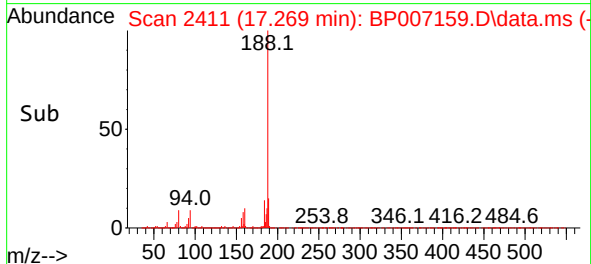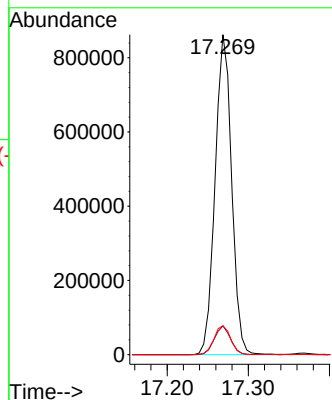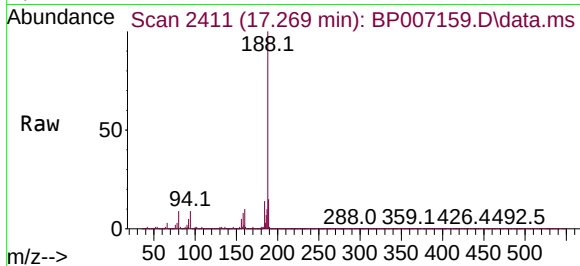

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.357 min Scan# 3106
Delta R.T. -0.000 min
Lab File: BP007159.D
Acq: 24 Sep 2021 15:10

Tgt Ion:240 Resp: 1264590
Ion Ratio Lower Upper
240 100
120 10.2 6.5 9.7#
236 26.4 20.6 31.0

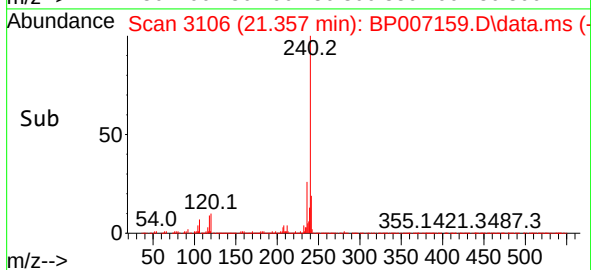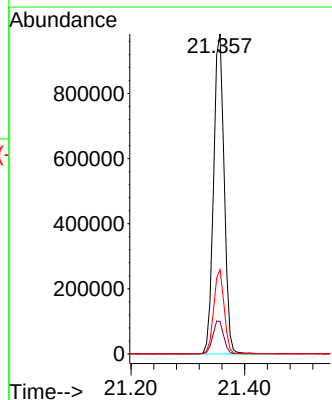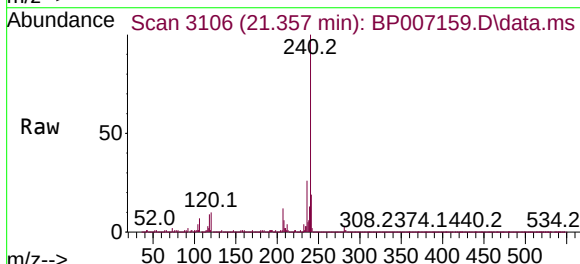







#79
 Terphenyl-d14
 Concen: 80.609 ng
 RT: 19.827 min Scan# 2846
 Delta R.T. -0.006 min
 Lab File: BP007159.D
 Acq: 24 Sep 2021 15:10

Instrument :
 BNA_P
 ClientSampleId :
 SW-RR-01-(2.0)

Tgt Ion:244 Resp: 5319571

Ion	Ratio	Lower	Upper
244	100		
212	7.1	6.0	9.0
122	9.9	7.1	10.7

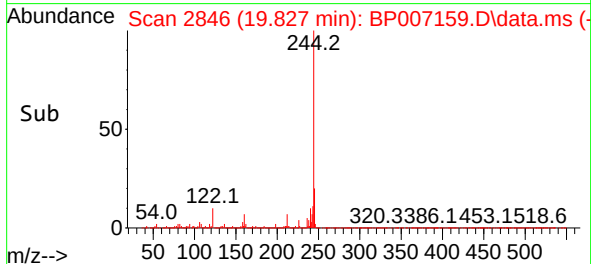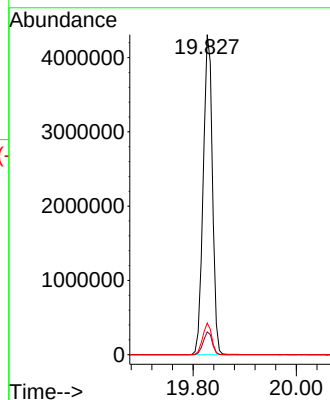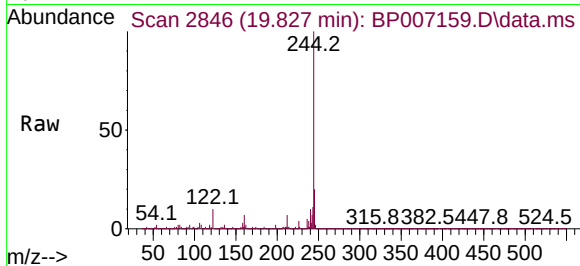

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.768 min Scan# 3516
 Delta R.T. -0.000 min
 Lab File: BP007159.D
 Acq: 24 Sep 2021 15:10

Tgt Ion:264 Resp: 1364581

Ion	Ratio	Lower	Upper
264	100		
260	24.1	18.6	28.0
265	22.4	17.6	26.4

