
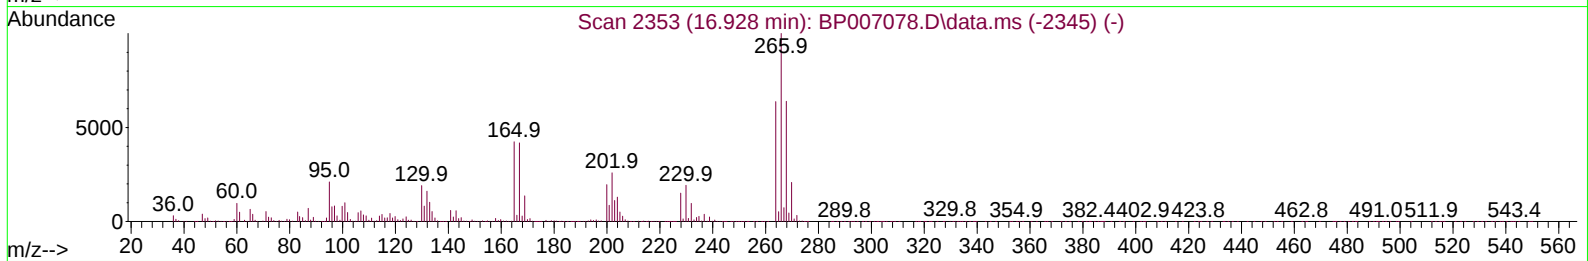
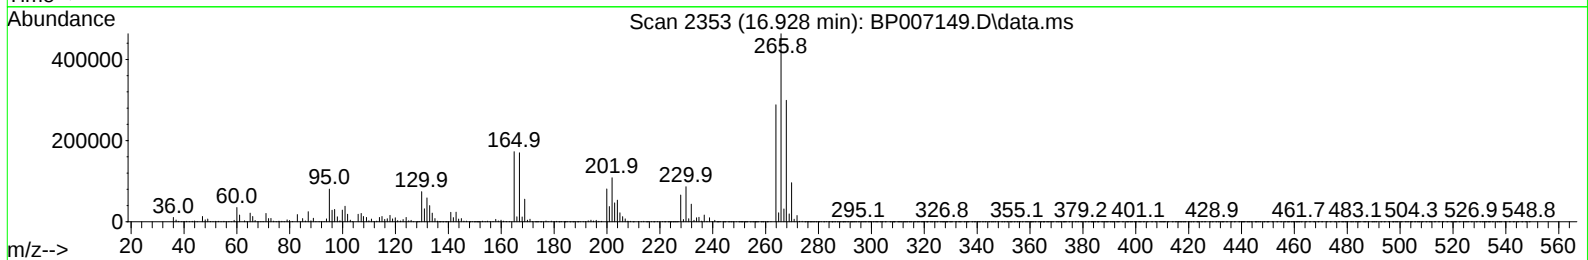


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092421\
 Data File : BP007149.D
 Acq On : 24 Sep 2021 09:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 11:03:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

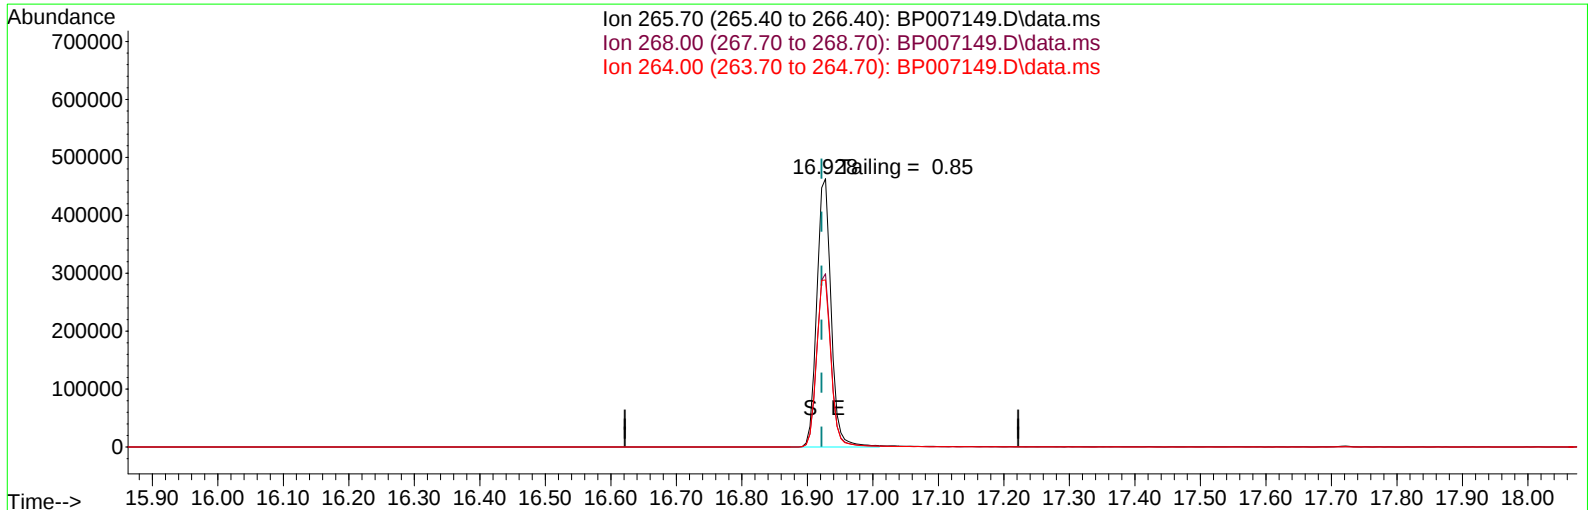

TIC: BP007149.D\data.ms

(70) Pentachlorophenol (C)




16.928min (+ 0.006) 658939.33 ng

response 708817

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.57
264.00	62.90	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092421\
 Data File : BP007149.D
 Acq On : 24 Sep 2021 09:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 11:03:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

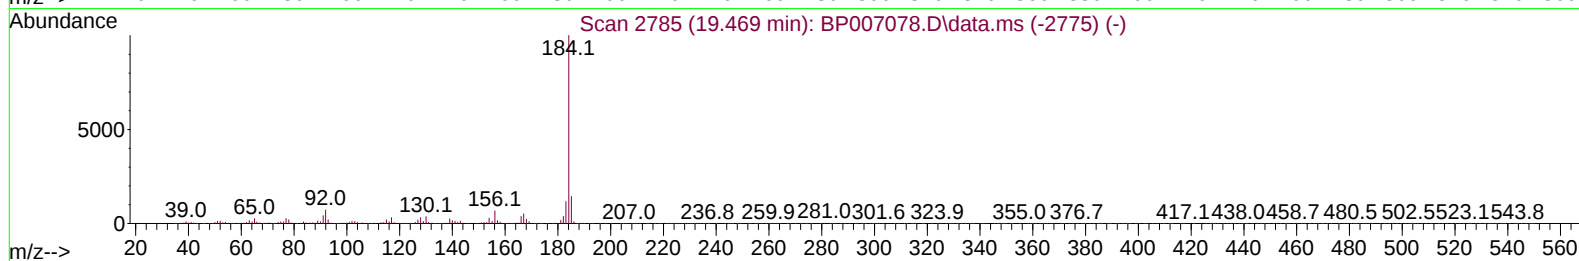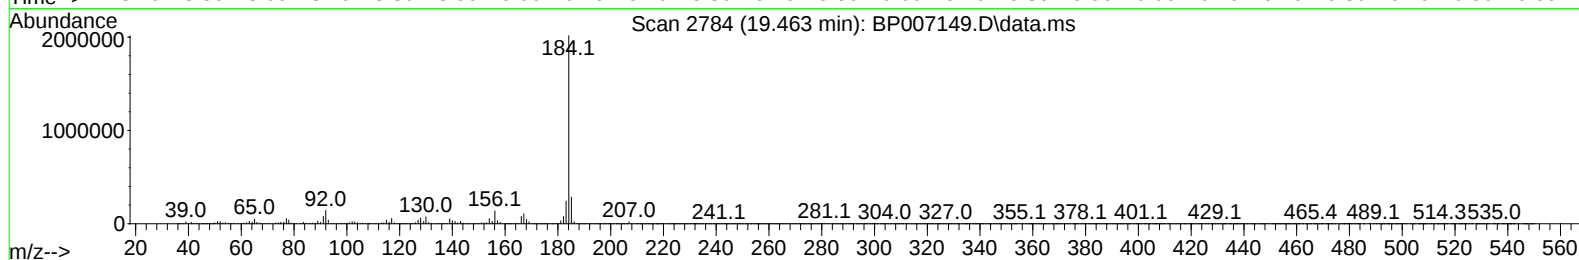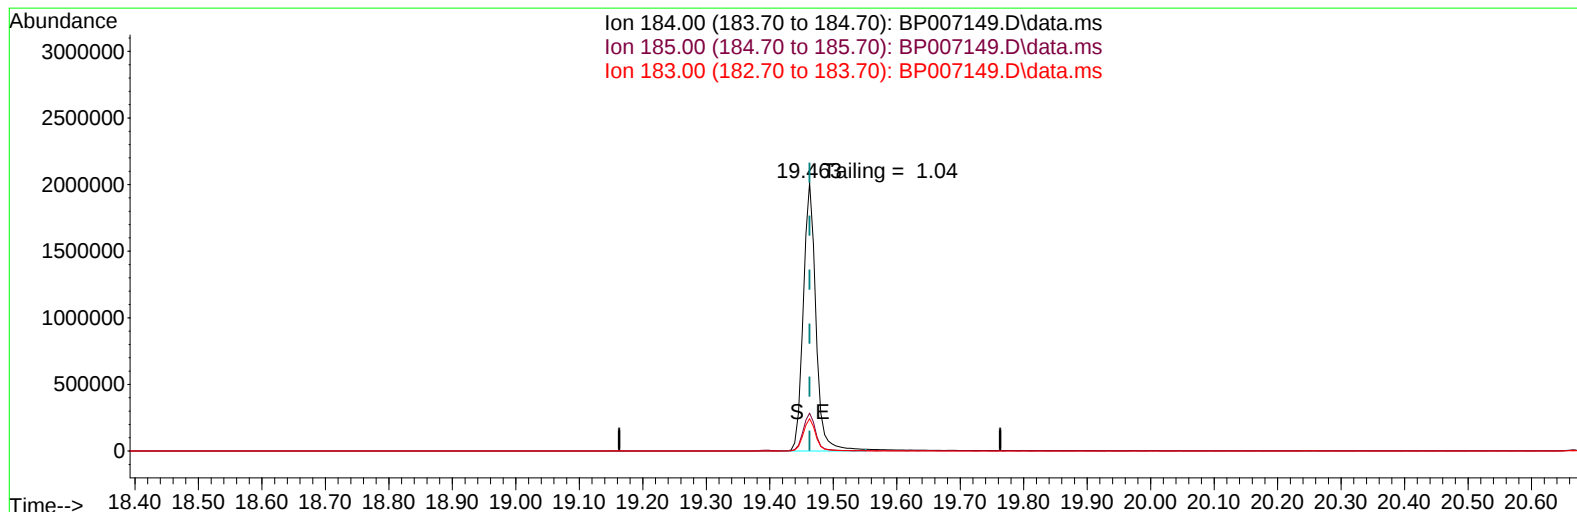

TIC: BP007149.D\data.ms

(77) Benzidine**19.463min (-0.000) 246204.84 ng****response 2852480**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.15
183.00	11.90	12.08
0.00	0.00	0.00