

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP092421\  
 Data File : BP007157.D  
 Acq On : 24 Sep 2021 13:59  
 Operator : CG/JU  
 Sample : M3823-02  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DKM-ENV-IC

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007157.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.369       | 44            | 48          | 57           | rVB      | 394489         | 458686        | 2.96%           | 0.564%        |
| 2         | 3.616       | 86            | 90          | 98           | rBV      | 138221         | 211433        | 1.36%           | 0.260%        |
| 3         | 4.516       | 238           | 243         | 248          | rBV      | 512485         | 741268        | 4.78%           | 0.912%        |
| 4         | 4.587       | 250           | 255         | 258          | rBV3     | 91039          | 178992        | 1.15%           | 0.220%        |
| 5         | 4.975       | 316           | 321         | 324          | rBV      | 249448         | 341846        | 2.20%           | 0.420%        |
| 6         | 5.010       | 324           | 327         | 335          | rVB      | 209774         | 289996        | 1.87%           | 0.357%        |
| 7         | 5.469       | 398           | 405         | 414          | rBV      | 4131920        | 5995853       | 38.63%          | 7.375%        |
| 8         | 6.034       | 490           | 501         | 516          | rBV3     | 46648          | 172479        | 1.11%           | 0.212%        |
| 9         | 7.063       | 668           | 676         | 690          | rBV      | 3450605        | 5637314       | 36.32%          | 6.934%        |
| 10        | 7.893       | 808           | 817         | 824          | rBV      | 967327         | 1538879       | 9.92%           | 1.893%        |
| 11        | 9.051       | 1006          | 1014        | 1031         | rBV      | 2530434        | 4200522       | 27.06%          | 5.167%        |
| 12        | 10.475      | 1249          | 1256        | 1273         | rBV      | 762287         | 1419588       | 9.15%           | 1.746%        |
| 13        | 10.692      | 1284          | 1293        | 1300         | rBV      | 1245086        | 2106010       | 13.57%          | 2.590%        |
| 14        | 11.957      | 1500          | 1508        | 1517         | rBV      | 117916         | 210049        | 1.35%           | 0.258%        |
| 15        | 12.381      | 1564          | 1580        | 1598         | rBV      | 2164710        | 5917864       | 38.13%          | 7.279%        |
| 16        | 13.145      | 1703          | 1710        | 1725         | rBV      | 6707746        | 10242347      | 65.99%          | 12.598%       |
| 17        | 13.328      | 1735          | 1741        | 1752         | rBV      | 184300         | 331154        | 2.13%           | 0.407%        |
| 18        | 13.492      | 1764          | 1769        | 1787         | rVB      | 206389         | 351964        | 2.27%           | 0.433%        |
| 19        | 14.522      | 1937          | 1944        | 1952         | rBV      | 1884734        | 2785120       | 17.95%          | 3.426%        |
| 20        | 16.010      | 2191          | 2197        | 2215         | rVB      | 5449316        | 7998637       | 51.54%          | 9.838%        |
| 21        | 16.774      | 2321          | 2327        | 2343         | rBV      | 787661         | 1115106       | 7.18%           | 1.372%        |
| 22        | 17.269      | 2405          | 2411        | 2417         | rBV      | 2217660        | 3295708       | 21.23%          | 4.054%        |
| 23        | 17.945      | 2521          | 2526        | 2531         | rVB      | 144685         | 176135        | 1.13%           | 0.217%        |
| 24        | 18.163      | 2558          | 2563        | 2572         | rBV      | 960522         | 1318584       | 8.50%           | 1.622%        |
| 25        | 19.392      | 2768          | 2772        | 2786         | rBV      | 445756         | 685076        | 4.41%           | 0.843%        |
| 26        | 19.833      | 2841          | 2847        | 2852         | rBV      | 12081540       | 15520260      | 100.00%         | 19.090%       |
| 27        | 21.068      | 3053          | 3057        | 3063         | rBV3     | 361560         | 488924        | 3.15%           | 0.601%        |
| 28        | 21.357      | 3101          | 3106        | 3111         | rBV      | 2929281        | 3692164       | 23.79%          | 4.541%        |
| 29        | 23.768      | 3510          | 3516        | 3528         | rVB2     | 1853020        | 3877850       | 24.99%          | 4.770%        |




Sum of corrected areas: 81299808

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP092421\  
Data File : BP007157.D  
Acq On : 24 Sep 2021 13:59  
Operator : CG/JU  
Sample : M3823-02  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DKM-ENV-IC

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP092121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

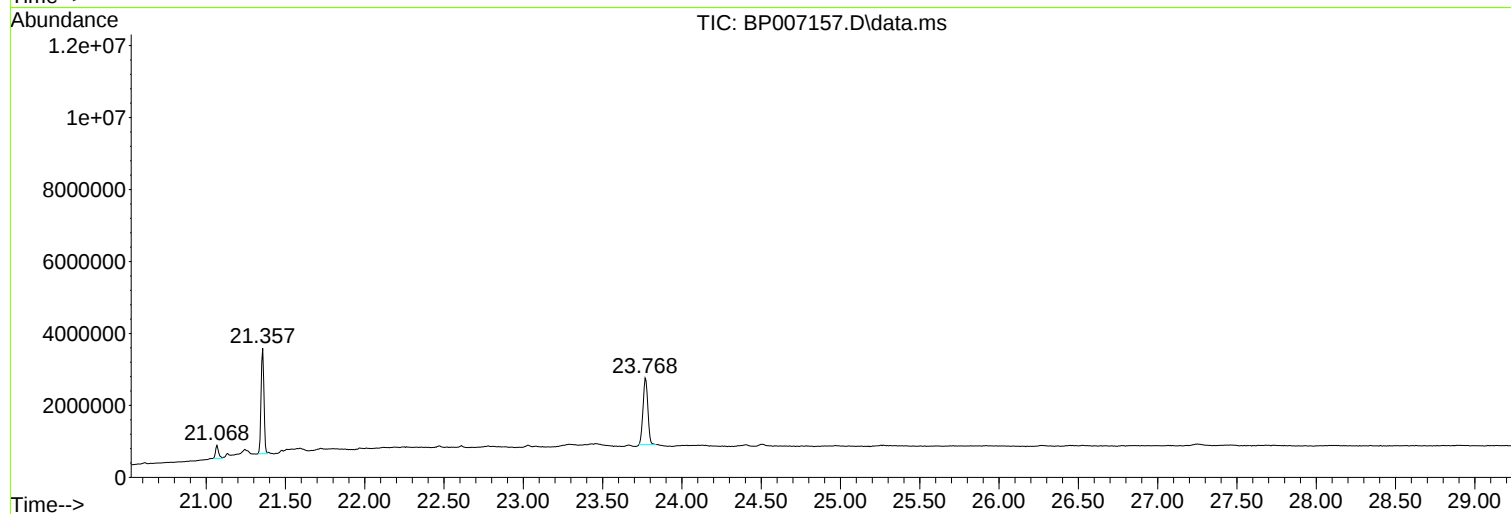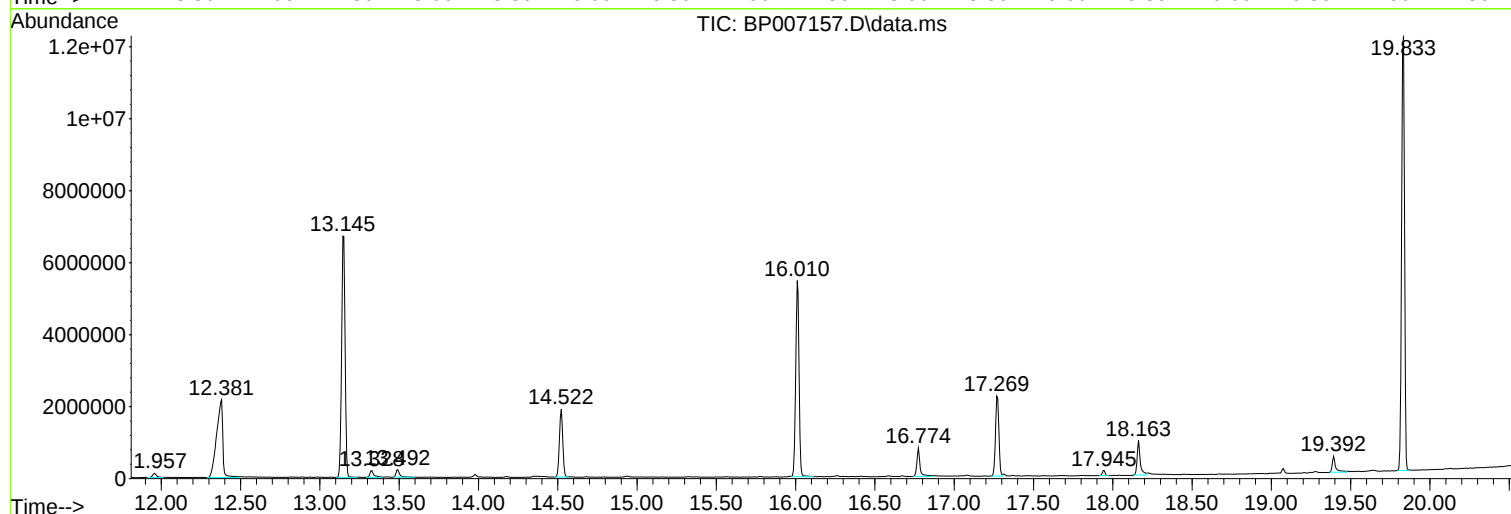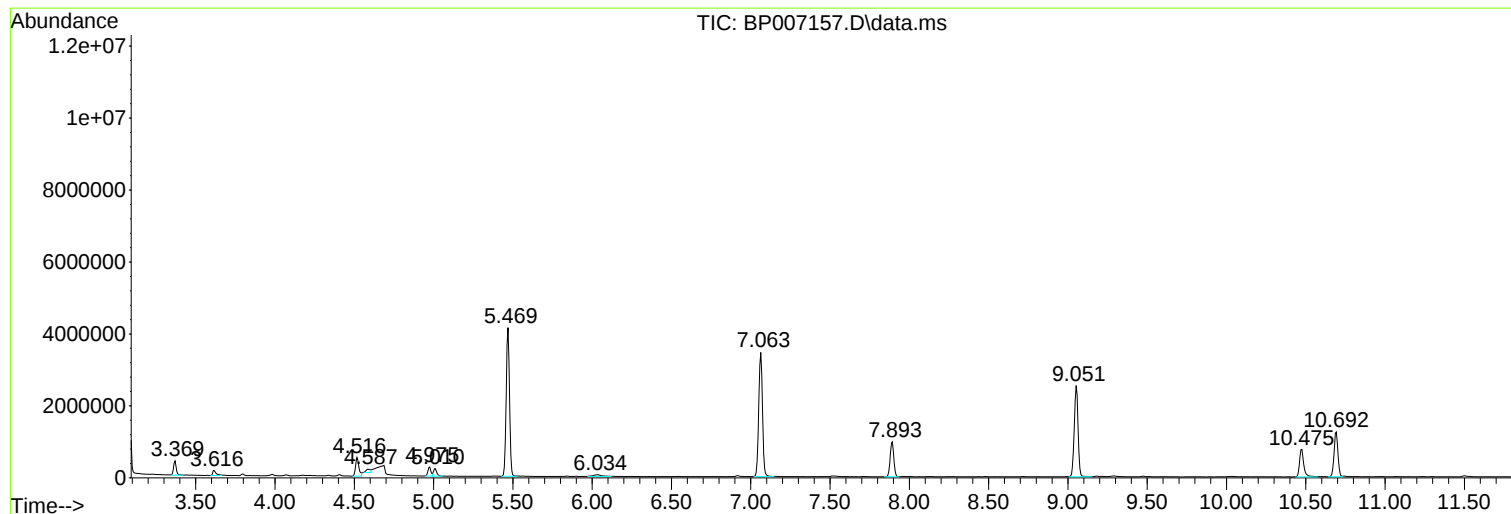

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP092421\  
Data File : BP007157.D  
Acq On : 24 Sep 2021 13:59  
Operator : CG/JU  
Sample : M3823-02  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DKM-ENV-IC

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP092121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP092421\  
Data File : BP007157.D  
Acq On : 24 Sep 2021 13:59  
Operator : CG/JU  
Sample : M3823-02  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DKM-ENV-IC

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP092121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|