
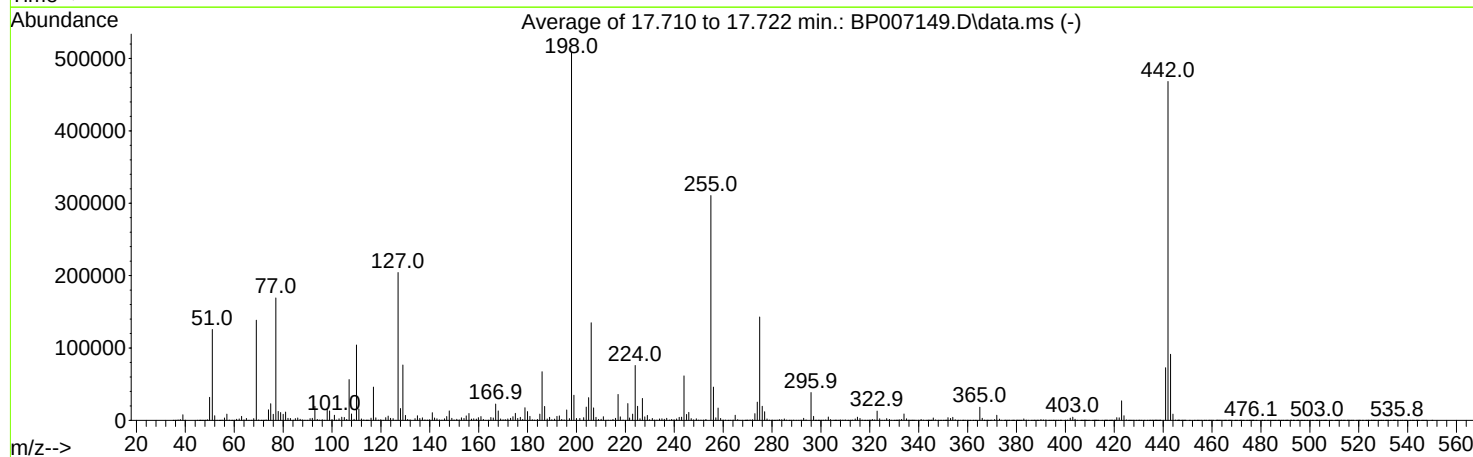


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092421\
 Data File : BP007149.D
 Acq On : 24 Sep 2021 09:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 23 11:17:25 2021

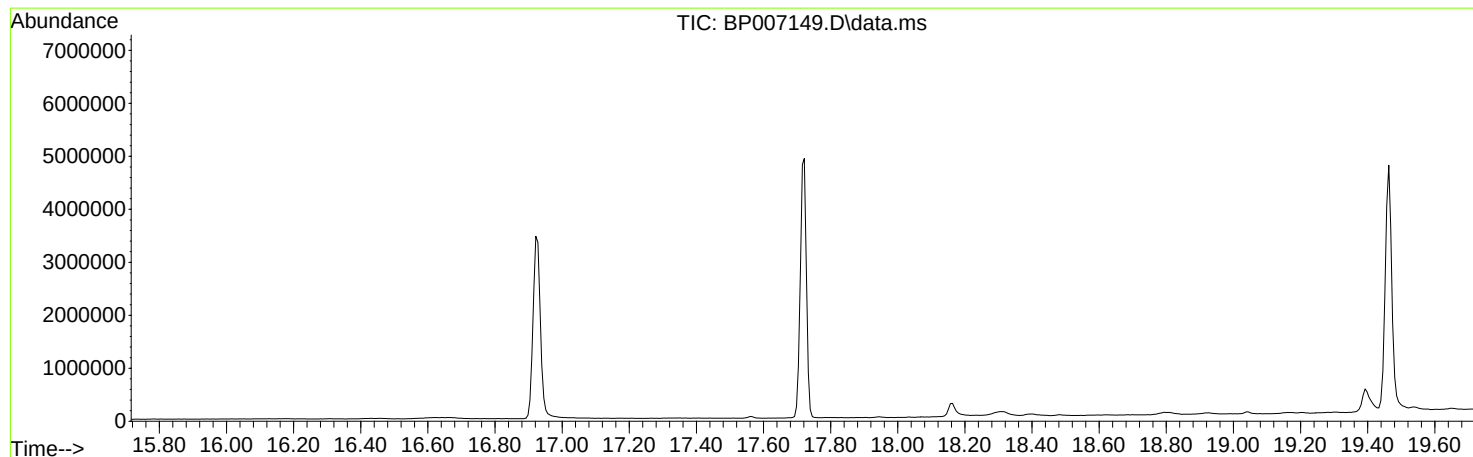




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.7	125639	PASS
68	69	0.00	2	1.8	2488	PASS
69	198	0.00	100	27.2	138380	PASS
70	69	0.00	2	0.5	758	PASS
127	198	10	80	40.2	204384	PASS
197	198	0.00	2	0.5	2558	PASS
198	198	100	100	100.0	508262	PASS
199	198	5	9	6.8	34754	PASS
275	198	10	60	28.1	142888	PASS
365	198	1	100	3.6	18239	PASS
441	198	0.01	100	14.3	72658	PASS
442	442	100	100	100.0	468224	PASS
443	442	15	24	19.5	91333	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092421\
 Data File : BP007149.D
 Acq On : 24 Sep 2021 09:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 24 11:03:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

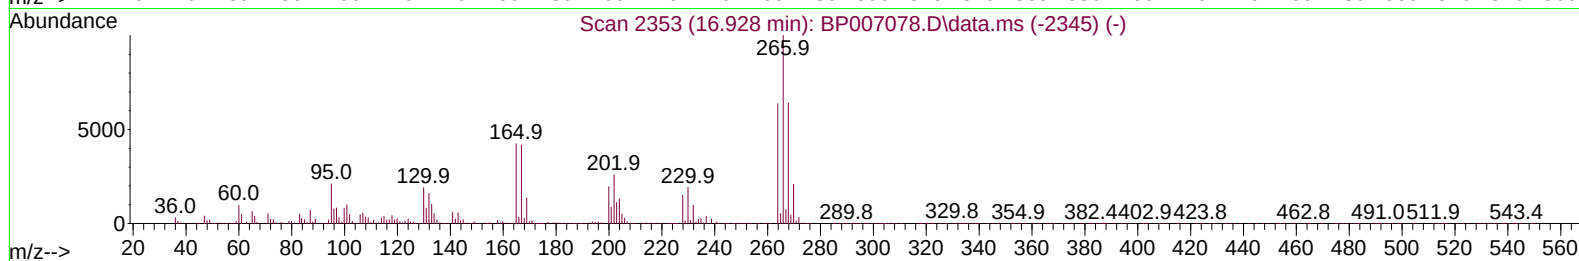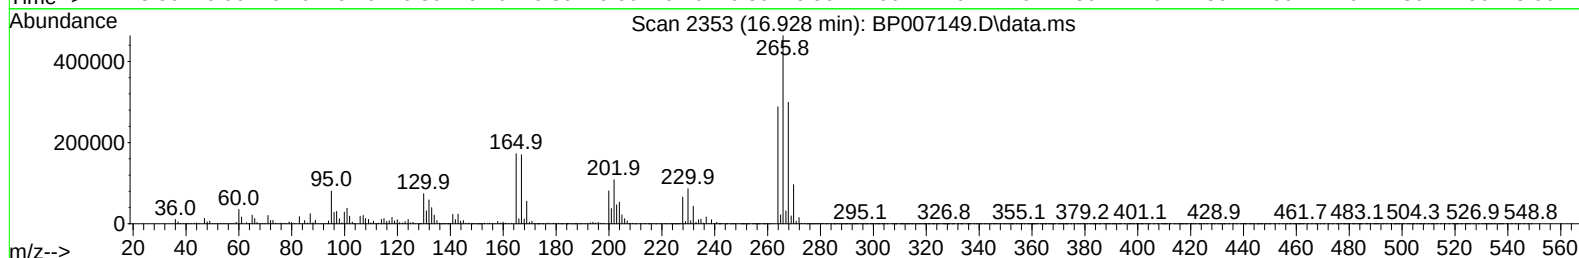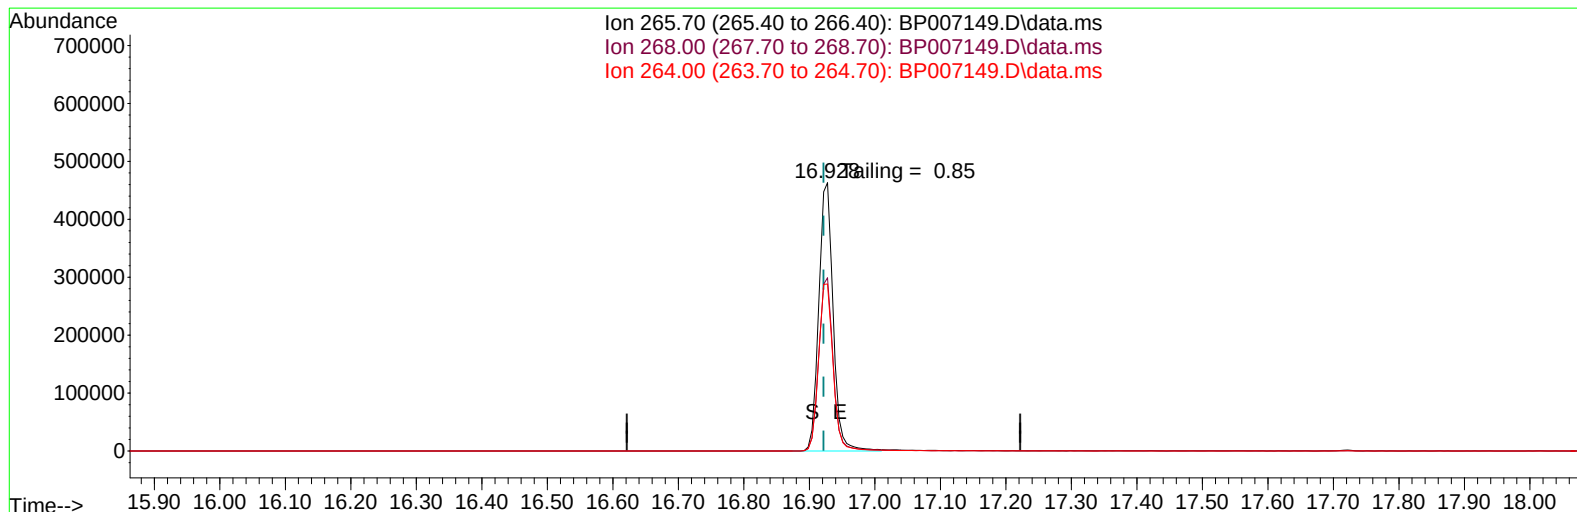

TIC: BP007149.D\data.ms

(70) Pentachlorophenol (C)

16.928min (+ 0.006) 658939.33 ng




response 708817

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.57
264.00	62.90	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092421\
 Data File : BP007149.D
 Acq On : 24 Sep 2021 09:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 24 11:03:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

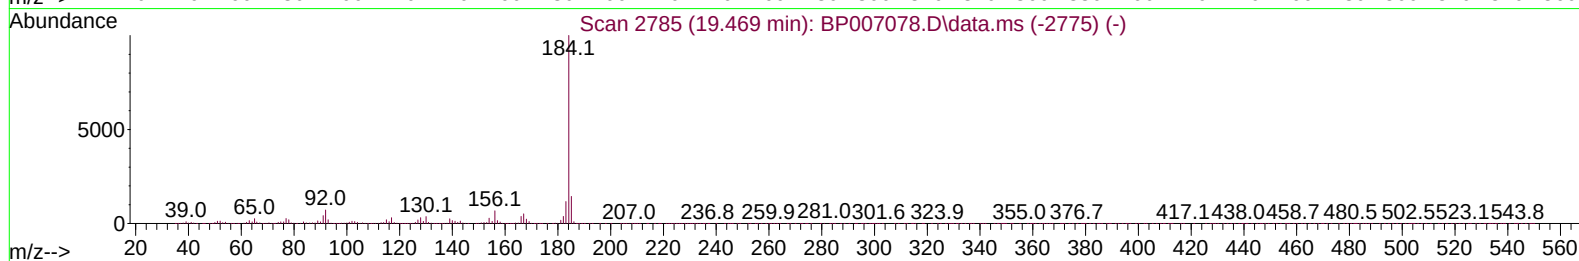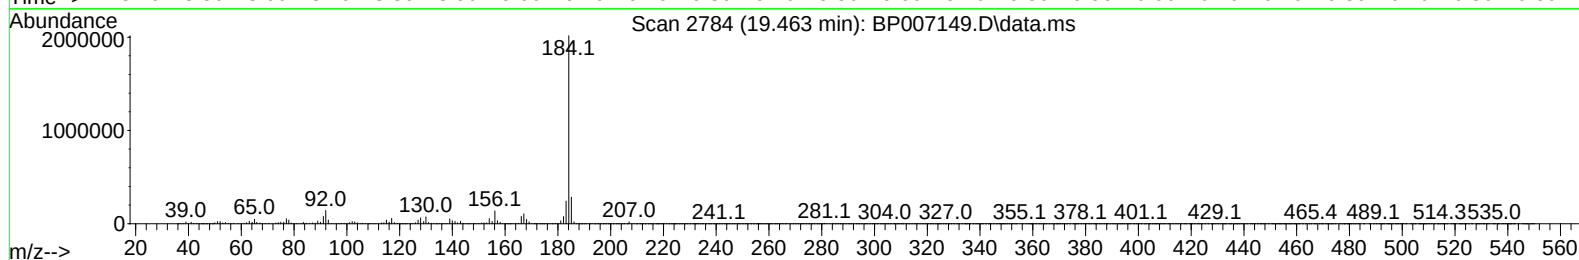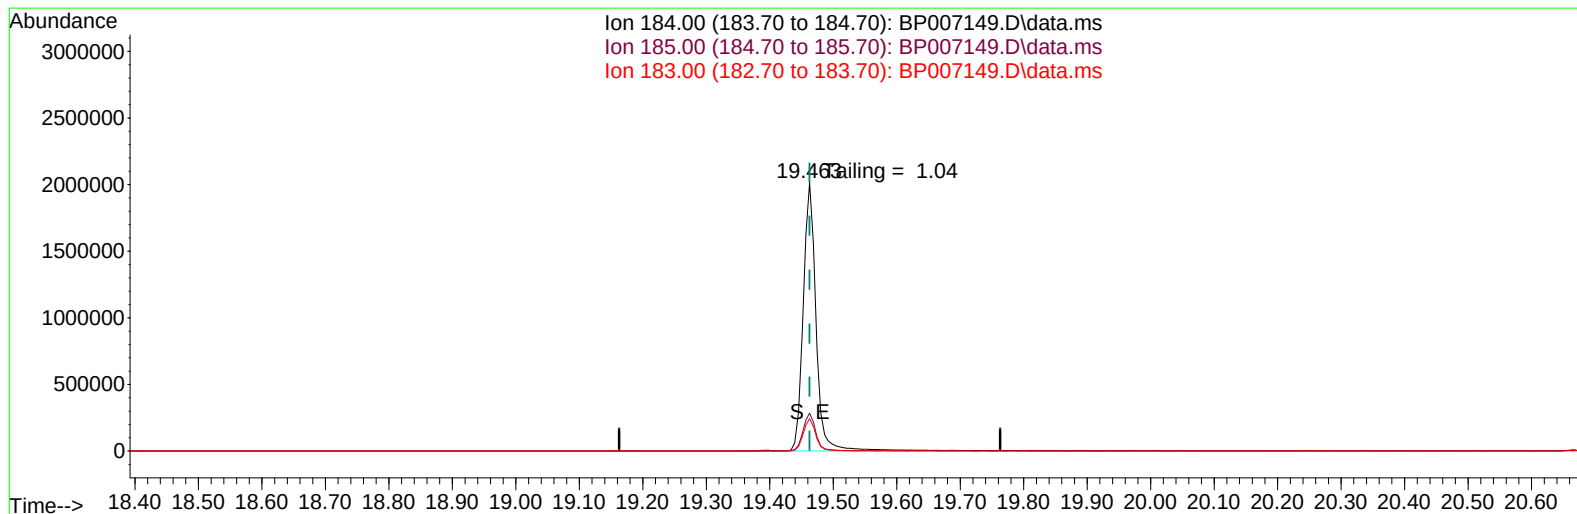

TIC: BP007149.D\data.ms

(77) Benzidine

19.463min (-0.000) 246204.84 ng

response 2852480

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.15
183.00	11.90	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/24/2021	BNA_P	BP007149.D
Compound Name	Response	Retention Time
DDT	1751993	20.66
DDD	14078	20.23
DDE	3710	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17788	1769781	1.01