
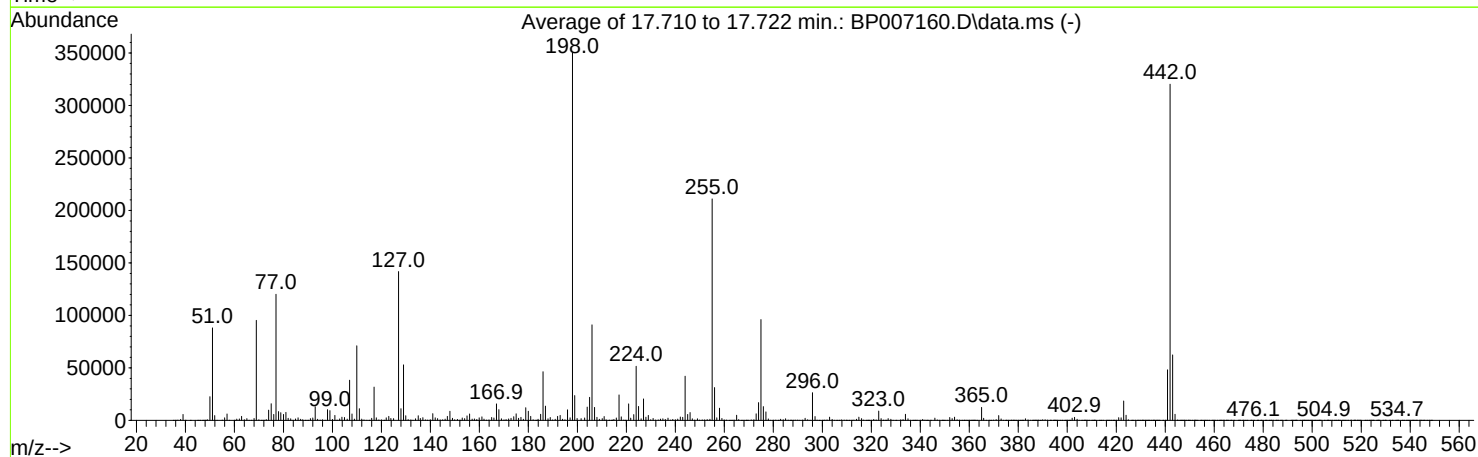


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092421\
 Data File : BP007160.D
 Acq On : 24 Sep 2021 15:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 23 11:17:25 2021

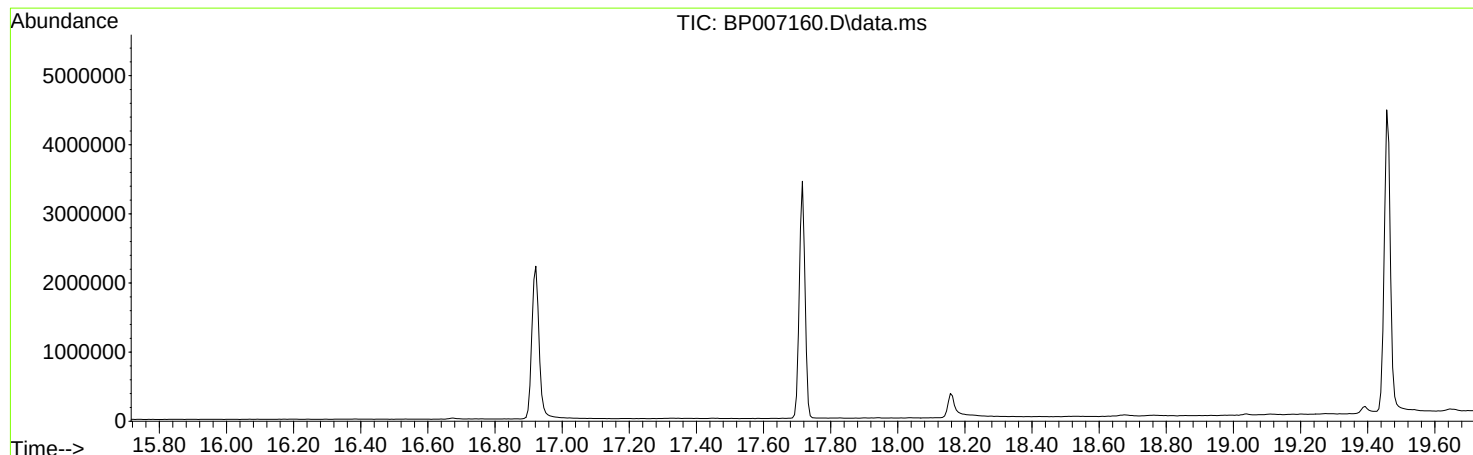




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	88061	PASS
68	69	0.00	2	1.9	1848	PASS
69	198	0.00	100	27.2	95252	PASS
70	69	0.00	2	0.6	560	PASS
127	198	10	80	40.5	141776	PASS
197	198	0.00	2	0.7	2384	PASS
198	198	100	100	100.0	350445	PASS
199	198	5	9	6.8	23689	PASS
275	198	10	60	27.4	96065	PASS
365	198	1	100	3.5	12398	PASS
441	198	0.01	100	13.8	48240	PASS
442	442	100	100	100.0	320320	PASS
443	442	15	24	19.4	62294	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092421\
Data File : BP007160.D
Acq On : 24 Sep 2021 15:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 24 17:15:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 23 11:17:25 2021
Response via : Initial Calibration

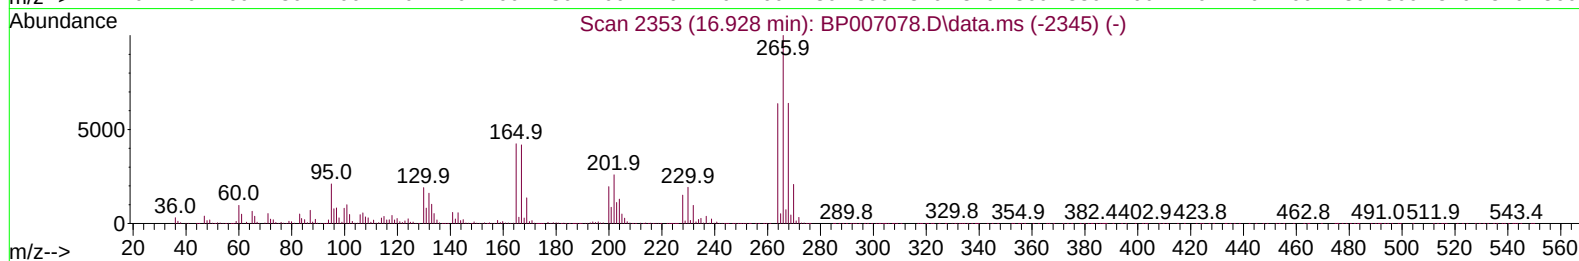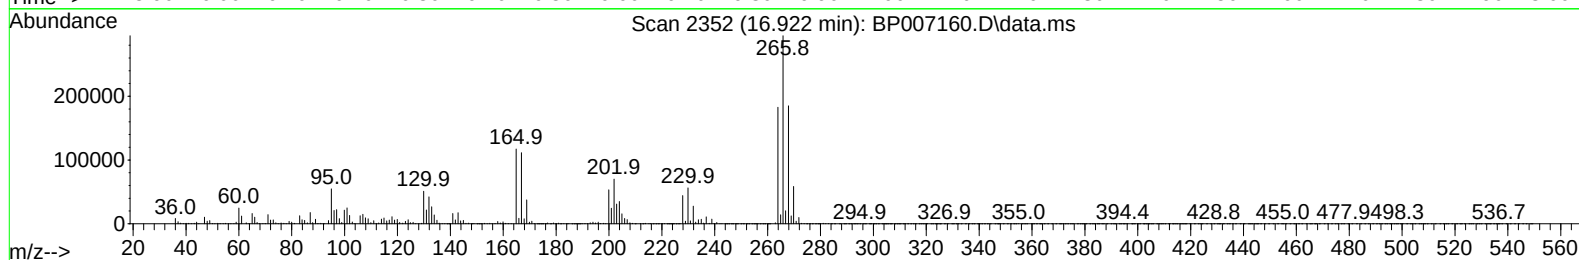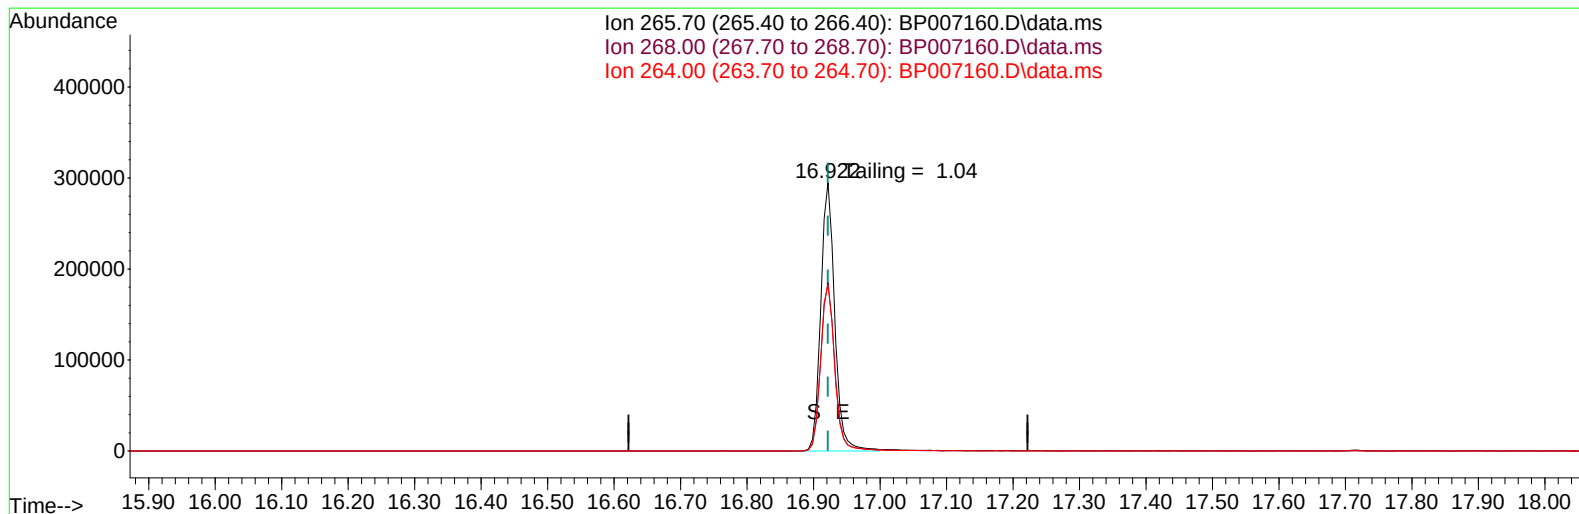

TIC: BP007160.D\data.ms

(70) Pentachlorophenol (C)

16.922min (-0.000) 1013718.02 ng




response 434655

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.74
264.00	62.90	61.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092421\
 Data File : BP007160.D
 Acq On : 24 Sep 2021 15:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 24 17:15:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

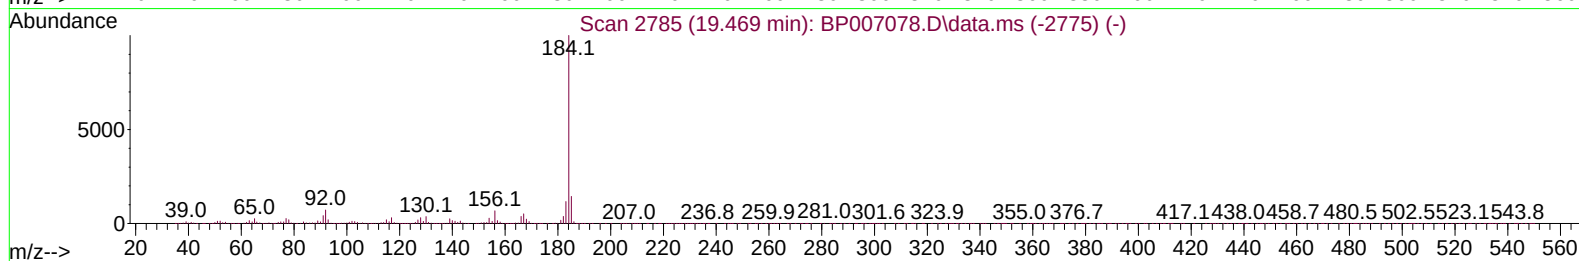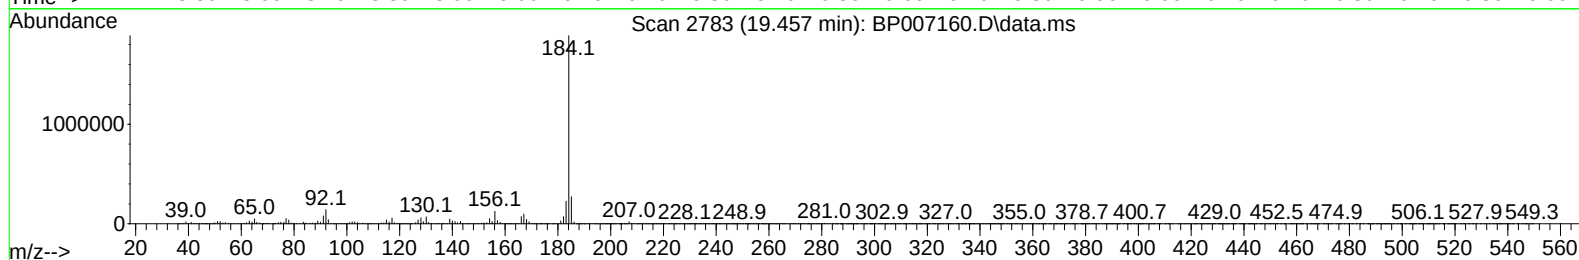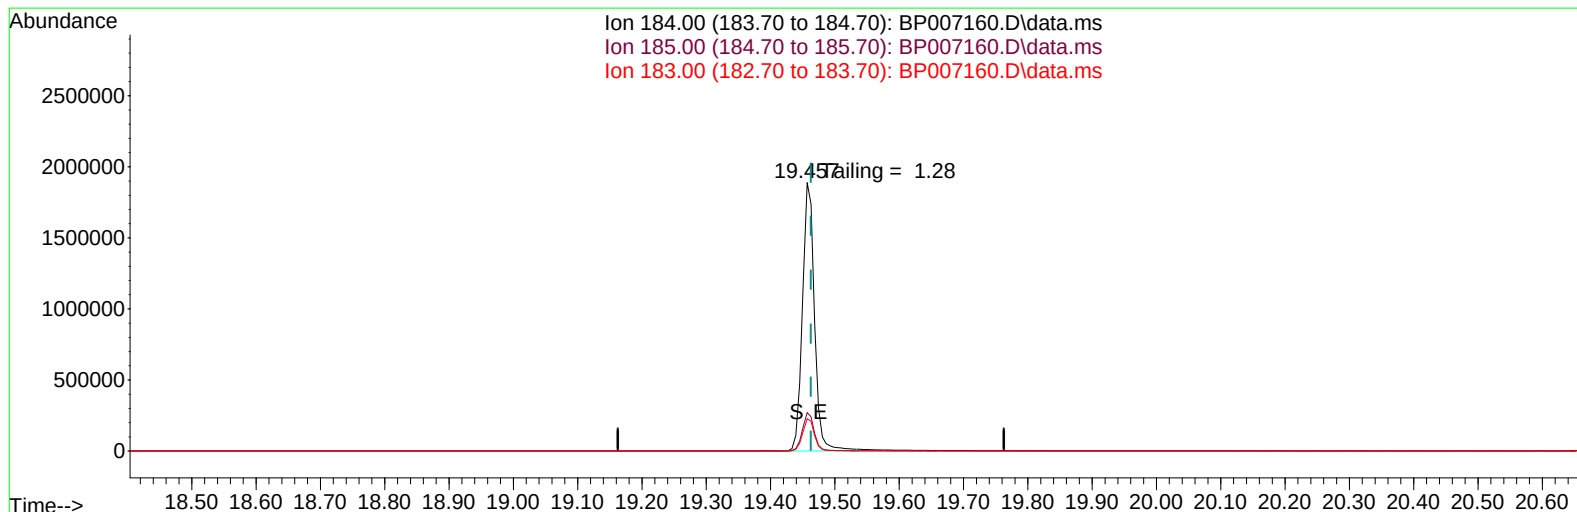

TIC: BP007160.D\data.ms

(77) Benzidine

19.457min (-0.006) 437786.90 ng

response 2502421

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.34
183.00	11.90	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/24/2021	BNA_P	BP007160.D
Compound Name	Response	Retention Time
DDT	1250203	20.66
DDD	8186	20.23
DDE	1539	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9725	1259928	0.77