

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092425\
 Data File : BP025851.D
 Acq On : 24 Sep 2025 18:50
 Operator : CG/JU
 Sample : Q3167-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RT4784

Quant Time: Sep 24 19:11:50 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 16:45:04 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.743	152	139362	20.000	ng	-0.02
21) Naphthalene-d8	10.519	136	552940	20.000	ng	0.00
39) Acenaphthene-d10	14.372	164	387955	20.000	ng	0.00
64) Phenanthrene-d10	17.183	188	911264	20.000	ng	0.00
76) Chrysene-d12	21.619	240	1026394	20.000	ng	-0.02
86) Perylene-d12	24.989	264	1059657	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.384	112	1064778	123.281	ng	0.00
7) Phenol-d6	6.949	99	1217121	106.020	ng	0.00
23) Nitrobenzene-d5	8.890	82	918376	73.264	ng	-0.01
42) 2,4,6-Tribromophenol	15.895	330	724355	149.692	ng	-0.01
45) 2-Fluorobiphenyl	12.978	172	2111610	72.473	ng	-0.01
79) Terphenyl-d14	19.901	244	4622075	81.012	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092425\
Data File : BP025851.D
Acq On : 24 Sep 2025 18:50
Operator : CG/JU
Sample : Q3167-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RT4784

Quant Time: Sep 24 19:11:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration




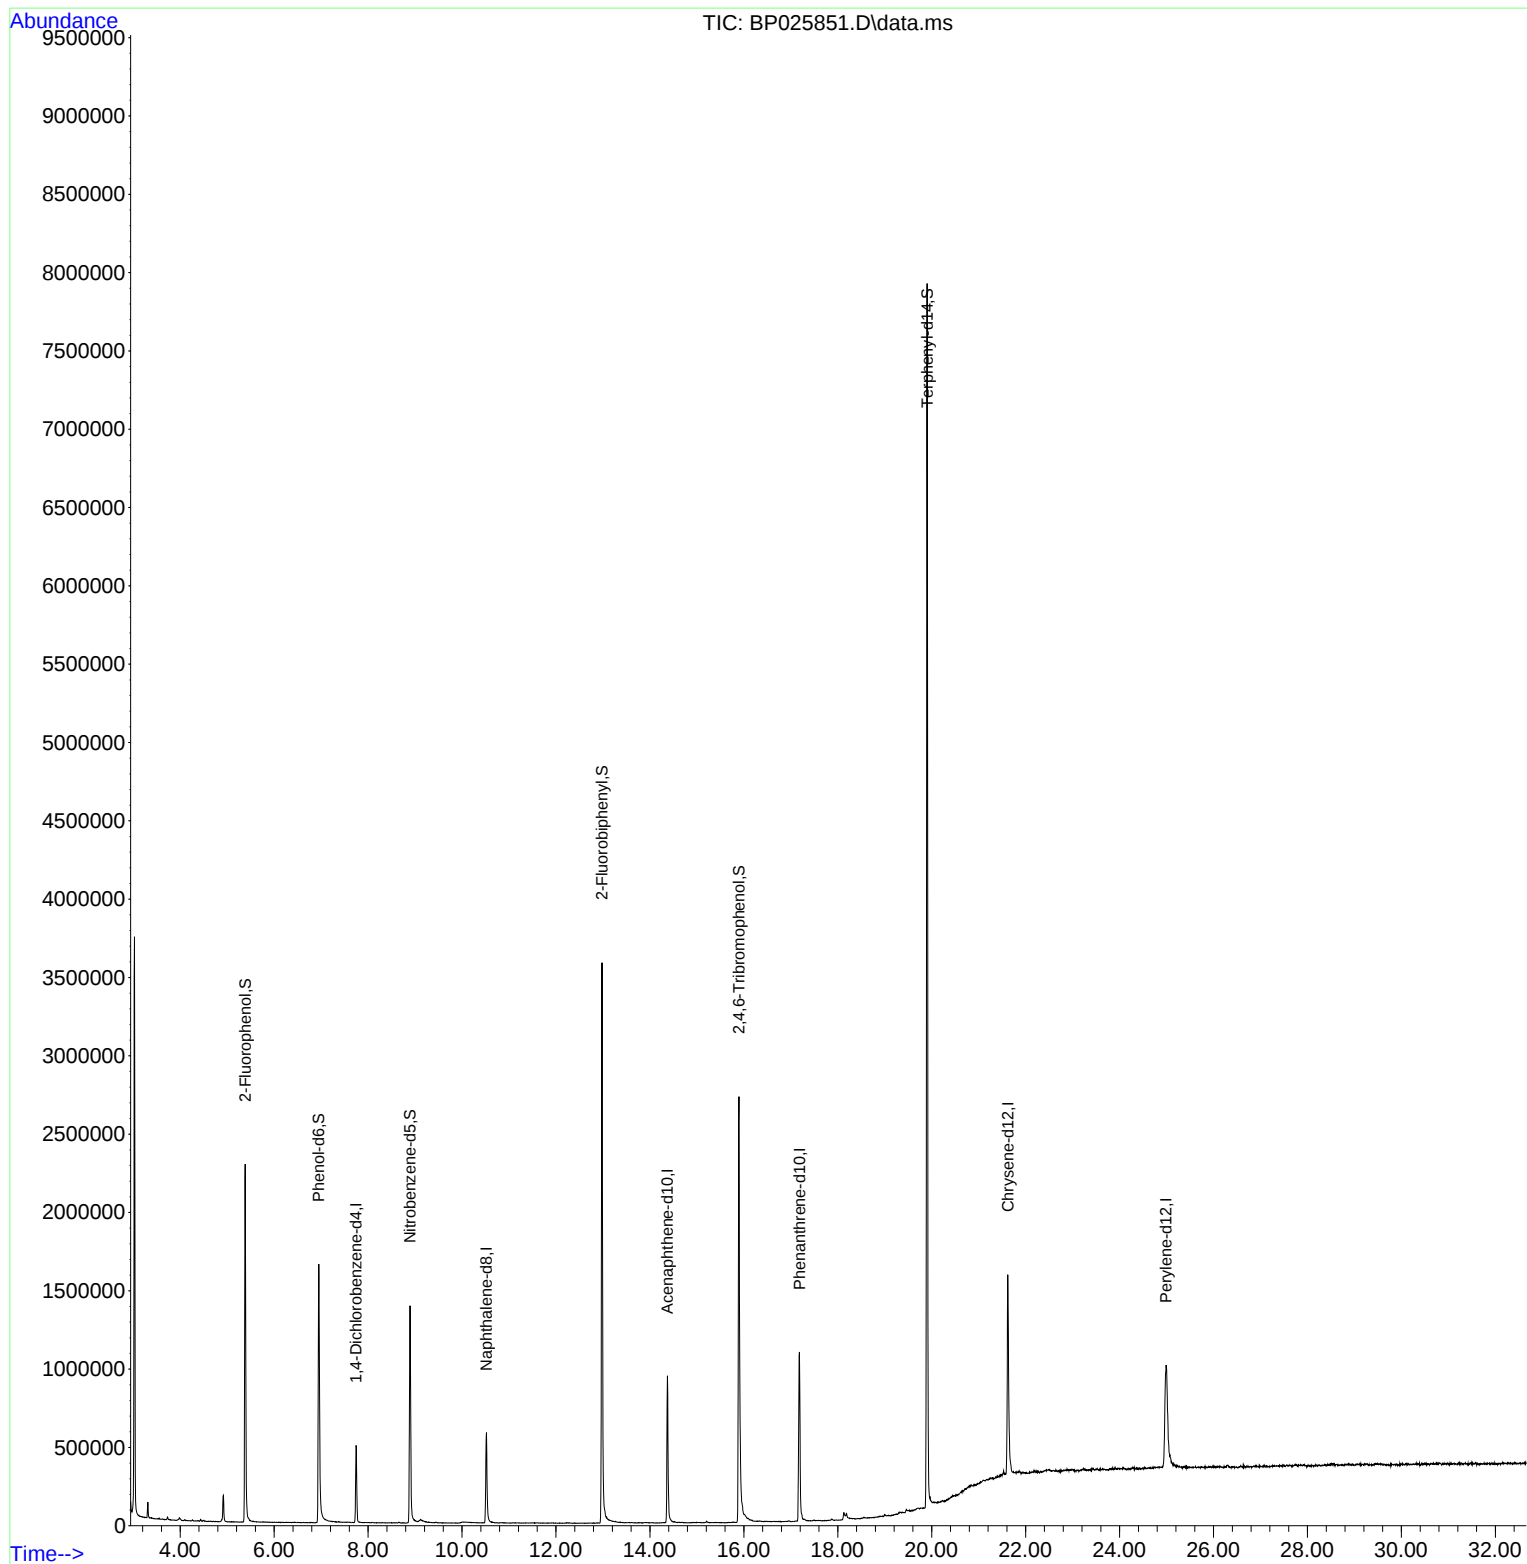




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.743 min Scan# 81
Delta R.T. -0.017 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50




Instrument :
BNA_P
ClientSampleId :
RT4784


Tgt Ion:152 Resp: 139362
Ion Ratio Lower Upper
152 100
150 153.3 124.3 186.5
115 61.4 50.3 75.5

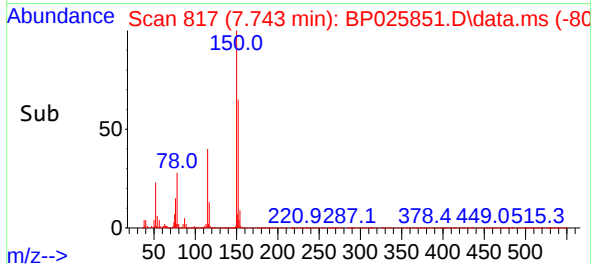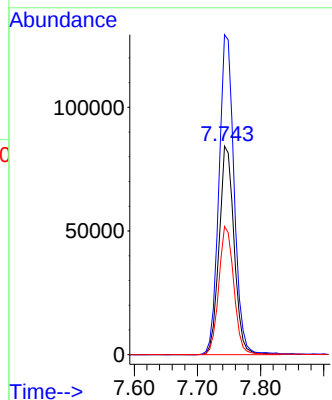

#5
2-Fluorophenol
Concen: 123.281 ng
RT: 5.384 min Scan# 416
Delta R.T. -0.000 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50

Tgt Ion:112 Resp: 1064778
Ion Ratio Lower Upper
112 100
64 60.3 50.2 75.4
63 31.2 26.7 40.1


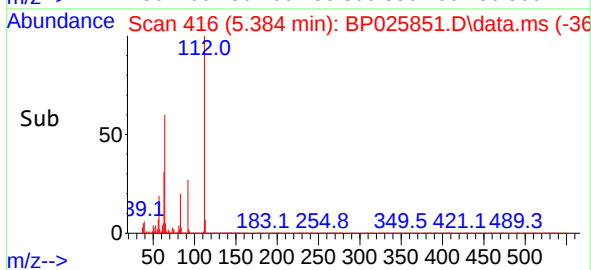
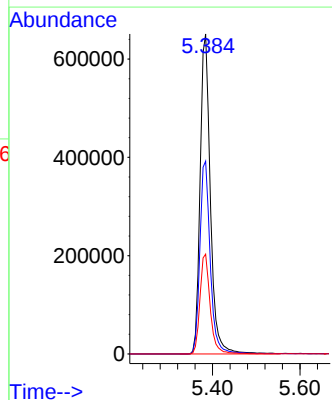
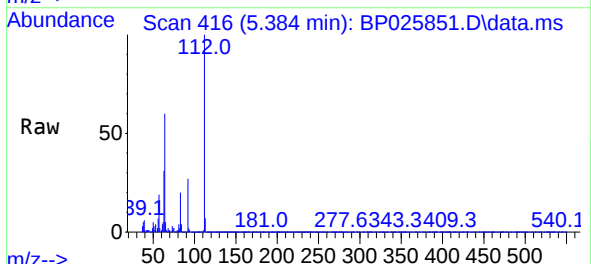


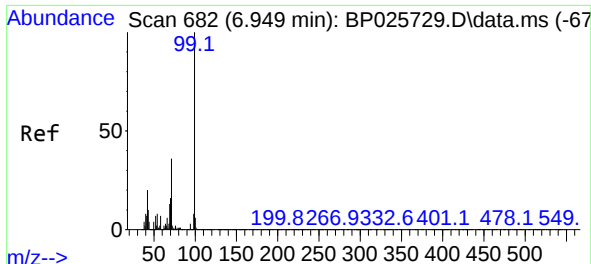

#7
Phenol-d6
Concen: 106.020 ng
RT: 6.949 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50




Instrument :
BNA_P
ClientSampleId :
RT4784


Tgt Ion: 99 Resp: 1217121
Ion Ratio Lower Upper
99 100
42 17.9 15.6 23.4
71 35.0 28.6 43.0

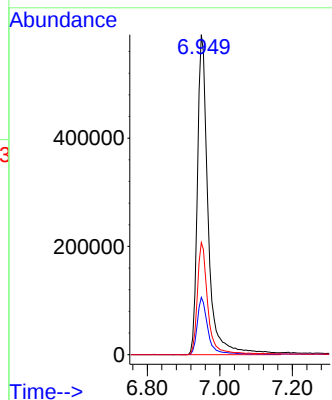

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.519 min Scan# 1289
Delta R.T. -0.006 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50

Tgt Ion: 136 Resp: 552940
Ion Ratio Lower Upper
136 100
137 11.2 8.7 13.1
54 8.7 7.5 11.3
68 6.0 5.0 7.6


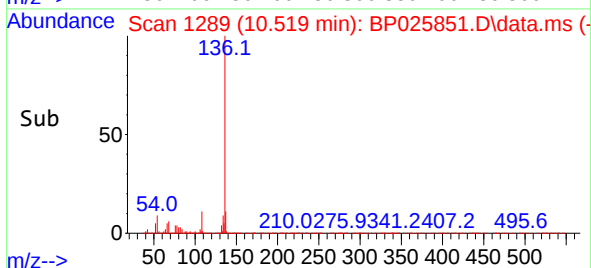
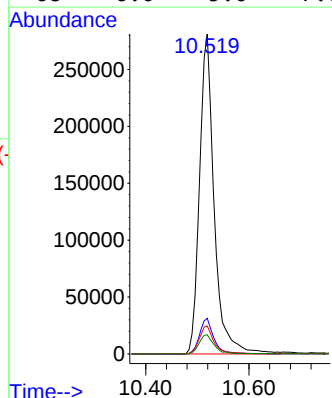
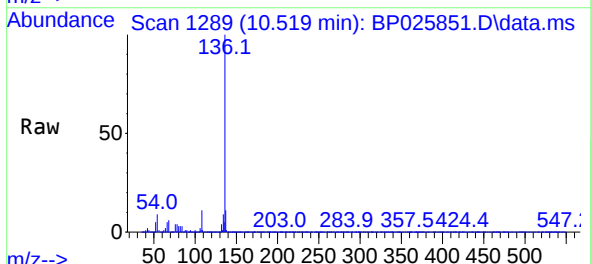


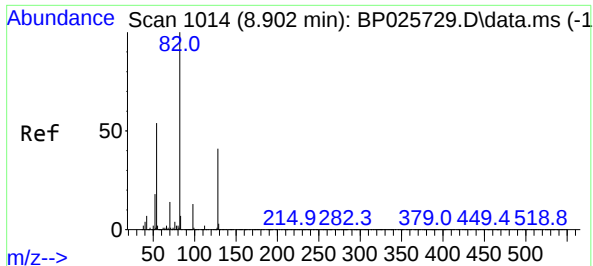

#23
Nitrobenzene-d5
Concen: 73.264 ng
RT: 8.890 min Scan# 1014
Delta R.T. -0.012 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50




Instrument :
BNA_P
ClientSampleId :
RT4784


Tgt Ion: 82 Resp: 918376
Ion Ratio Lower Upper
82 100
128 41.9 32.9 49.3
54 52.8 43.4 65.2

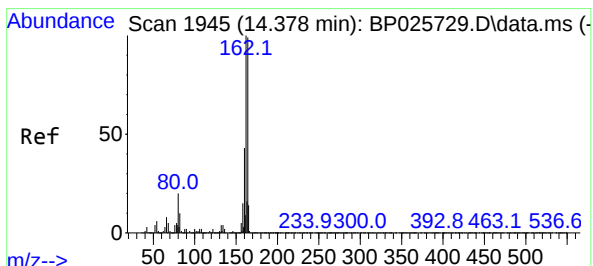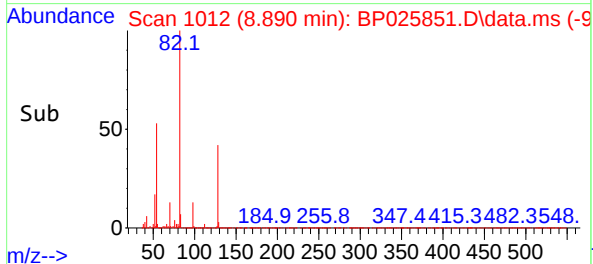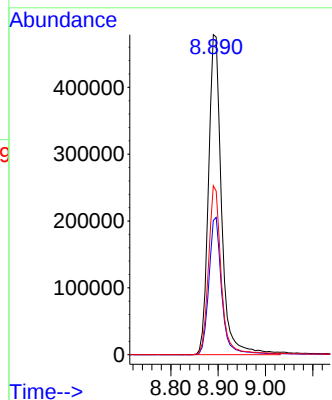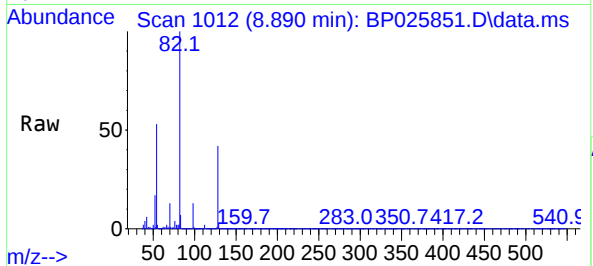

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.372 min Scan# 1944
Delta R.T. -0.006 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50

Tgt Ion: 164 Resp: 387955
Ion Ratio Lower Upper
164 100
162 97.7 80.6 120.8
160 42.9 35.0 52.6


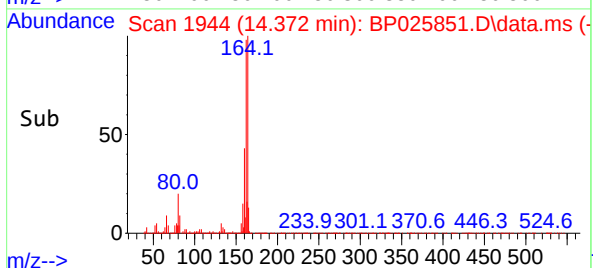
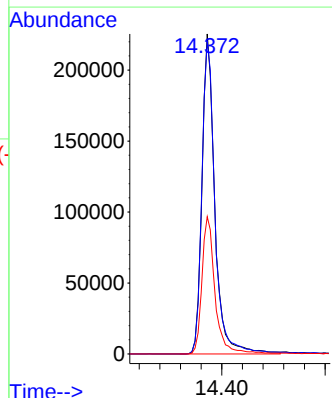
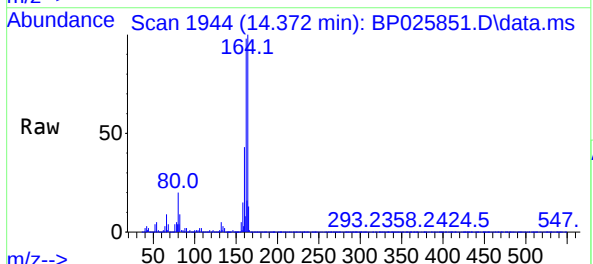




#42
2,4,6-Tribromophenol
Concen: 149.692 ng
RT: 15.895 min Scan# 21
Delta R.T. -0.012 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50




Instrument :
BNA_P
ClientSampleId :
RT4784


Tgt Ion:330 Resp: 724355
Ion Ratio Lower Upper
330 100
332 96.6 76.9 115.3
141 34.2 31.0 46.4

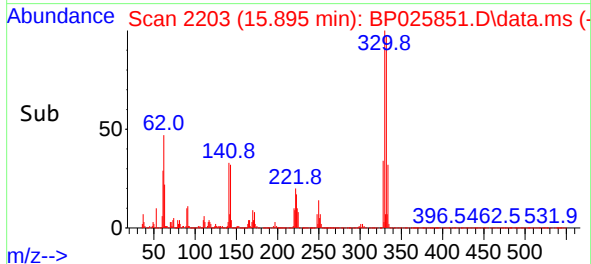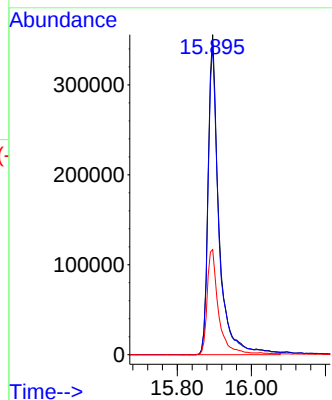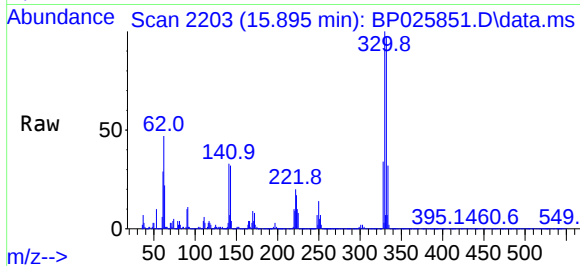

#45
2-Fluorobiphenyl
Concen: 72.473 ng
RT: 12.978 min Scan# 1707
Delta R.T. -0.012 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50

Tgt Ion:172 Resp: 2111610
Ion Ratio Lower Upper
172 100
171 35.2 27.8 41.6
170 23.3 18.6 27.8


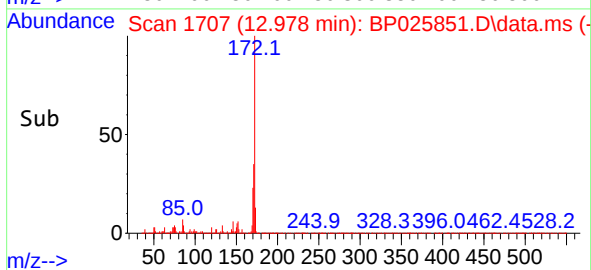
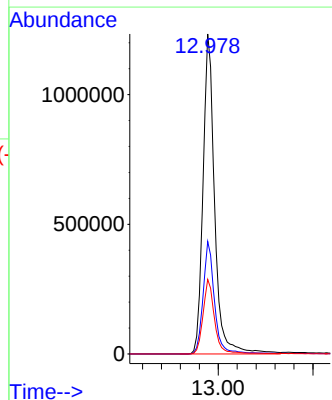
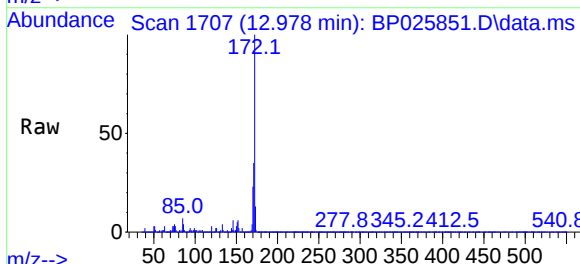




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.183 min Scan# 2422
Delta R.T. -0.000 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50




Instrument :
BNA_P
ClientSampleId :
RT4784


Tgt Ion:188 Resp: 911264
Ion Ratio Lower Upper
188 100
94 8.9 7.4 11.0
80 10.2 7.7 11.5

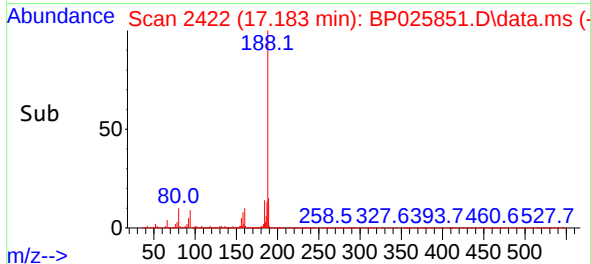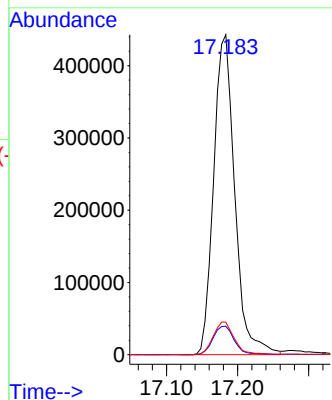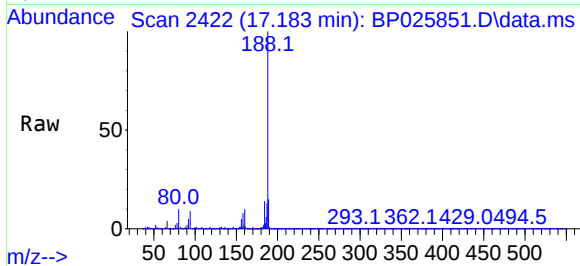

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.619 min Scan# 3176
Delta R.T. -0.024 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50

Tgt Ion:240 Resp: 1026394
Ion Ratio Lower Upper
240 100
120 10.4 8.0 12.0
236 25.8 20.7 31.1


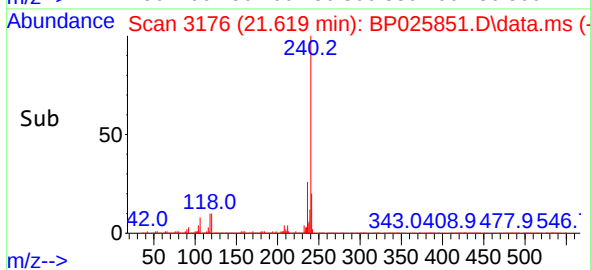
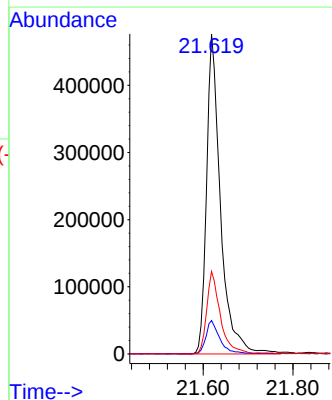
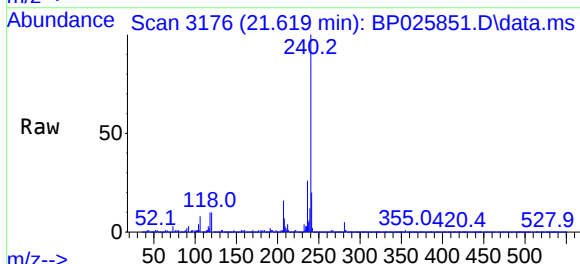




#79
Terphenyl-d14
Concen: 81.012 ng
RT: 19.901 min Scan# 21
Delta R.T. -0.012 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50

Instrument :
BNA_P
ClientSampleId :
RT4784

Tgt Ion:244 Resp: 4622075
Ion Ratio Lower Upper
244 100
212 7.4 5.9 8.9
122 9.5 7.1 10.7

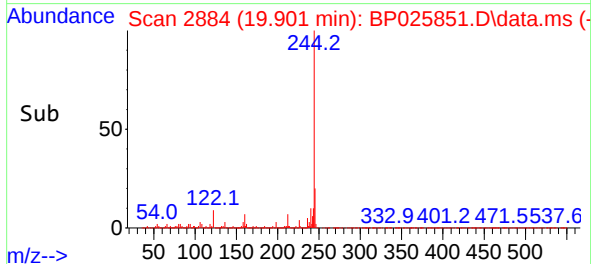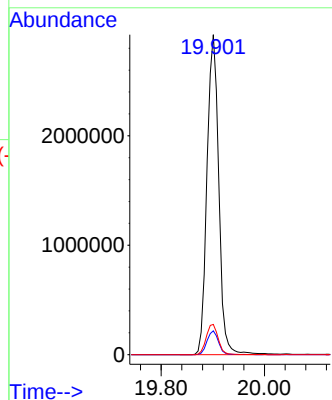

#86
Perylene-d12
Concen: 20.000 ng
RT: 24.989 min Scan# 3749
Delta R.T. -0.012 min
Lab File: BP025851.D
Acq: 24 Sep 2025 18:50

Tgt Ion:264 Resp: 1059657
Ion Ratio Lower Upper
264 100
260 23.5 18.3 27.5
265 21.7 17.3 25.9

