

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092425\
 Data File : BP025841.D
 Acq On : 24 Sep 2025 11:39
 Operator : CG/JU
 Sample : PB169765BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB169765BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.014	9	13	18	rVB	106969	118524	1.05%	0.244%
2	5.384	409	416	439	rBV	3347246	5062620	45.06%	10.412%
3	6.955	675	683	706	rBV	2697878	5079035	45.20%	10.446%
4	7.749	808	818	827	rBV	564105	932786	8.30%	1.918%
5	8.896	1004	1013	1031	rBV	1760026	3292899	29.31%	6.772%
6	10.513	1281	1288	1308	rBV	626667	1231158	10.96%	2.532%
7	12.972	1699	1706	1716	rBV	4118256	7122995	63.39%	14.650%
8	14.372	1936	1944	1959	rBV	958669	1649393	14.68%	3.392%
9	15.889	2194	2202	2235	rBV	3106713	6296894	56.04%	12.951%
10	17.184	2414	2422	2435	rBV	1169851	2040925	18.16%	4.197%
11	18.125	2577	2582	2591	rBV5	45031	115624	1.03%	0.238%
12	19.595	2827	2832	2837	rBV	116253	155727	1.39%	0.320%
13	19.901	2878	2884	2901	rBV	8046049	11235935	100.00%	23.108%
14	20.648	3006	3011	3016	rBV	183939	346645	3.09%	0.713%
15	20.689	3016	3018	3023	rVB3	130859	203823	1.81%	0.419%
16	21.630	3172	3178	3193	rVB2	892385	2064600	18.37%	4.246%
17	24.995	3743	3750	3768	rVB	509153	1673108	14.89%	3.441%




Sum of corrected areas: 48622691

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092425\
Data File : BP025841.D
Acq On : 24 Sep 2025 11:39
Operator : CG/JU
Sample : PB169765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169765BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

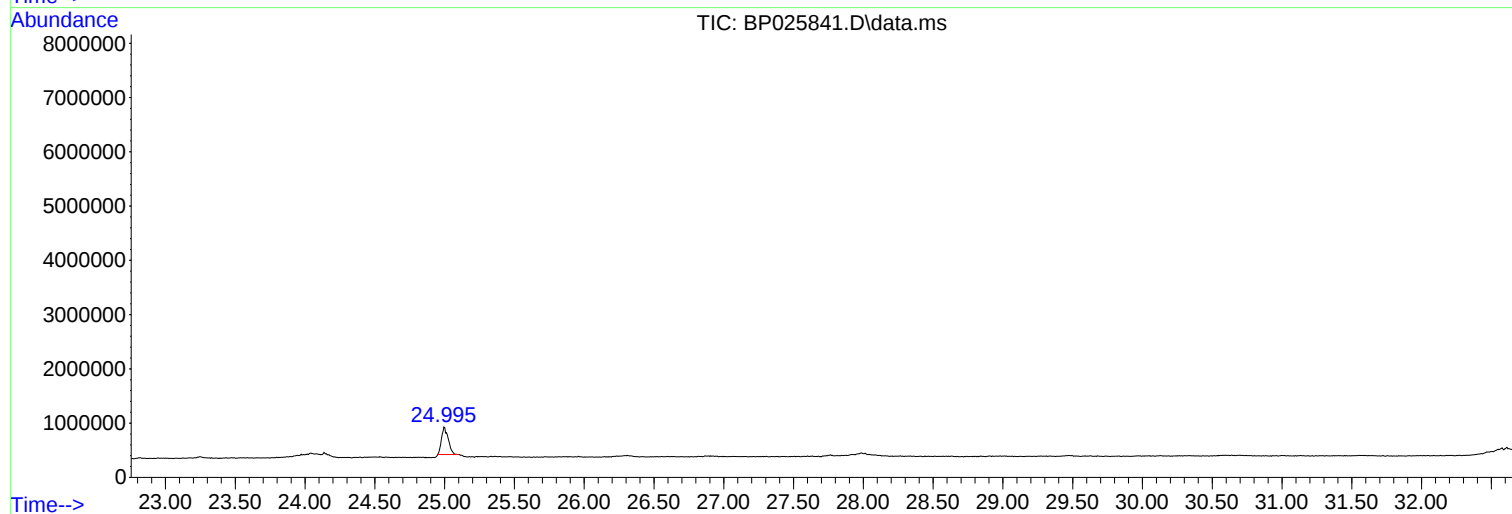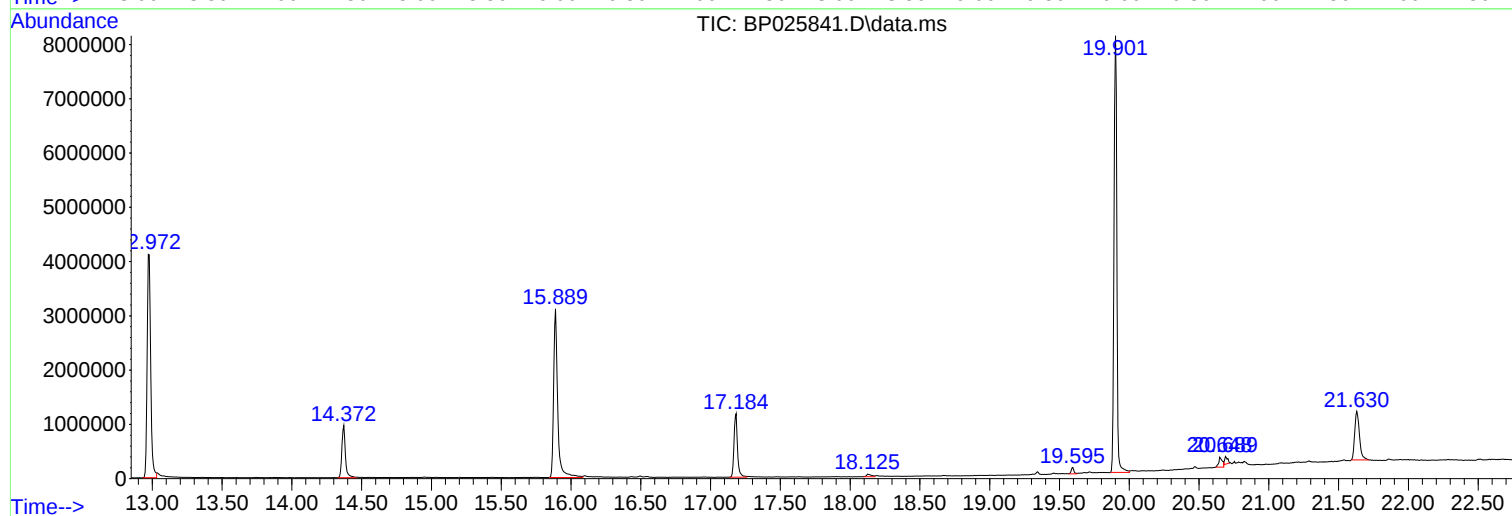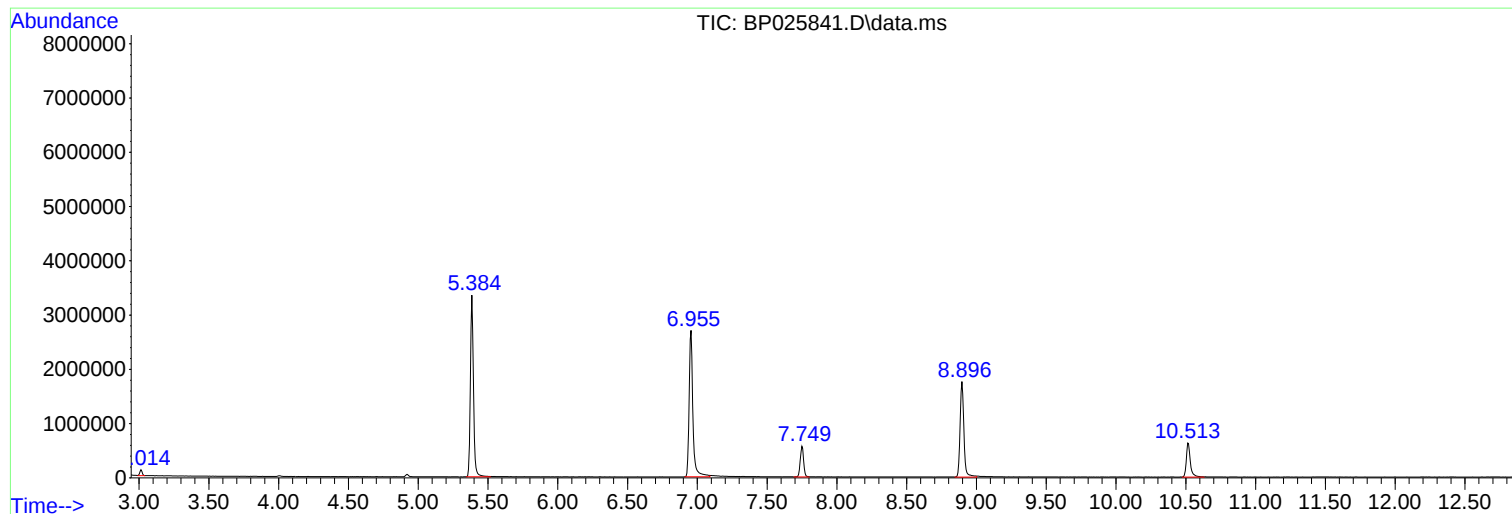

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092425\
Data File : BP025841.D
Acq On : 24 Sep 2025 11:39
Operator : CG/JU
Sample : PB169765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169765BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Bromo dodecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.648	3.36 ng	346645	Chrysene-d12	21.630

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Bromo dodecane	248	C12H25Br	013187-99-0	93
2		Octacosane, 1-iodo-	520	C28H57I	1000406-32-2	87
3		4-Methylheneicosane	310	C22H46	025117-29-7	87
4		Heptadecane, 9-octyl-	352	C25H52	007225-64-1	87
5		Hexacosane, 1-iodo-	492	C26H53I	1000406-32-1	87

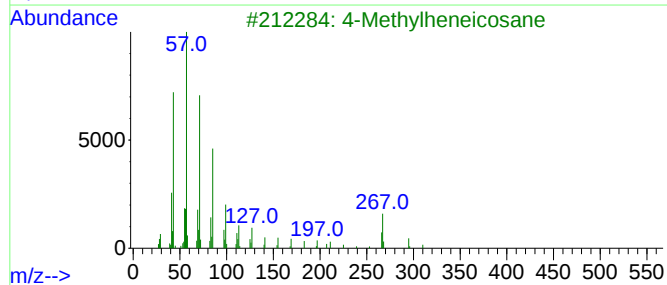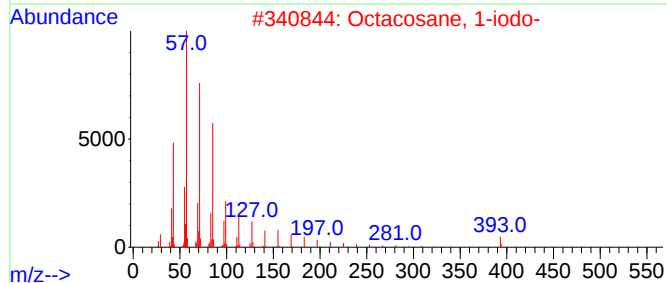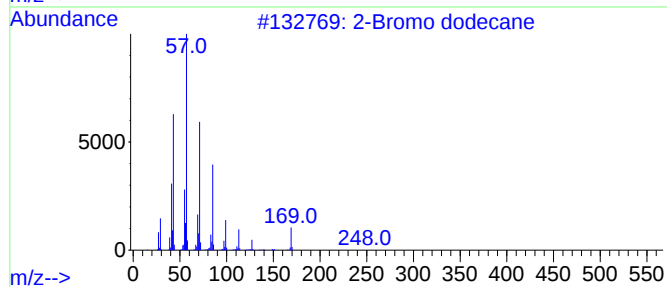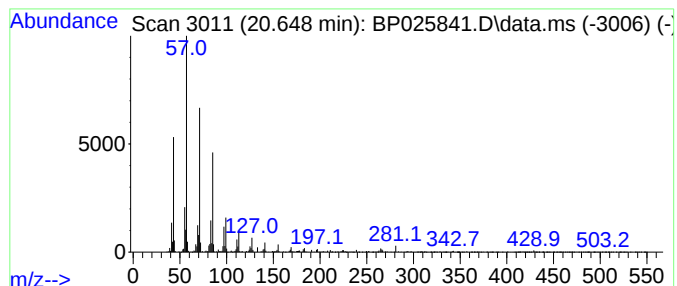

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092425\
Data File : BP025841.D
Acq On : 24 Sep 2025 11:39
Operator : CG/JU
Sample : PB169765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169765BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Bromo dodecane	20.648	3.4	ng	346645	5	21.630	2064600	20.0