


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092425\
Data File : BP025839.D
Acq On : 24 Sep 2025 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

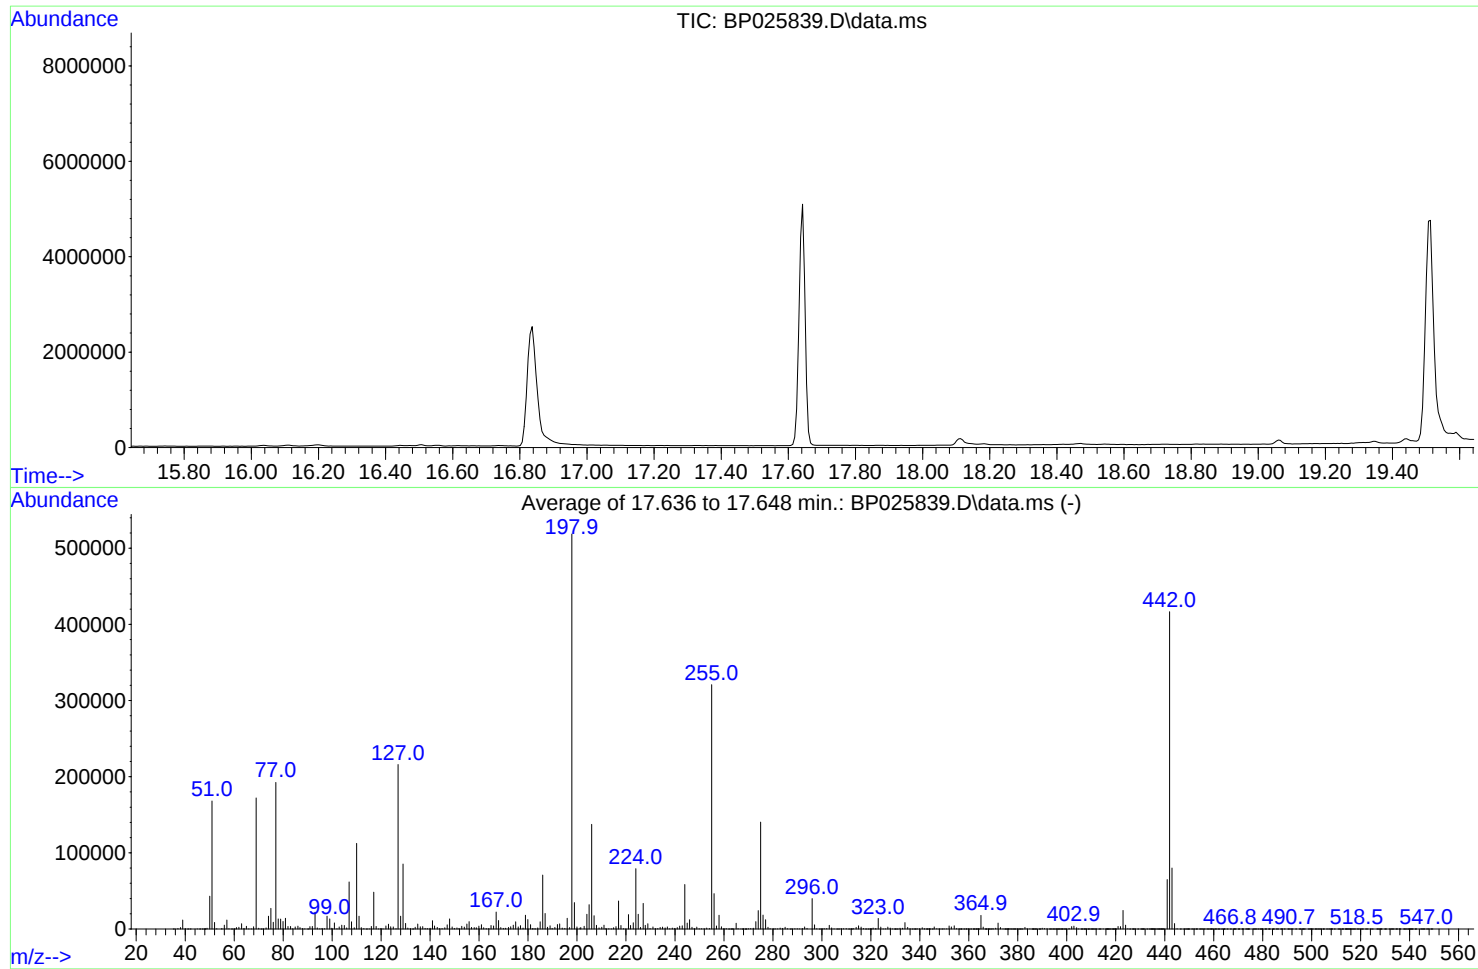

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	2940	PASS
69	69	100	100	100.0	172032	PASS
70	69	0.00	2	0.6	974	PASS
197	198	0.00	2	0.4	1892	PASS
198	198	100	100	100.0	518464	PASS
199	198	5	9	6.7	34777	PASS
365	198	1	100	3.5	17953	PASS
441	443	0.01	150	80.9	64858	PASS
442	442	100	100	100.0	416597	PASS
443	442	15	24	19.2	80122	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/24/2025	BNA_P	<u>BP025839.D</u>
Compound Name	Response	Retention Time
DDT	2051649	20.795
DDD	30839	20.336
DDE	8545	19.813
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
39384	2091033	1.88

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092425\
Data File : BP025839.D
Acq On : 24 Sep 2025 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 24 10:42:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

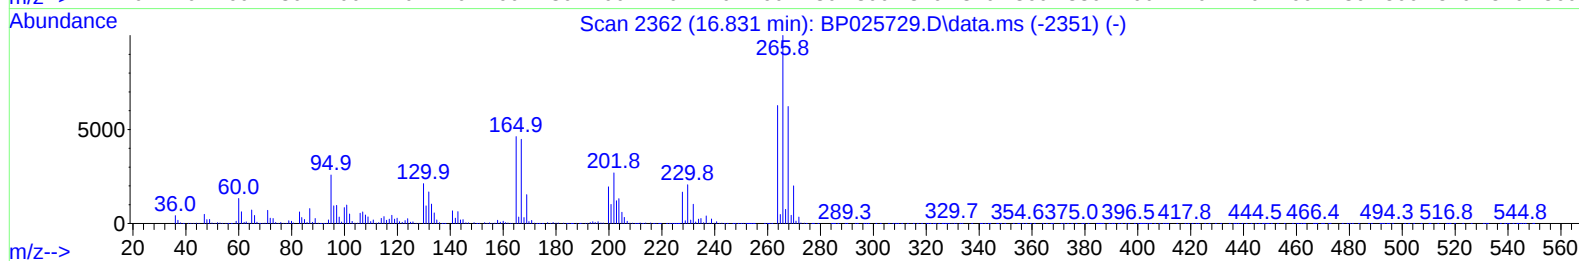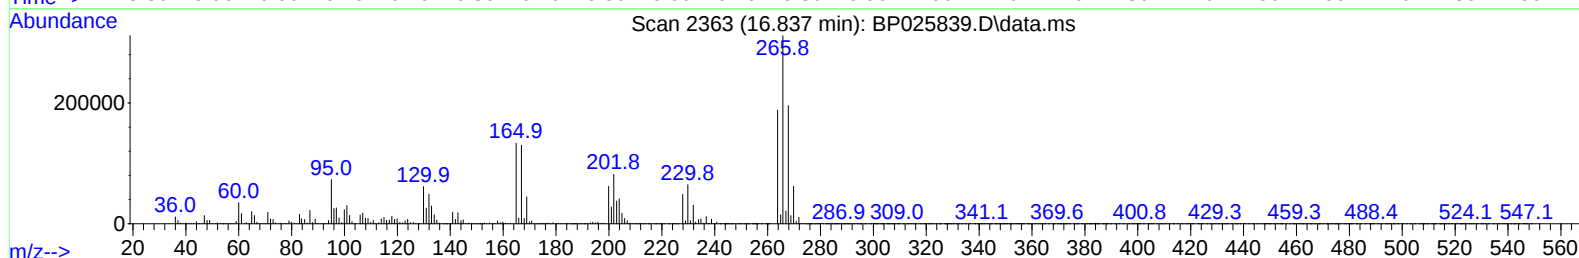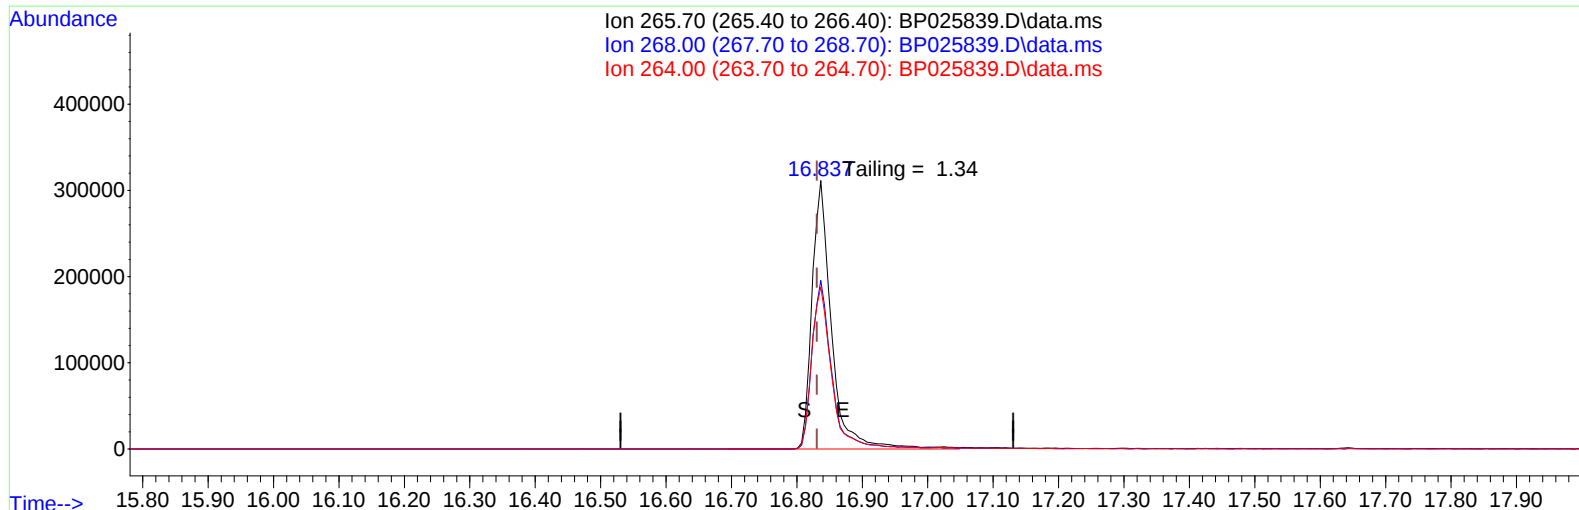

TIC: BP025839.D\data.ms

(70) Pentachlorophenol (C)

16.837min (+ 0.006) 822322.01 ng




response 638308

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.80
264.00	62.70	60.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092425\
Data File : BP025839.D
Acq On : 24 Sep 2025 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 24 10:42:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

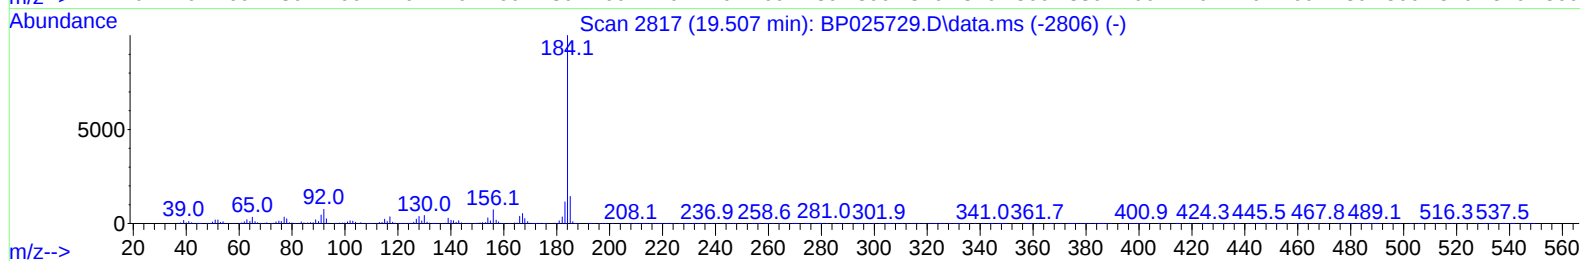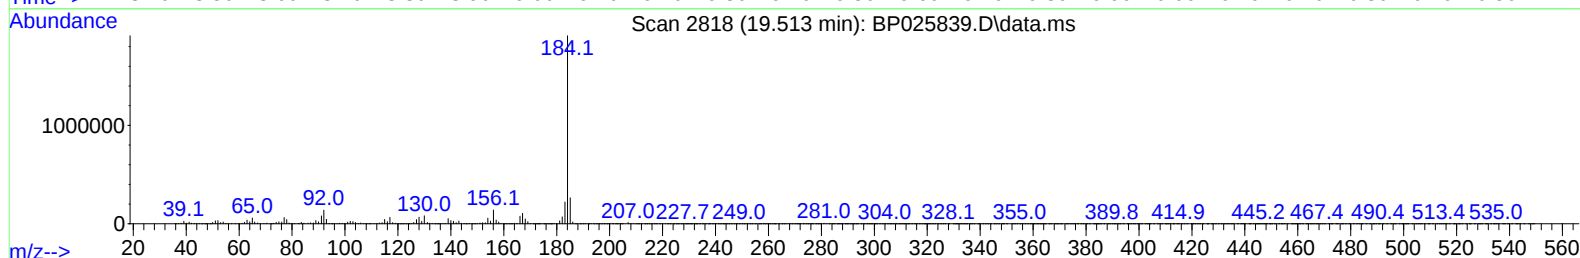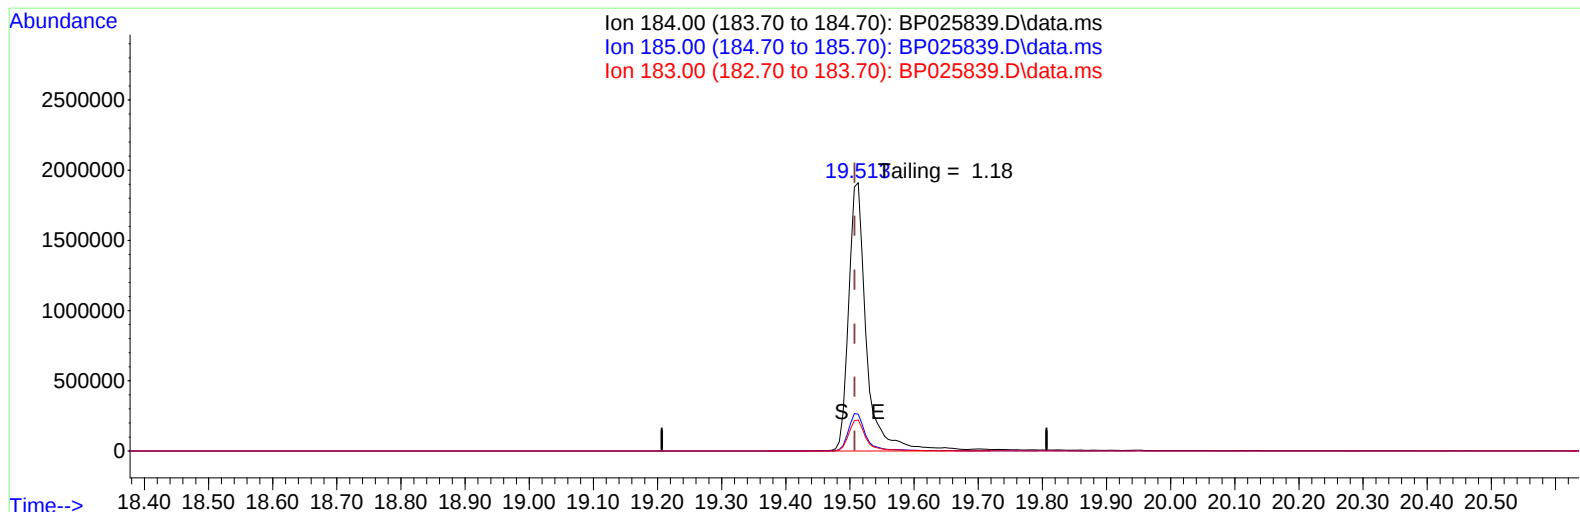

TIC: BP025839.D\data.ms

(77) Benzidine

19.513min (+ 0.006) 55388.79 ng

response 3650489

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.76
183.00	11.50	11.58
0.00	0.00	0.00