
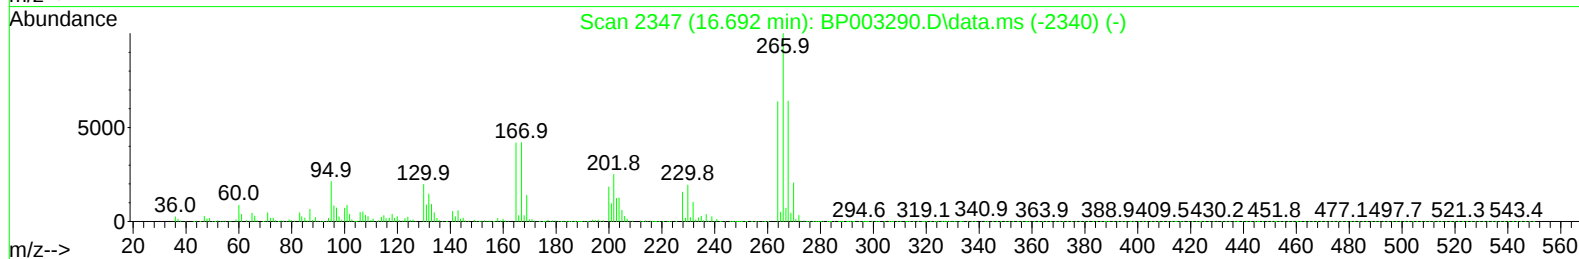
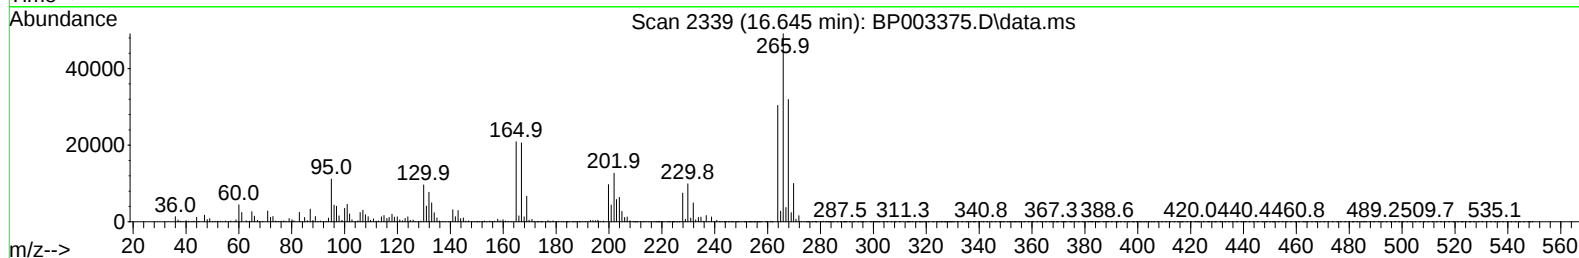


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092520\
Data File : BP003375.D
Acq On : 25 Sep 2020 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 06:39:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 22 12:48:08 2020
Response via : Initial Calibration

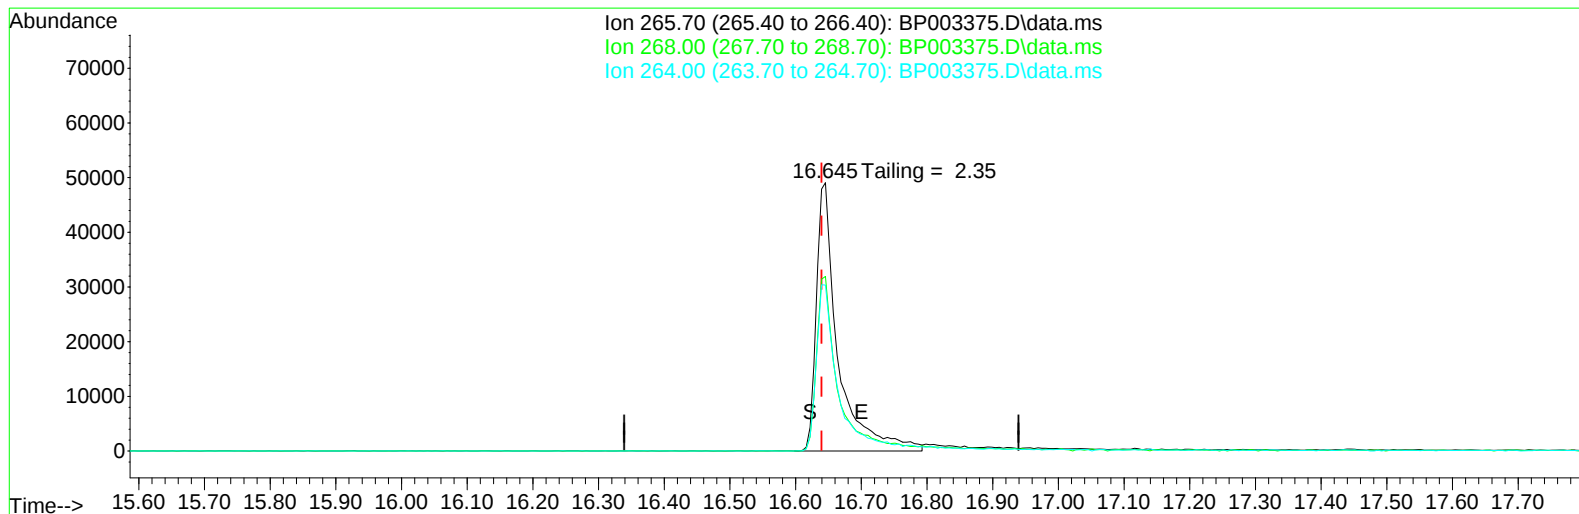

TIC: BP003375.D\data.ms

(70) Pentachlorophenol (C)




16.645min (+ 0.006) 668566.88 ng

response 112549

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.06
264.00	63.30	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092520\
 Data File : BP003375.D
 Acq On : 25 Sep 2020 11:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 06:39:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 22 12:48:08 2020
 Response via : Initial Calibration

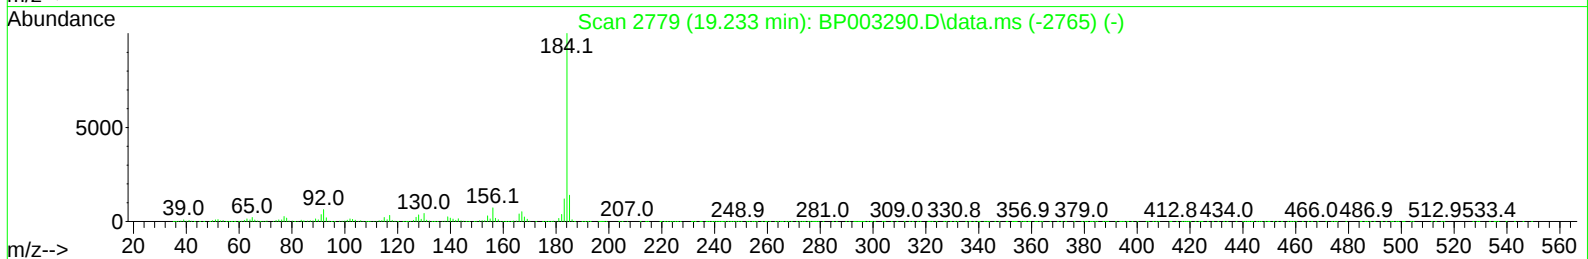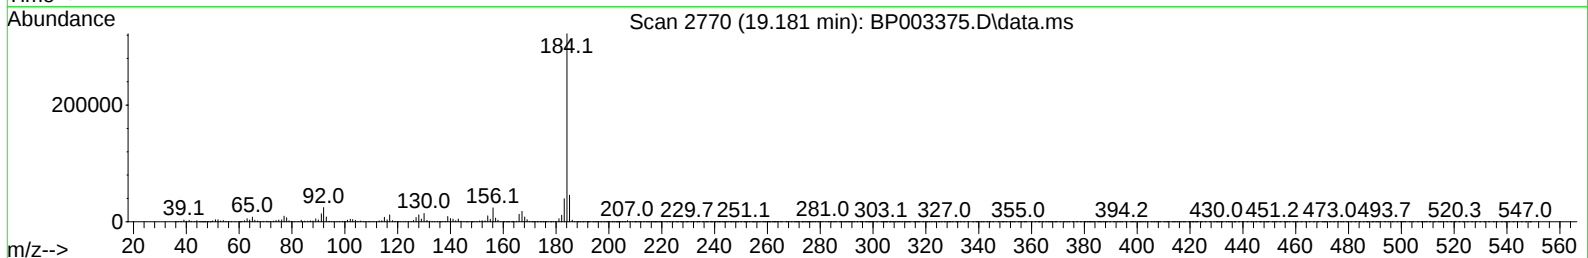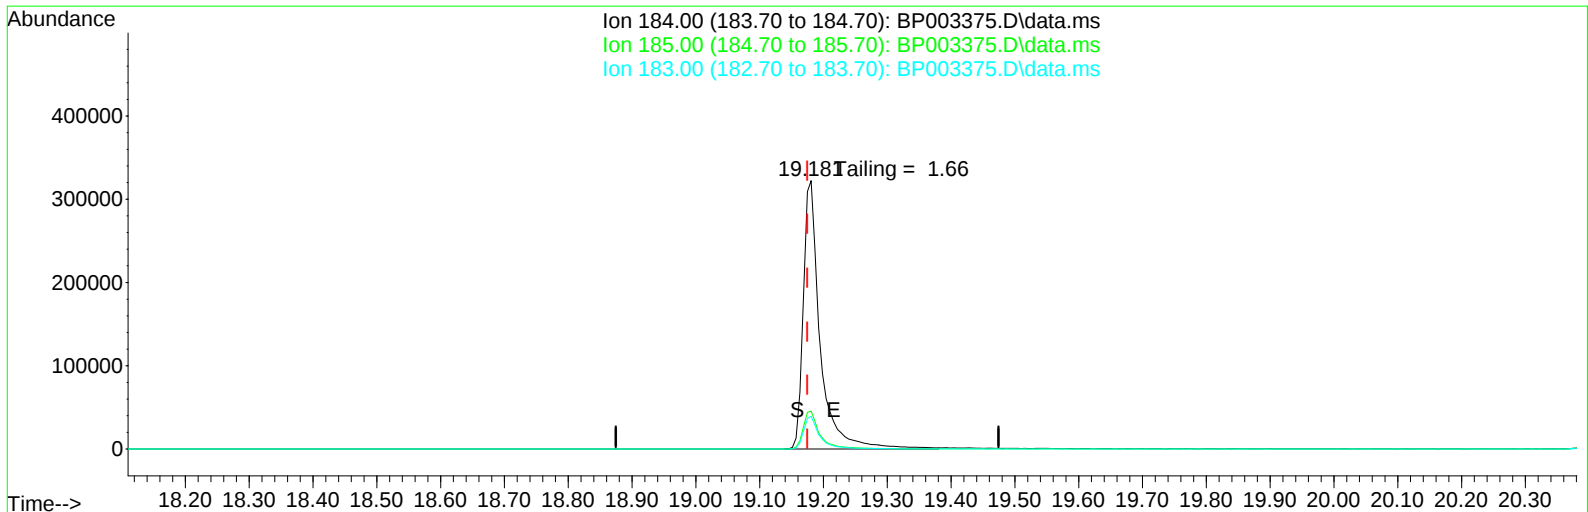

TIC: BP003375.D\data.ms

(77) Benzidine**19.181min (+ 0.006) 738065.57 ng****response 595050**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.13
183.00	12.00	12.25
0.00	0.00	0.00