
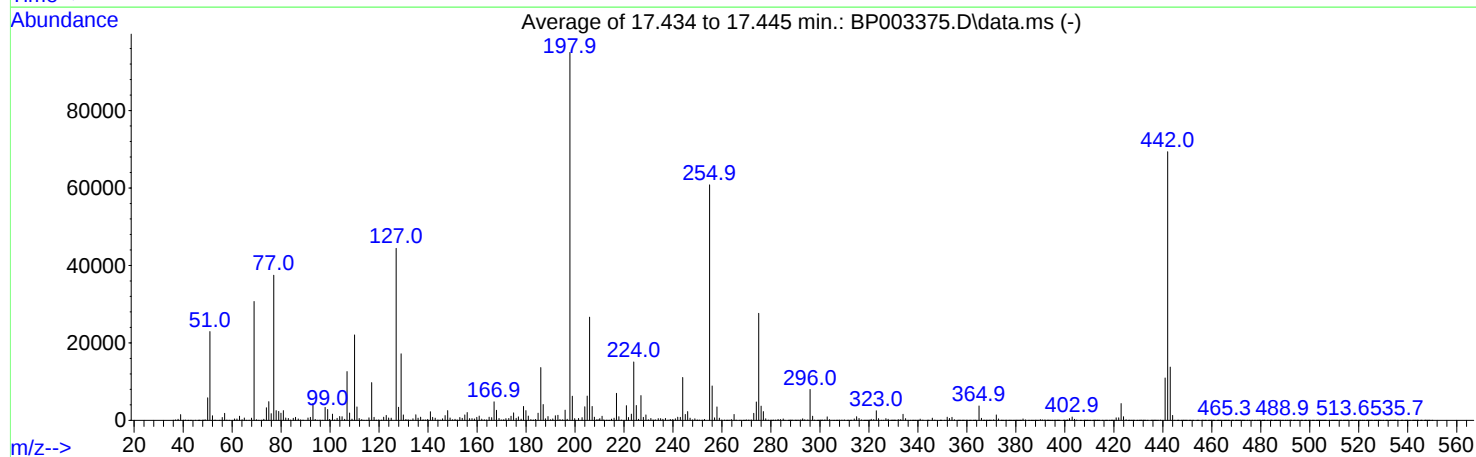


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092520\
 Data File : BP003375.D
 Acq On : 25 Sep 2020 11:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 22 12:48:08 2020

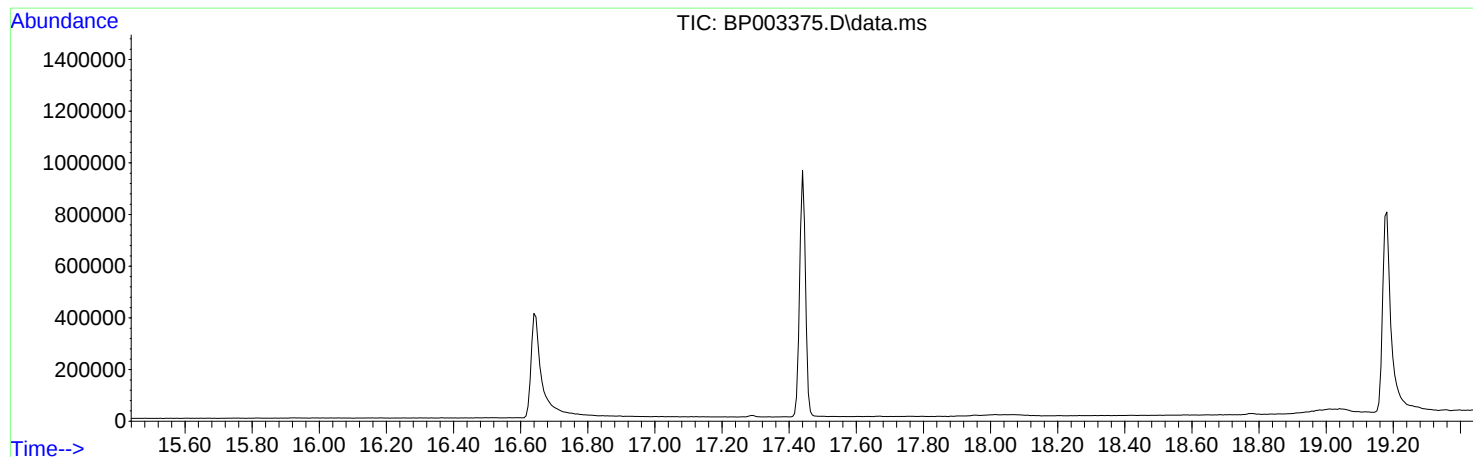

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.1	22932	PASS
68	69	0.00	2	1.8	566	PASS
69	198	0.00	100	32.3	30678	PASS
70	69	0.00	2	0.5	155	PASS
127	198	10	80	46.8	44419	PASS
197	198	0.00	2	0.3	278	PASS
198	198	100	100	100.0	94979	PASS
199	198	5	9	6.6	6255	PASS
275	198	10	60	29.1	27643	PASS
365	198	1	100	3.9	3712	PASS
441	198	0.01	100	11.5	10964	PASS
442	198	50	100	73.1	69384	PASS
443	442	15	24	19.8	13741	PASS