
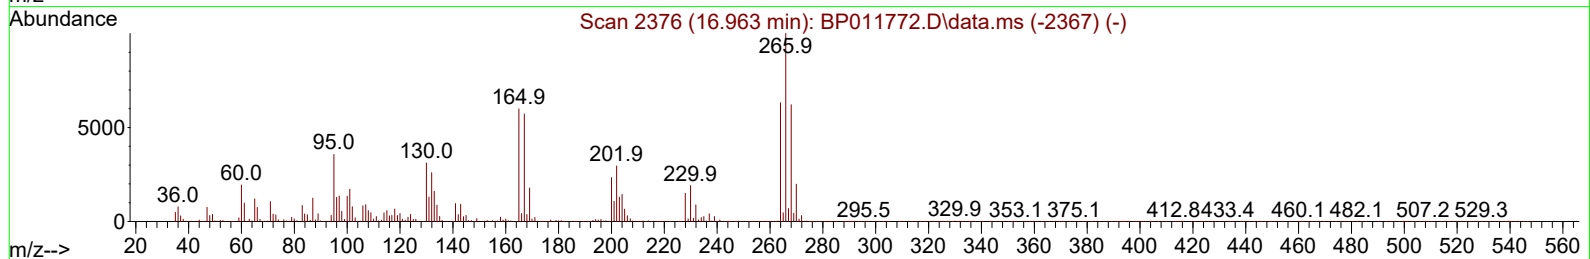
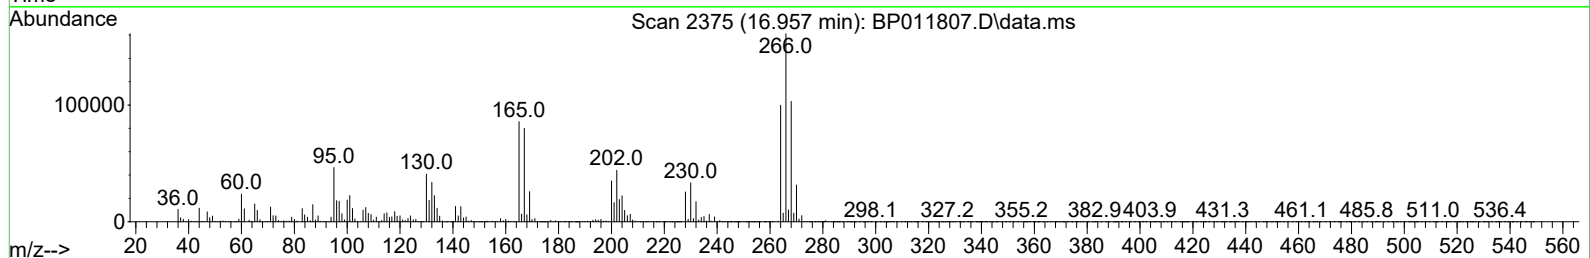


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
Data File : BP011807.D
Acq On : 27 Sep 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 06:56:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:03:33 2022
Response via : Initial Calibration

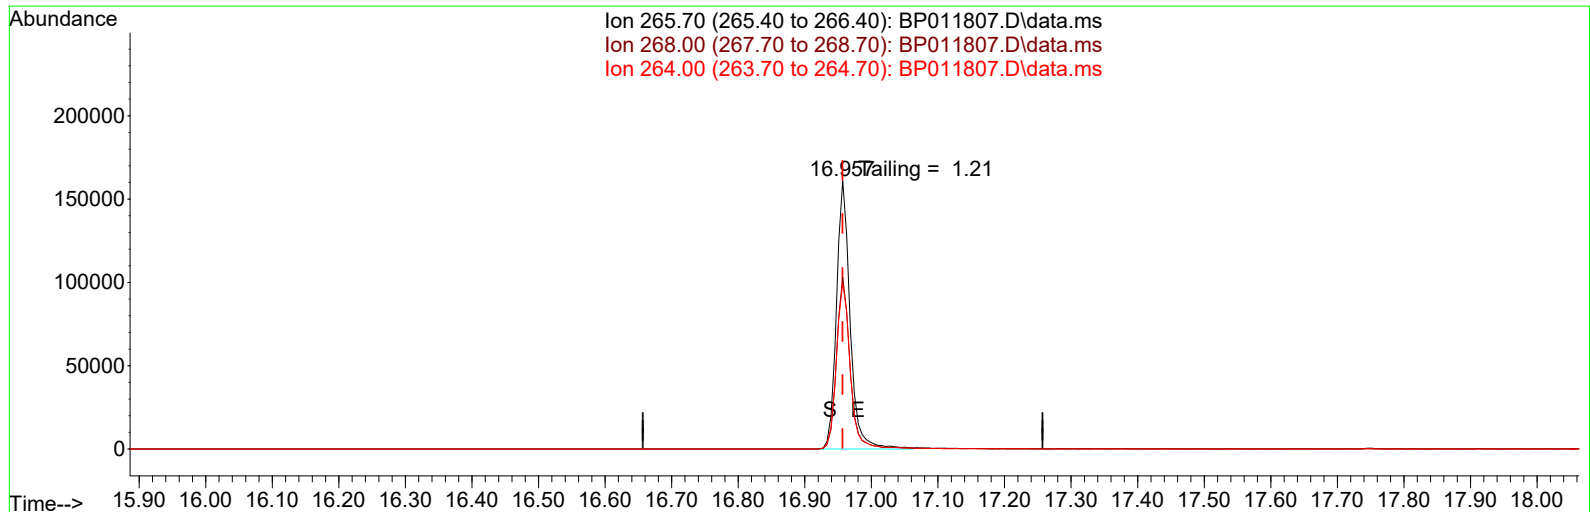

TIC: BP011807.D\data.ms

(70) Pentachlorophenol (C)




16.957min (-0.000) 1331873.36 ng

response 229667

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	63.97
264.00	63.20	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
Data File : BP011807.D
Acq On : 27 Sep 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 06:56:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:03:33 2022
Response via : Initial Calibration

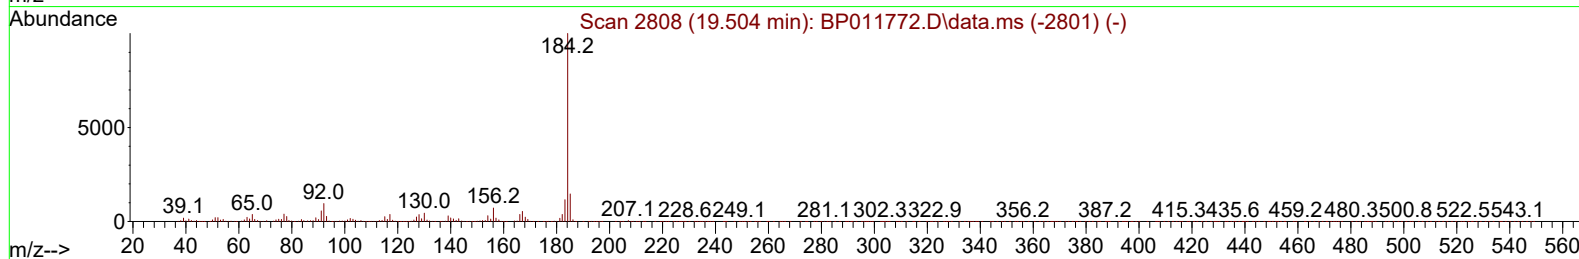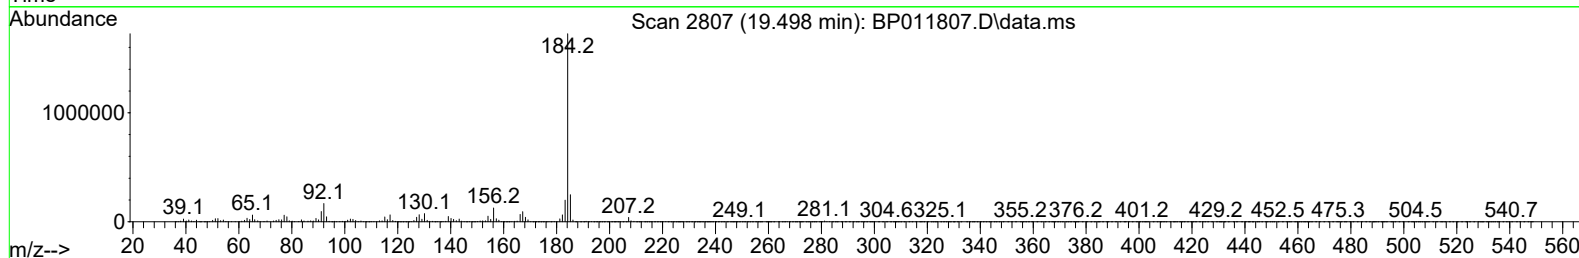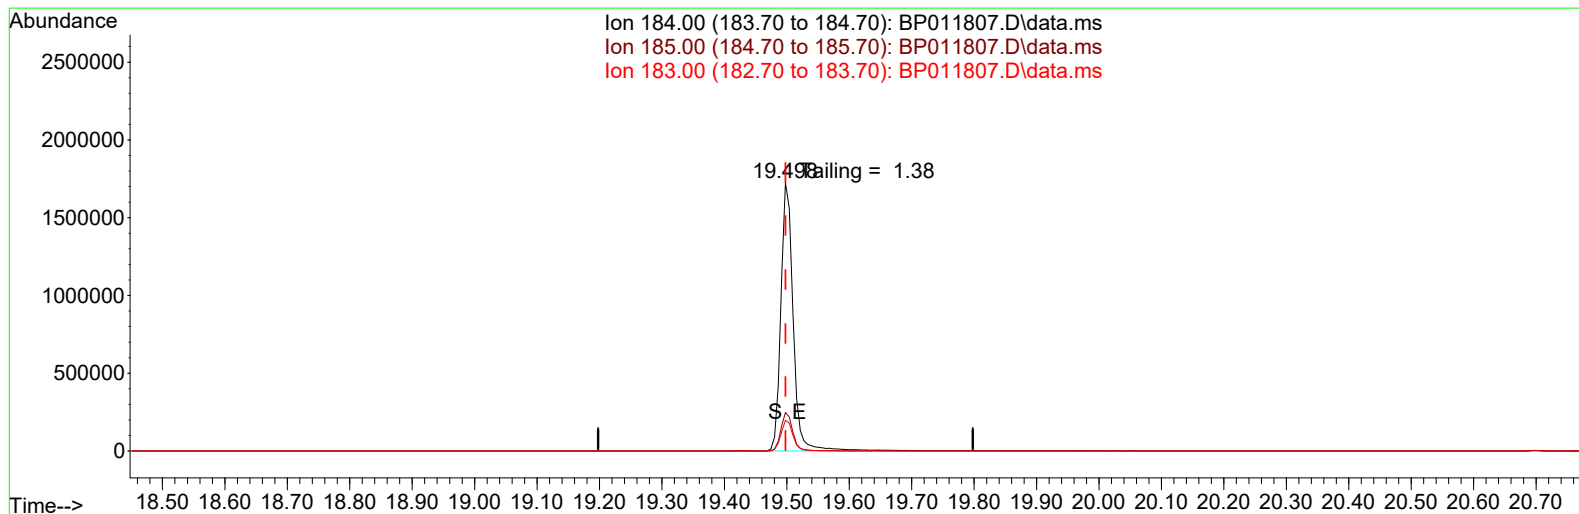

TIC: BP011807.D\data.ms

(77) Benzidine**19.498min (-0.000) 463422.63 ng****response 2383443**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.38
183.00	11.60	11.45
0.00	0.00	0.00