

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
 Data File : BP011809.D
 Acq On : 27 Sep 2022 11:06
 Operator : CG/JU
 Sample : PB147869BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB147869BL

Quant Time: Sep 28 02:05:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:03:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	248056	20.000	ng	0.00
21) Naphthalene-d8	10.722	136	1056908	20.000	ng	0.00
39) Acenaphthene-d10	14.551	164	683273	20.000	ng	0.00
64) Phenanthrene-d10	17.310	188	1565312	20.000	ng	0.00
76) Chrysene-d12	21.392	240	1547337	20.000	ng	0.00
86) Perylene-d12	23.839	264	1566408	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.470	112	2440094	172.598	ng	0.00
7) Phenol-d6	7.075	99	3238382	154.919	ng	0.00
23) Nitrobenzene-d5	9.075	82	1725048	85.428	ng	0.00
42) 2,4,6-Tribromophenol	16.051	330	908734	197.517	ng	0.00
45) 2-Fluorobiphenyl	13.181	172	4115849	95.259	ng	0.00
79) Terphenyl-d14	19.869	244	7117181	105.761	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
Data File : BP011809.D
Acq On : 27 Sep 2022 11:06
Operator : CG/JU
Sample : PB147869BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB147869BL

Quant Time: Sep 28 02:05:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:03:33 2022
Response via : Initial Calibration




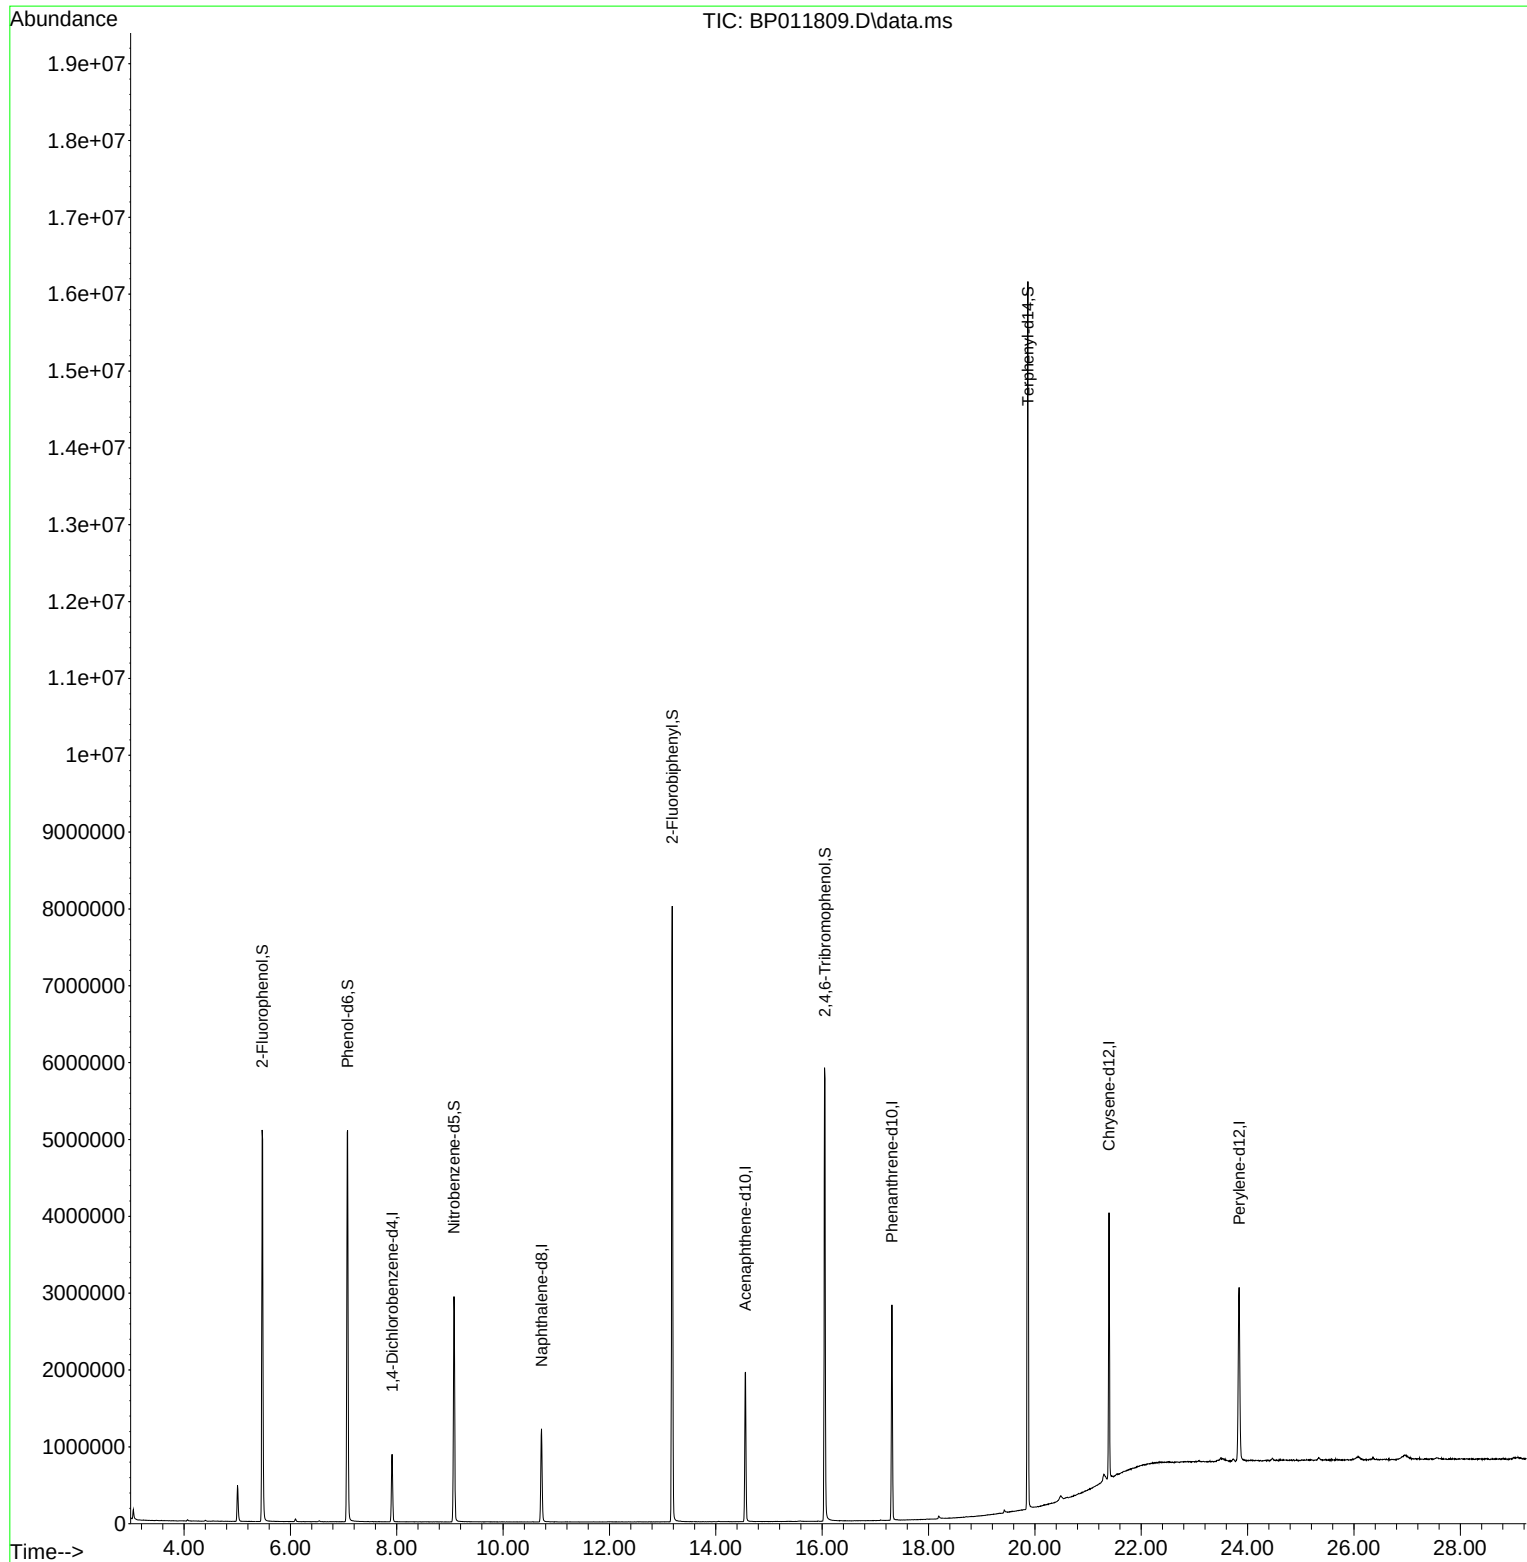




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.911 min Scan# 839
Delta R.T. 0.001 min
Lab File: BP011809.D
Acq: 27 Sep 2022 11:06




Instrument :
BNA_P
ClientSampleId :
PB147869BL


Tgt Ion:152 Resp: 248056
Ion Ratio Lower Upper
152 100
150 153.9 124.2 186.4
115 59.4 50.0 75.0

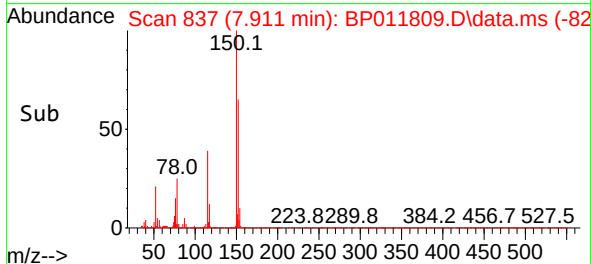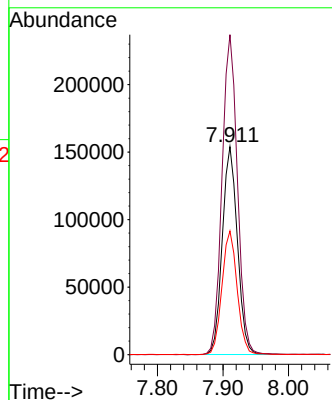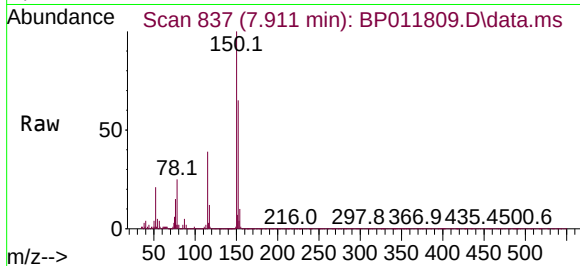

#5
2-Fluorophenol
Concen: 172.598 ng
RT: 5.470 min Scan# 422
Delta R.T. 0.000 min
Lab File: BP011809.D
Acq: 27 Sep 2022 11:06

Tgt Ion:112 Resp: 2440094
Ion Ratio Lower Upper
112 100
64 58.9 49.2 73.8
63 29.6 25.2 37.8


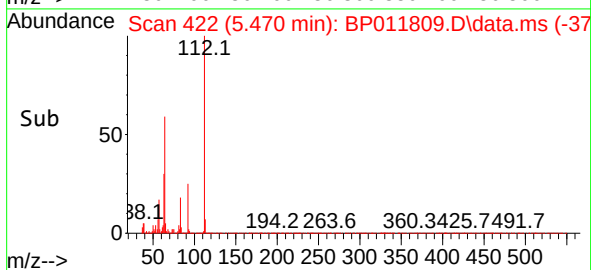
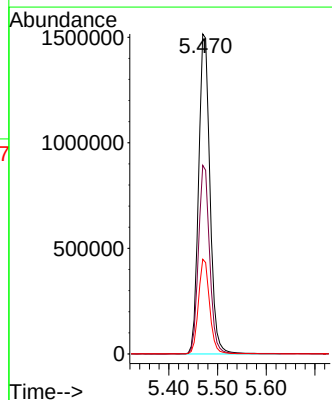
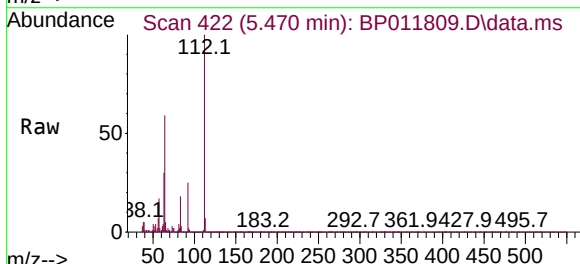




#7
Phenol-d6
Concen: 154.919 ng
RT: 7.075 min Scan# 69
Delta R.T. 0.006 min
Lab File: BP011809.D
Acq: 27 Sep 2022 11:06




Instrument :
BNA_P
ClientSampleId :
PB147869BL


Tgt Ion: 99 Resp: 3238382
Ion Ratio Lower Upper
99 100
42 15.1 15.4 23.2#
71 30.0 24.7 37.1

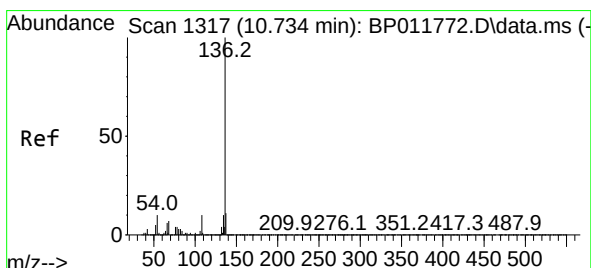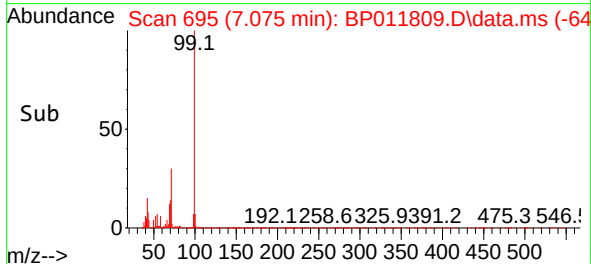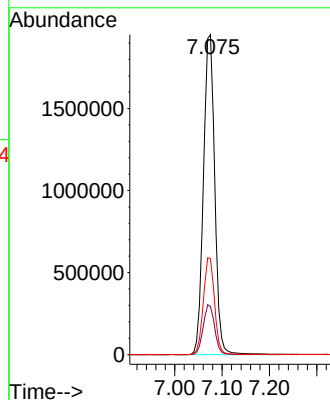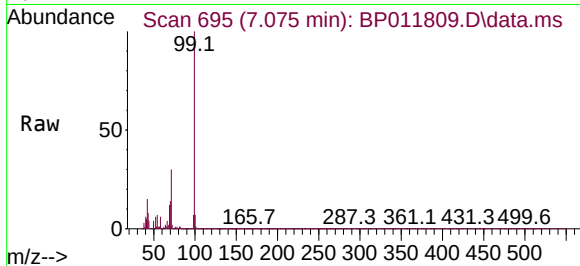

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.722 min Scan# 1315
Delta R.T. 0.000 min
Lab File: BP011809.D
Acq: 27 Sep 2022 11:06

Tgt Ion: 136 Resp: 1056908
Ion Ratio Lower Upper
136 100
137 10.8 8.8 13.2
54 8.6 8.2 12.4
68 6.9 5.8 8.8


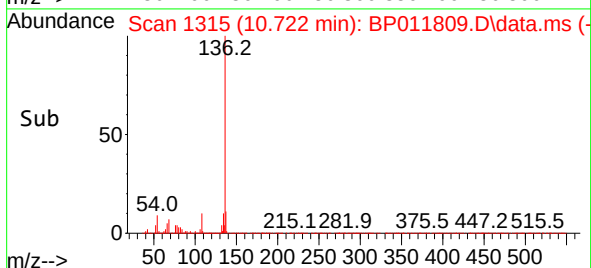
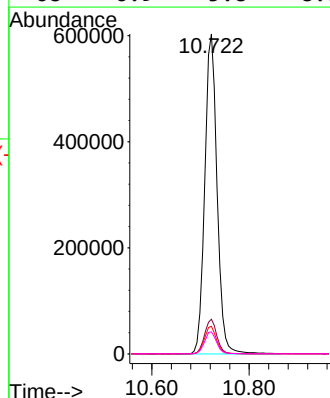
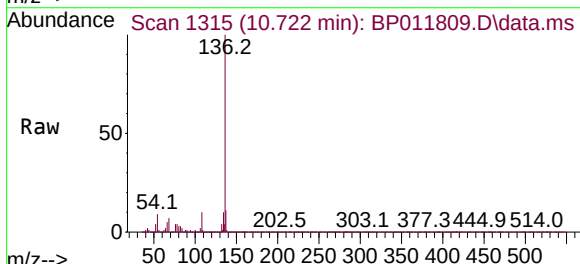




#23
Nitrobenzene-d5
Concen: 85.428 ng
RT: 9.075 min Scan# 1035
Delta R.T. 0.000 min
Lab File: BP011809.D
Acq: 27 Sep 2022 11:06




Instrument :
BNA_P
ClientSampleId :
PB147869BL


Tgt Ion: 82 Resp: 1725048
Ion Ratio Lower Upper
82 100
128 44.0 34.2 51.4
54 49.9 43.1 64.7

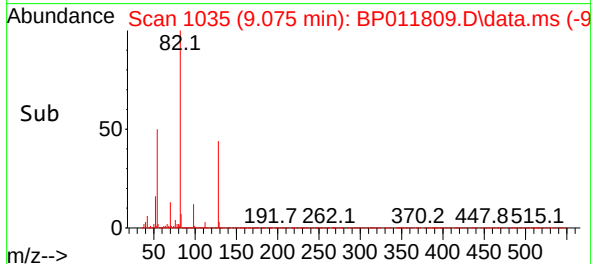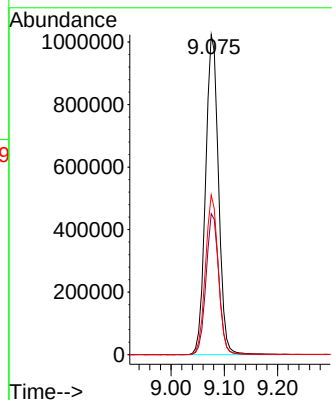

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.551 min Scan# 1966
Delta R.T. -0.006 min
Lab File: BP011809.D
Acq: 27 Sep 2022 11:06

Tgt Ion:164 Resp: 683273
Ion Ratio Lower Upper
164 100
162 101.5 82.5 123.7
160 46.6 37.8 56.6


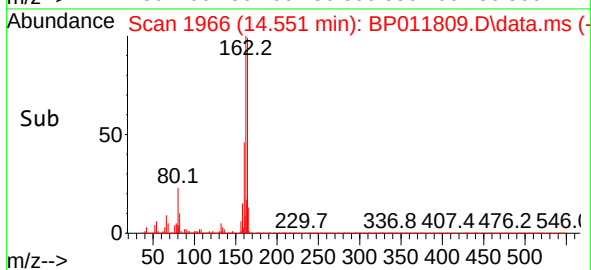
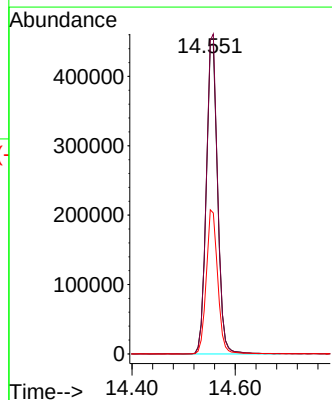
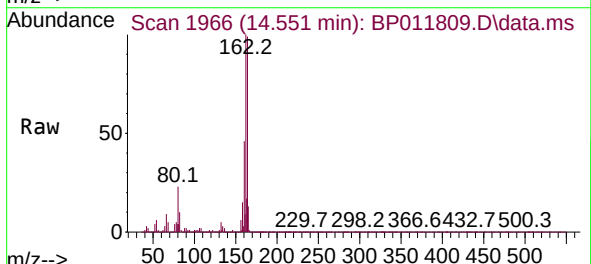




#42
2,4,6-Tribromophenol
Concen: 197.517 ng
RT: 16.051 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP011809.D
Acq: 27 Sep 2022 11:06




Instrument :
BNA_P
ClientSampleId :
PB147869BL


Tgt Ion:330 Resp: 908734
Ion Ratio Lower Upper
330 100
332 95.0 76.6 114.8
141 50.0 48.7 73.1

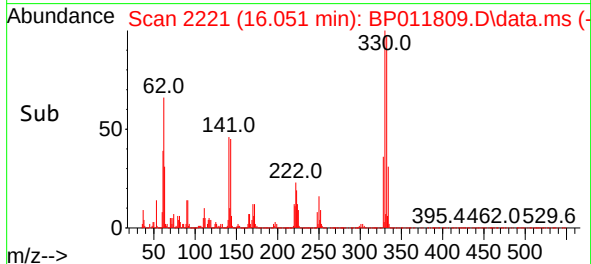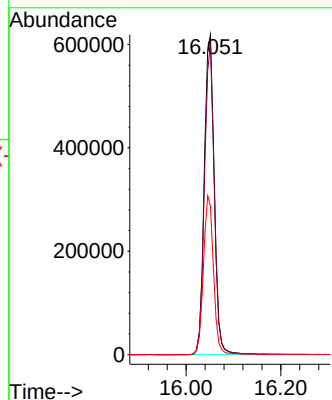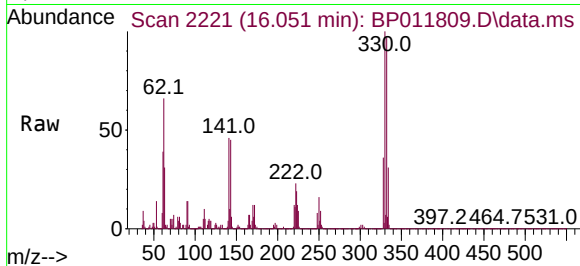

#45
2-Fluorobiphenyl
Concen: 95.259 ng
RT: 13.181 min Scan# 1733
Delta R.T. 0.000 min
Lab File: BP011809.D
Acq: 27 Sep 2022 11:06

Tgt Ion:172 Resp: 4115849
Ion Ratio Lower Upper
172 100
171 35.2 27.9 41.9
170 24.0 19.5 29.3


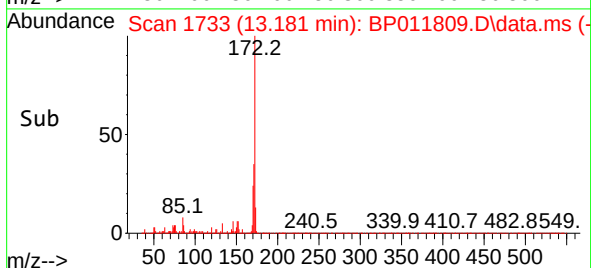
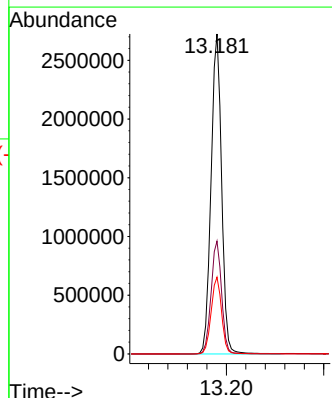
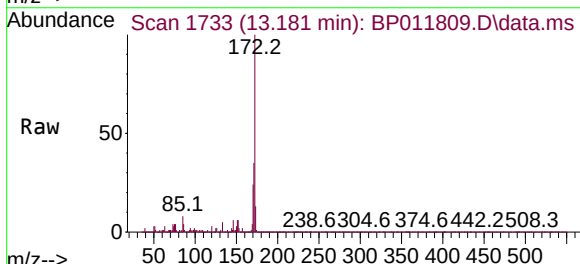




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.310 min Scan# 2437
Delta R.T. 0.000 min
Lab File: BP011809.D
Acq: 27 Sep 2022 11:06




Instrument :
BNA_P
ClientSampleId :
PB147869BL


Tgt Ion:188 Resp: 1565312
Ion Ratio Lower Upper
188 100
94 11.5 9.4 14.0
80 12.4 10.6 15.8

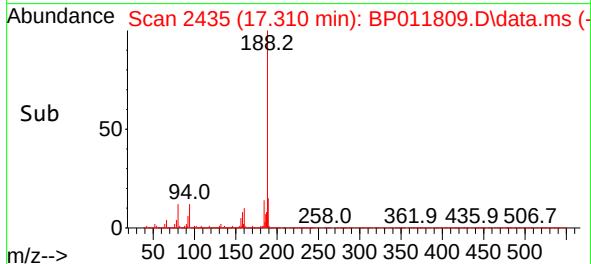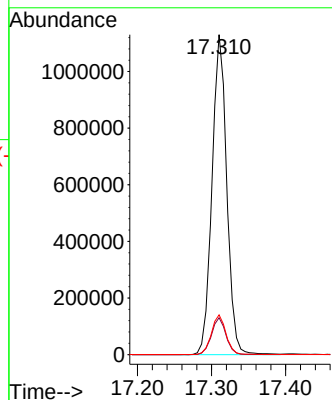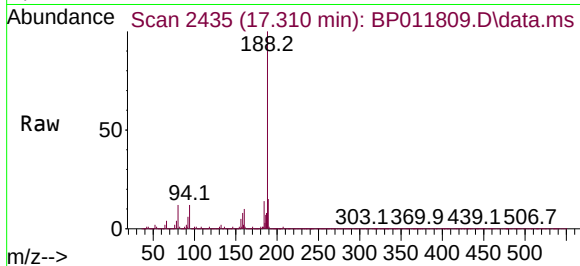

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.392 min Scan# 3129
Delta R.T. -0.006 min
Lab File: BP011809.D
Acq: 27 Sep 2022 11:06

Tgt Ion:240 Resp: 1547337
Ion Ratio Lower Upper
240 100
120 15.2 12.0 18.0
236 26.6 21.1 31.7

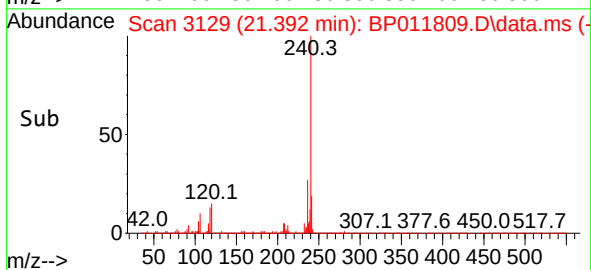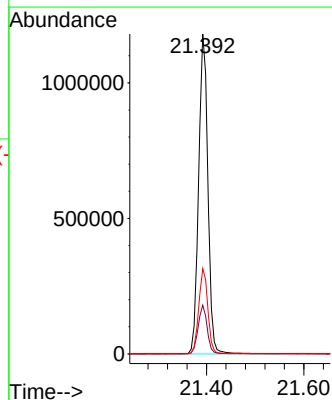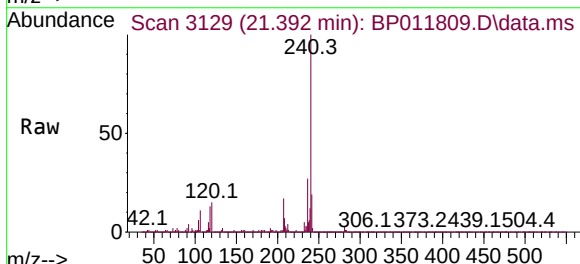

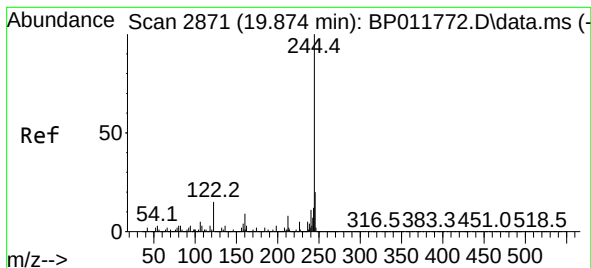

#79

Terphenyl-d14

Concen: 105.761 ng

RT: 19.869 min Scan# 2871

Delta R.T. 0.000 min

Lab File: BP011809.D

Acq: 27 Sep 2022 11:06

Instrument :

BNA_P

ClientSampleId :

PB147869BL





Tgt Ion:244 Resp: 7117181

Ion Ratio Lower Upper

244 100

212 8.3 6.5 9.7

122 13.7 11.8 17.8

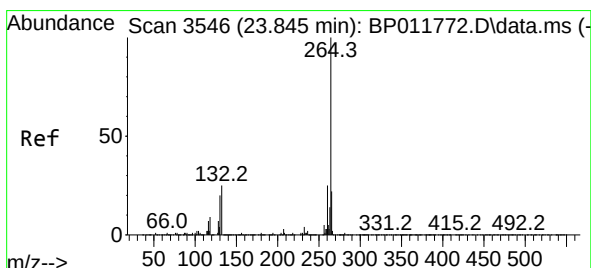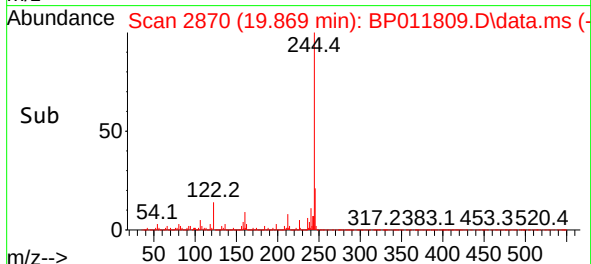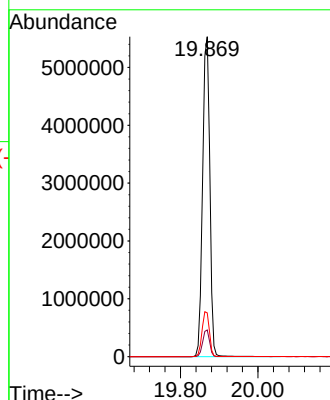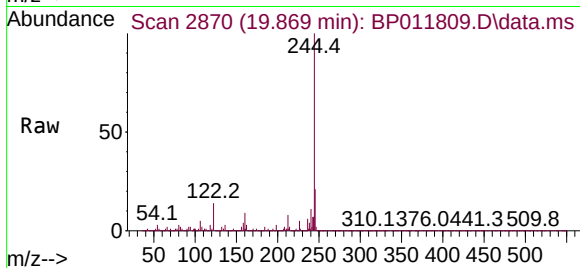

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.839 min Scan# 3545

Delta R.T. 0.000 min

Lab File: BP011809.D

Acq: 27 Sep 2022 11:06

Tgt Ion:264 Resp: 1566408

Ion Ratio Lower Upper

264 100

260 24.8 19.7 29.5

265 22.3 17.8 26.8

