

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
 Data File : BP011823.D
 Acq On : 27 Sep 2022 19:30
 Operator : CG/JU
 Sample : N4839-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 5592-2

Quant Time: Sep 28 02:09:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:03:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.910	152	351907	20.000	ng	0.00
21) Naphthalene-d8	10.716	136	1522881	20.000	ng	0.00
39) Acenaphthene-d10	14.551	164	970093	20.000	ng	0.00
64) Phenanthrene-d10	17.310	188	2060505	20.000	ng	0.00
76) Chrysene-d12	21.392	240	1934460	20.000	ng	0.00
86) Perylene-d12	23.833	264	1965342	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.469	112	1131696	56.426	ng	0.00
7) Phenol-d6	7.069	99	850959	28.695	ng	0.00
23) Nitrobenzene-d5	9.075	82	2262705	77.768	ng	0.00
42) 2,4,6-Tribromophenol	16.045	330	1271986	194.729	ng	0.00
45) 2-Fluorobiphenyl	13.181	172	5296981	86.348	ng	0.00
79) Terphenyl-d14	19.863	244	7969491	94.727	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
Data File : BP011823.D
Acq On : 27 Sep 2022 19:30
Operator : CG/JU
Sample : N4839-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
5592-2

Quant Time: Sep 28 02:09:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:03:33 2022
Response via : Initial Calibration




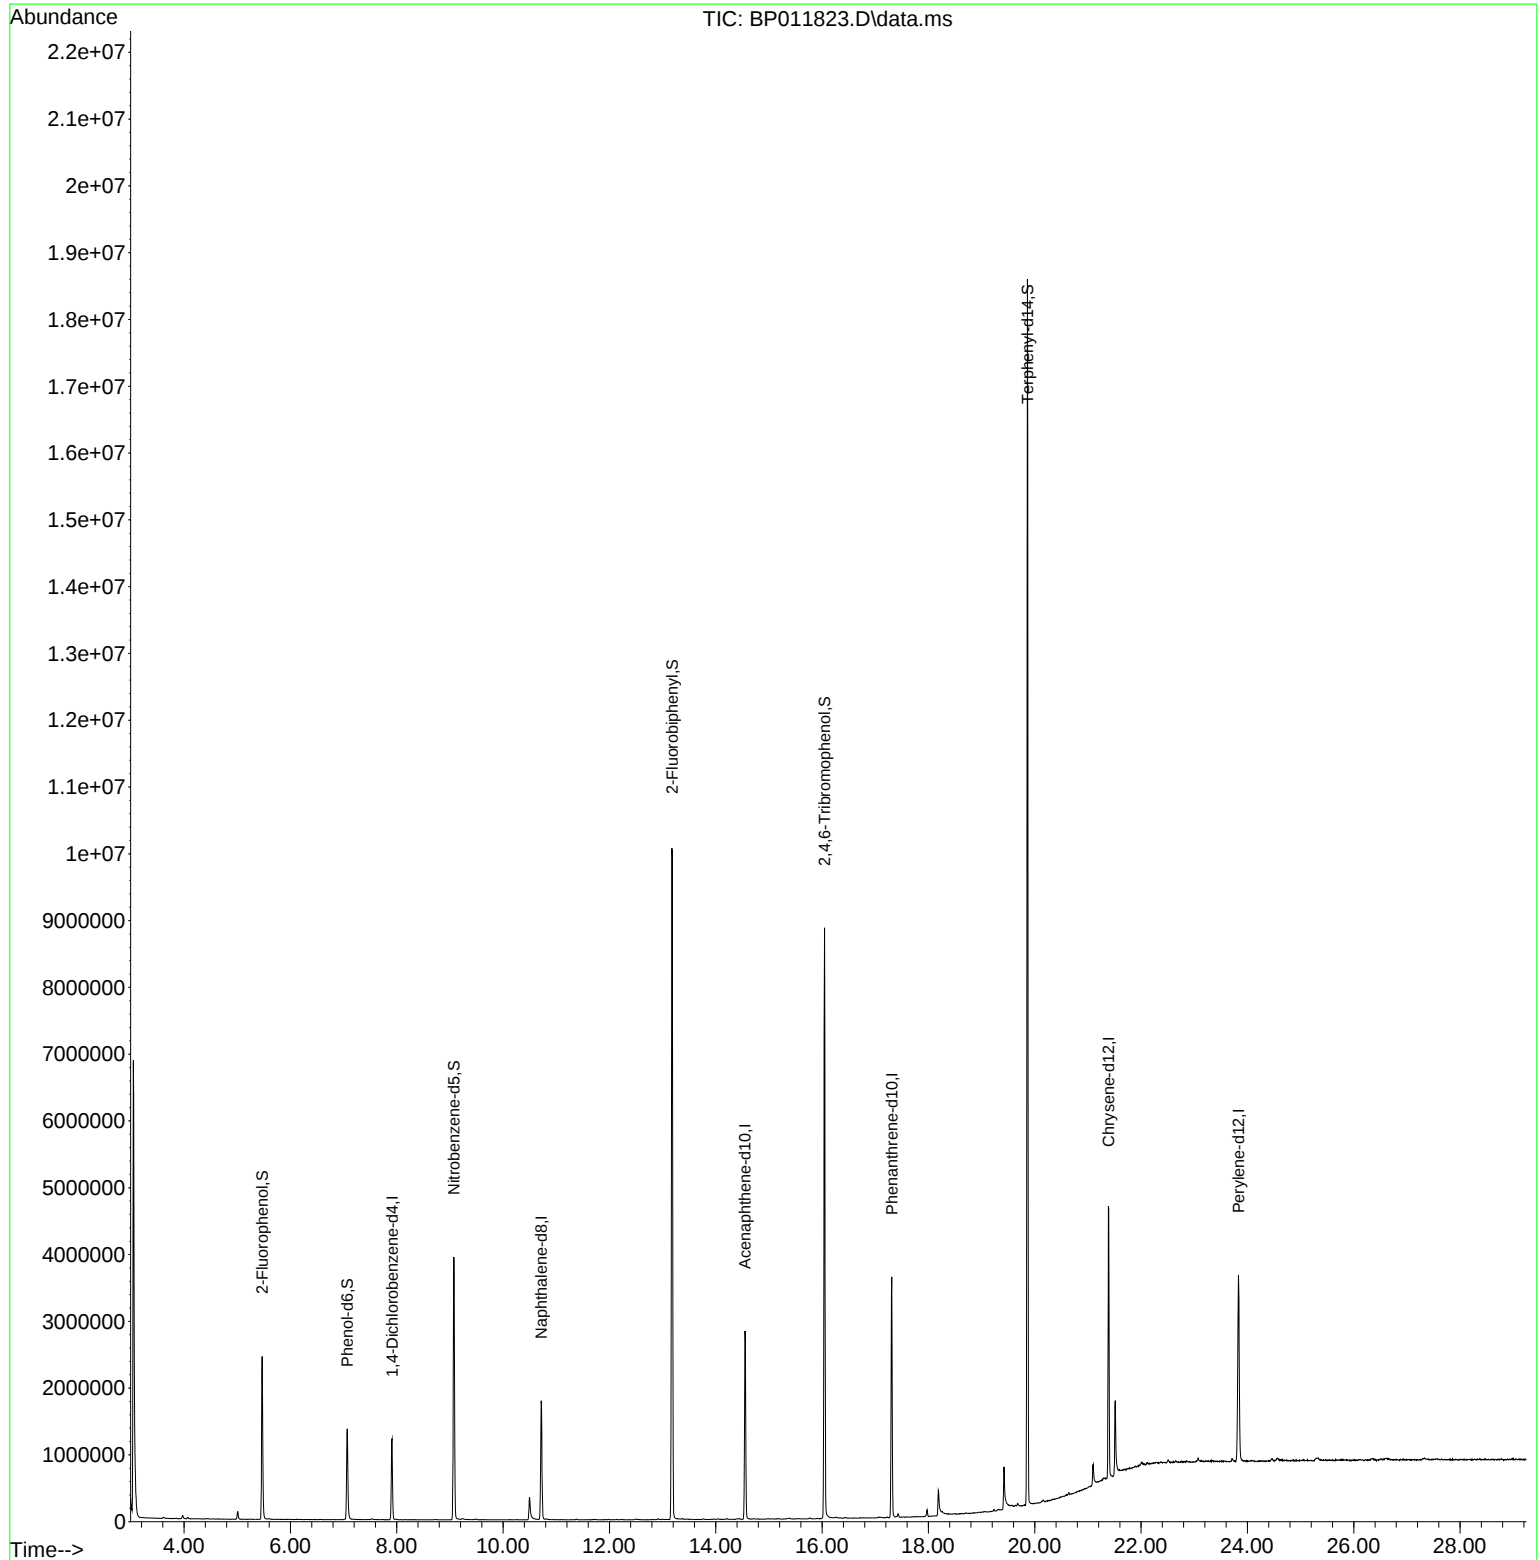


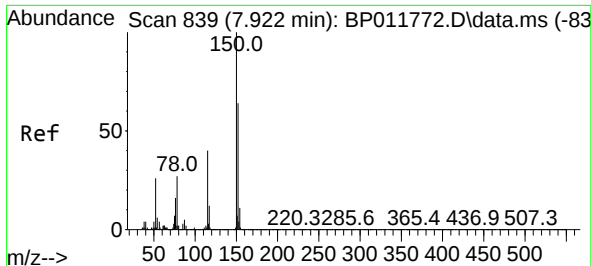

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.910 min Scan# 839
Delta R.T. 0.000 min
Lab File: BP011823.D
Acq: 27 Sep 2022 19:30




Instrument :
BNA_P
ClientSampleId :
5592-2


Tgt Ion:152 Resp: 351907
Ion Ratio Lower Upper
152 100
150 159.0 124.2 186.4
115 58.6 50.0 75.0

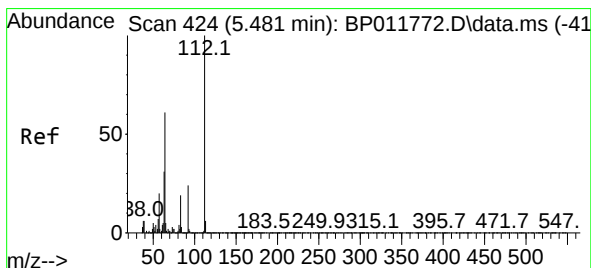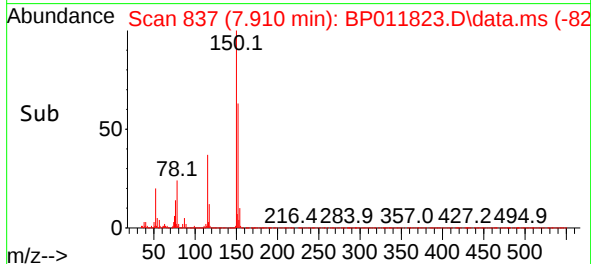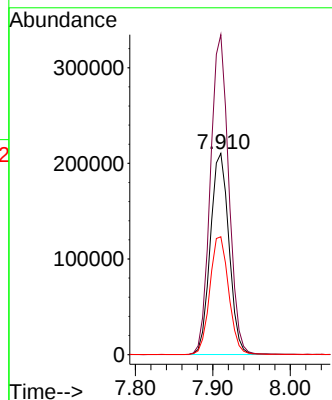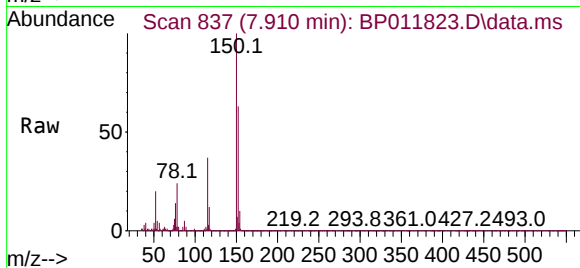

#5
2-Fluorophenol
Concen: 56.426 ng
RT: 5.469 min Scan# 422
Delta R.T. -0.000 min
Lab File: BP011823.D
Acq: 27 Sep 2022 19:30

Tgt Ion:112 Resp: 1131696
Ion Ratio Lower Upper
112 100
64 58.0 49.2 73.8
63 29.1 25.2 37.8


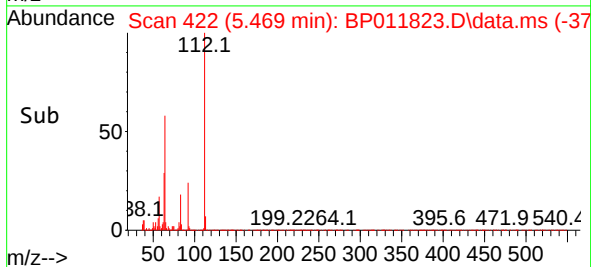
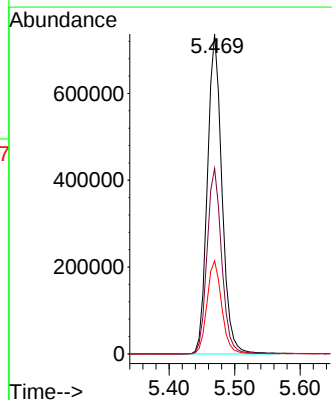
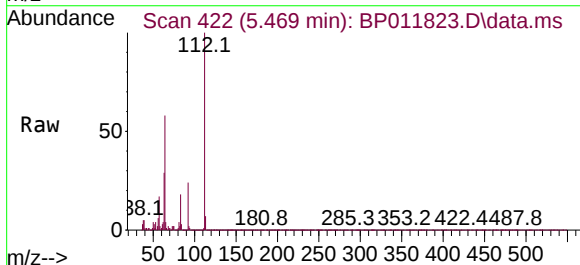


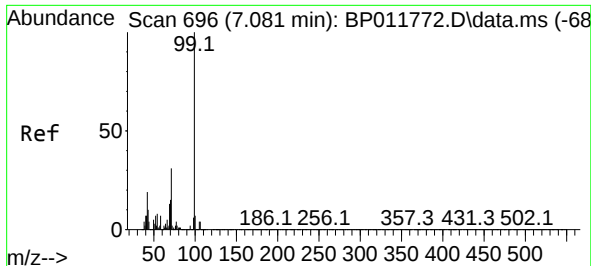

#7
Phenol-d6
Concen: 28.695 ng
RT: 7.069 min Scan# 69
Delta R.T. -0.000 min
Lab File: BP011823.D
Acq: 27 Sep 2022 19:30




Instrument :
BNA_P
ClientSampleId :
5592-2


Tgt Ion: 99 Resp: 850959
Ion Ratio Lower Upper
99 100
42 15.9 15.4 23.2
71 29.6 24.7 37.1

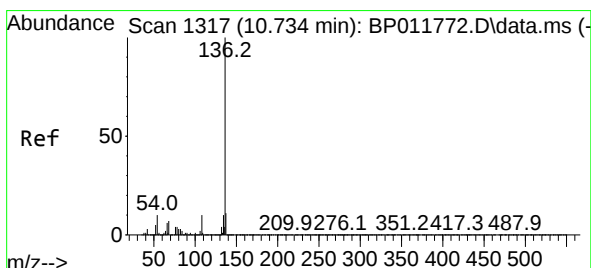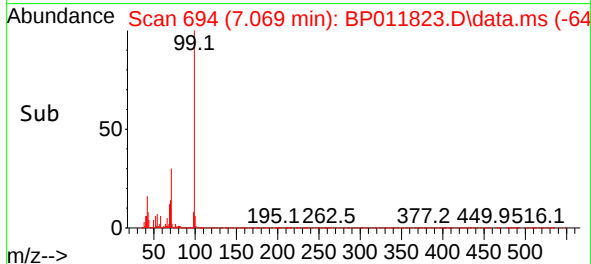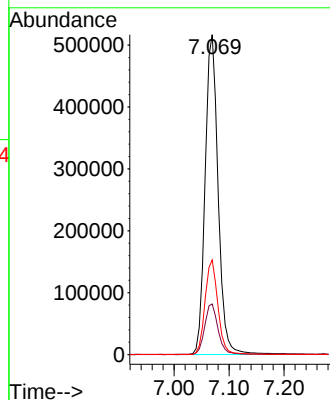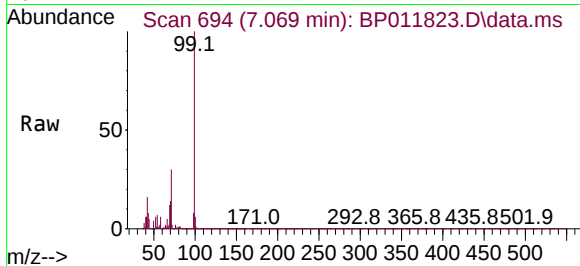

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.716 min Scan# 1314
Delta R.T. -0.006 min
Lab File: BP011823.D
Acq: 27 Sep 2022 19:30

Tgt Ion: 136 Resp: 1522881
Ion Ratio Lower Upper
136 100
137 11.2 8.8 13.2
54 8.7 8.2 12.4
68 7.0 5.8 8.8

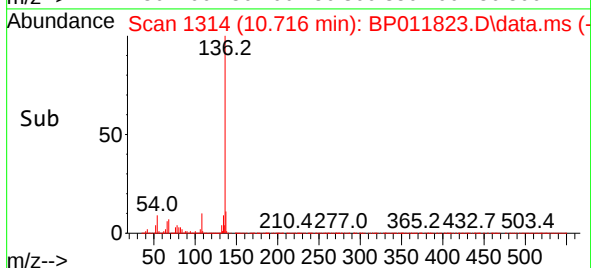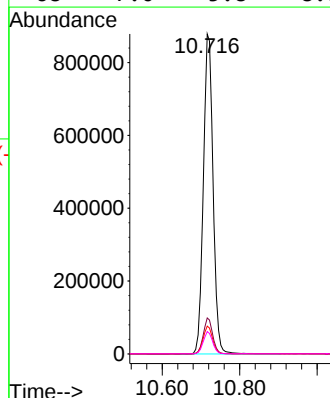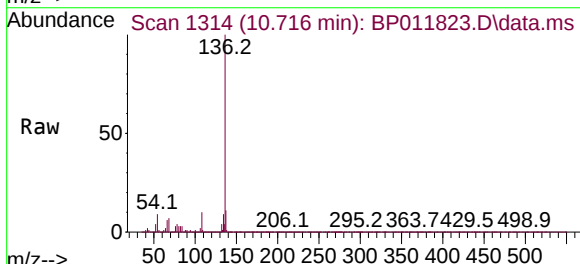

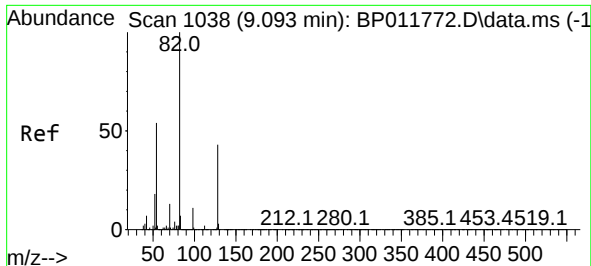

#23

Nitrobenzene-d5

Concen: 77.768 ng

RT: 9.075 min Scan# 1035

Delta R.T. -0.000 min

Lab File: BP011823.D

Acq: 27 Sep 2022 19:30

Instrument :





BNA_P

ClientSampleId :

5592-2

Tgt Ion: 82 Resp: 2262705

Ion	Ratio	Lower	Upper
82	100		
128	45.1	34.2	51.4
54	49.5	43.1	64.7

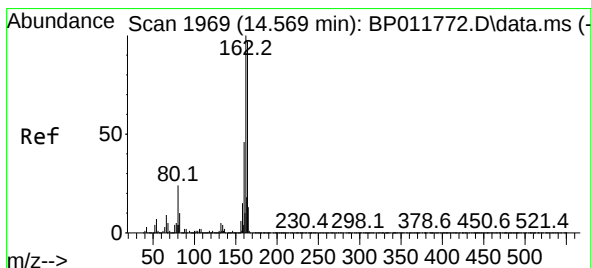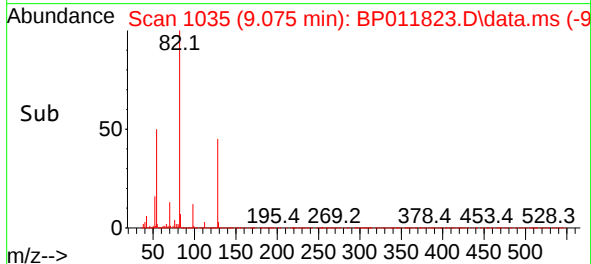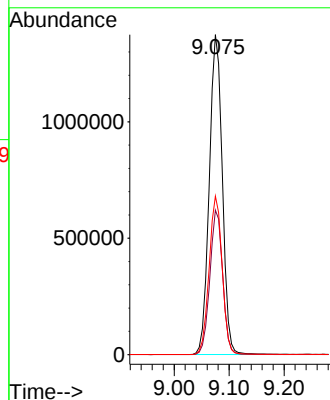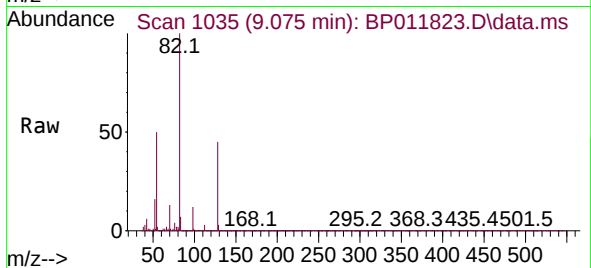

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.551 min Scan# 1966




Delta R.T. -0.006 min


Lab File: BP011823.D

Acq: 27 Sep 2022 19:30

Tgt Ion:164 Resp: 970093

Ion	Ratio	Lower	Upper
164	100		
162	101.5	82.5	123.7
160	45.8	37.8	56.6


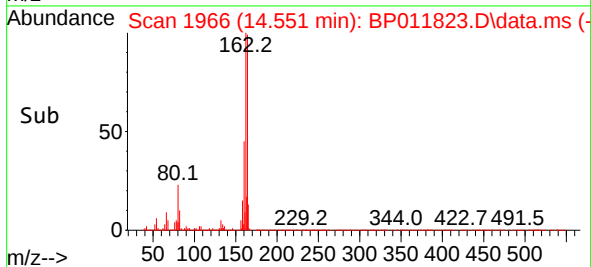
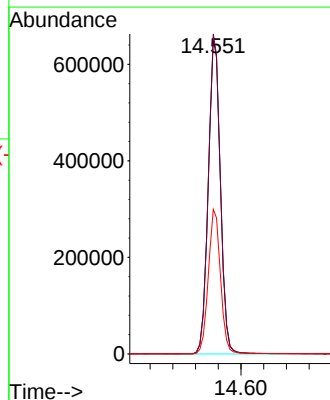
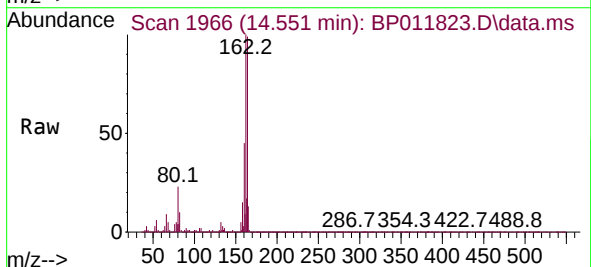


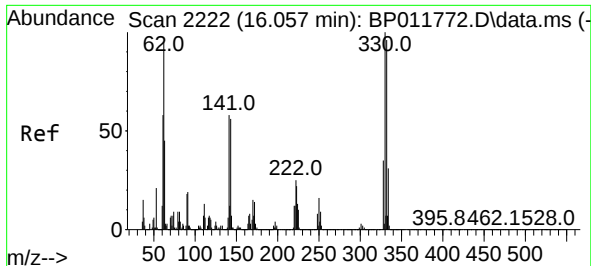

#42
2,4,6-Tribromophenol
Concen: 194.729 ng
RT: 16.045 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP011823.D
Acq: 27 Sep 2022 19:30




Instrument :
BNA_P
ClientSampleId :
5592-2


Tgt Ion:330 Resp: 1271986
Ion Ratio Lower Upper
330 100
332 95.2 76.6 114.8
141 49.5 48.7 73.1

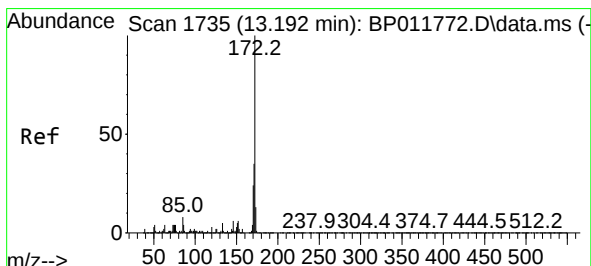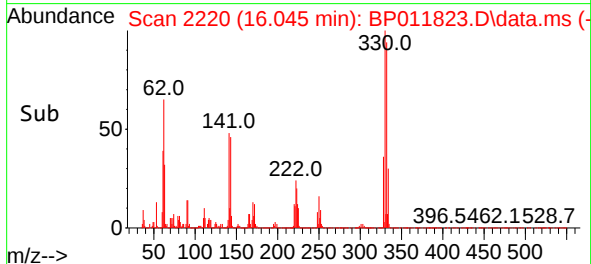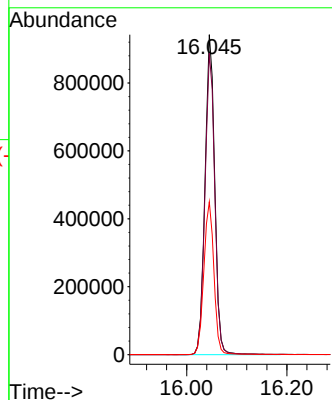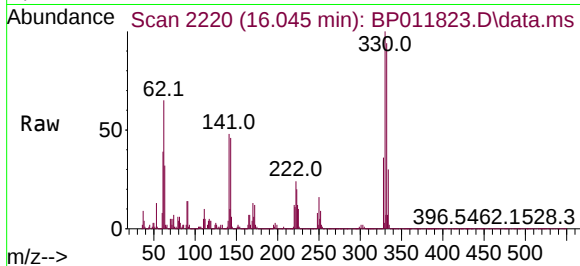

#45
2-Fluorobiphenyl
Concen: 86.348 ng
RT: 13.181 min Scan# 1733
Delta R.T. -0.000 min
Lab File: BP011823.D
Acq: 27 Sep 2022 19:30

Tgt Ion:172 Resp: 5296981
Ion Ratio Lower Upper
172 100
171 35.6 27.9 41.9
170 24.1 19.5 29.3

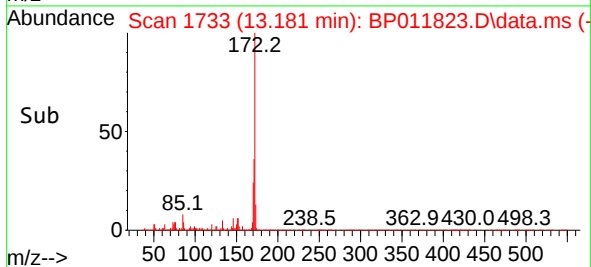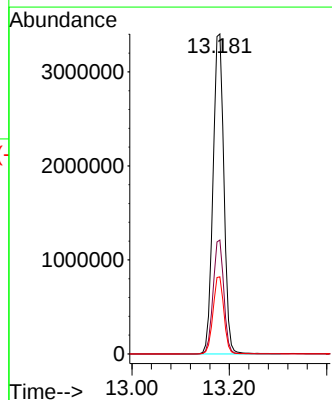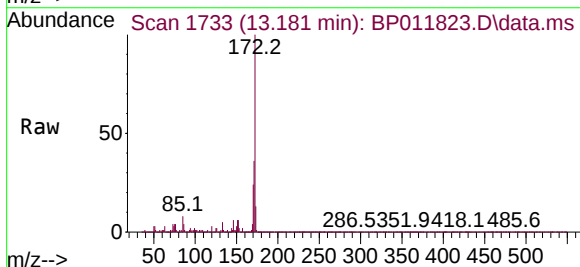

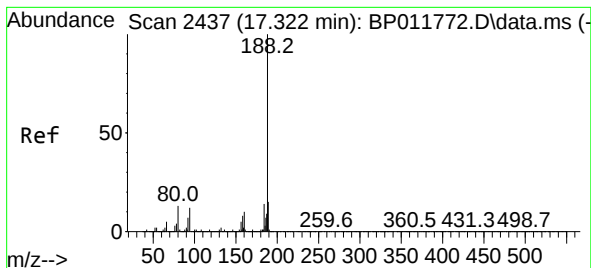

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.310 min Scan# 2437

Delta R.T. -0.000 min

Lab File: BP011823.D

Acq: 27 Sep 2022 19:30

Instrument :

BNA_P

ClientSampleId :

5592-2





Tgt Ion:188 Resp: 2060505

Ion Ratio Lower Upper

188 100

94 10.9 9.4 14.0

80 11.7 10.6 15.8

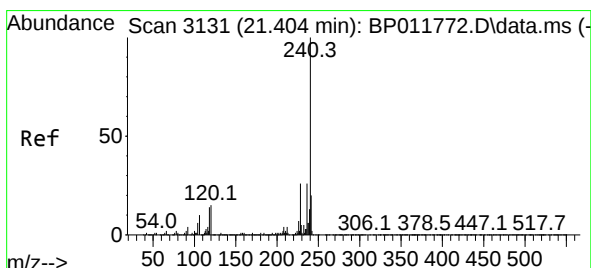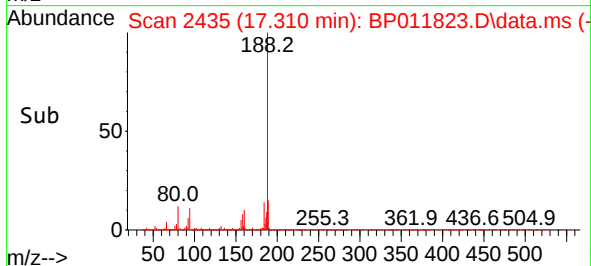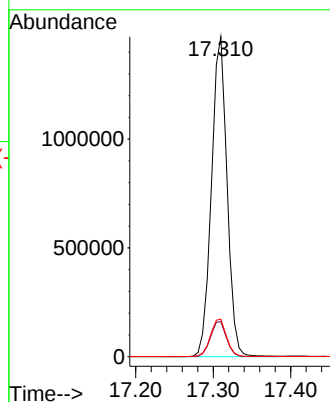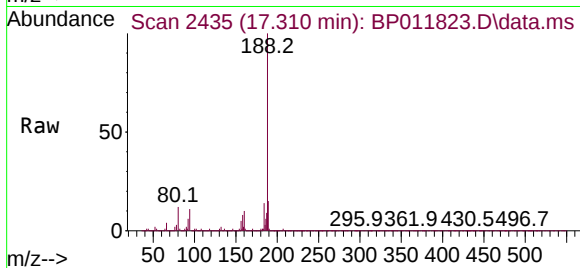

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.392 min Scan# 3129

Delta R.T. -0.006 min

Lab File: BP011823.D

Acq: 27 Sep 2022 19:30




Tgt Ion:240 Resp: 1934460


Ion Ratio Lower Upper

240 100

120 13.6 12.0 18.0

236 27.1 21.1 31.7

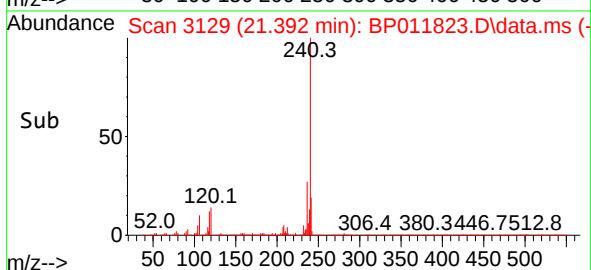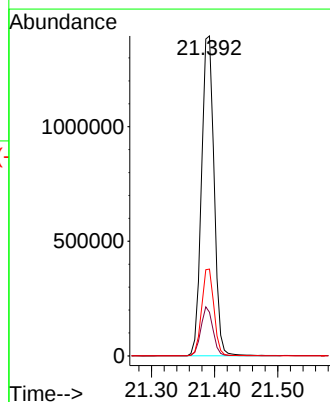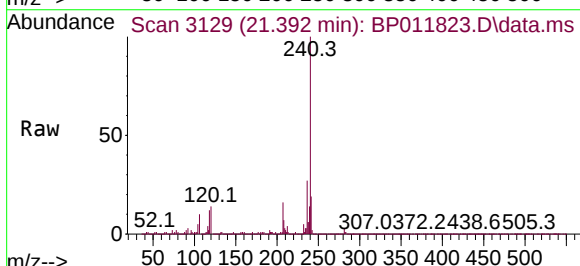

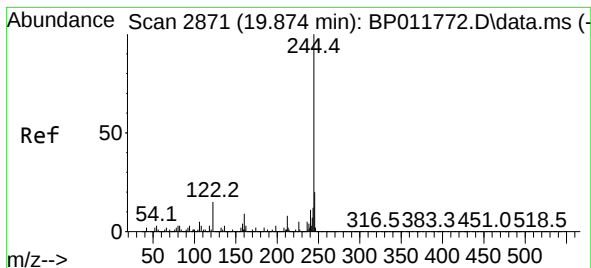

#79

Terphenyl-d14

Concen: 94.727 ng

RT: 19.863 min Scan# 2869

Delta R.T. -0.006 min

Lab File: BP011823.D

Acq: 27 Sep 2022 19:30

Instrument :

BNA_P

ClientSampleId :

5592-2





Tgt Ion:244 Resp: 7969491

Ion Ratio Lower Upper

244 100

212 8.5 6.5 9.7

122 14.6 11.8 17.8

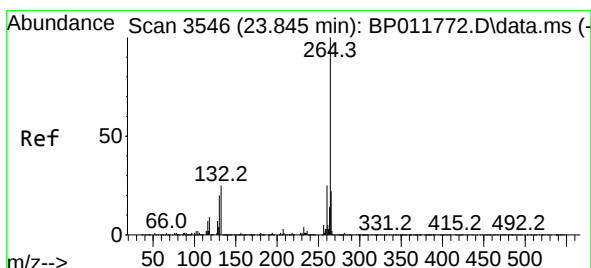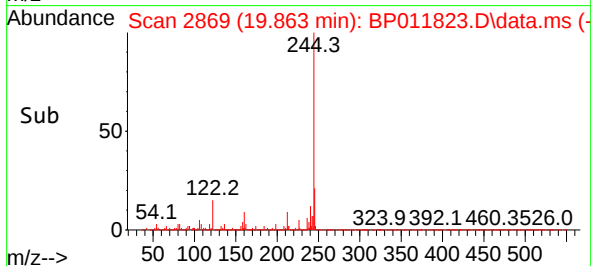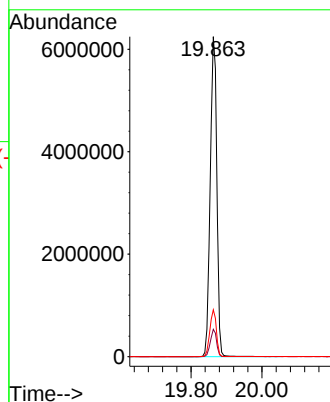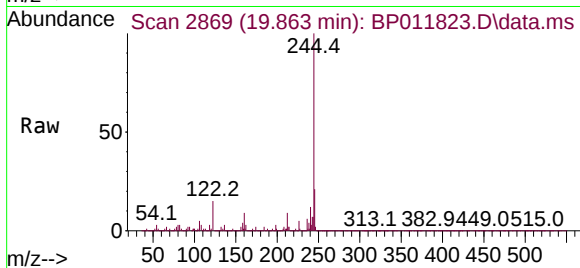

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.833 min Scan# 3544

Delta R.T. -0.006 min

Lab File: BP011823.D

Acq: 27 Sep 2022 19:30

Tgt Ion:264 Resp: 1965342

Ion Ratio Lower Upper

264 100

260 24.6 19.7 29.5

265 21.9 17.8 26.8

