

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
 Data File : BP011823.D
 Acq On : 27 Sep 2022 19:30
 Operator : CG/JU
 Sample : N4839-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 5592-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP011823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	6	10	32	rVB	6844766	10713930	46.78%	10.171%
2	5.469	415	422	439	rBV	2439221	3770478	16.46%	3.579%
3	7.069	682	694	708	rBV	1359526	2313771	10.10%	2.196%
4	7.910	828	837	845	rBV	1212314	2040694	8.91%	1.937%
5	9.075	1027	1035	1048	rBV	3932285	6515120	28.45%	6.185%
6	10.498	1271	1277	1298	rBV	340583	734765	3.21%	0.697%
7	10.716	1307	1314	1325	rBV	1775285	3034063	13.25%	2.880%
8	13.175	1725	1732	1749	rBV	10051885	15555816	67.92%	14.767%
9	14.551	1959	1966	1981	rBV	2818371	4240984	18.52%	4.026%
10	16.045	2208	2220	2241	rBV	8850470	12484643	54.51%	11.851%
11	17.310	2428	2435	2447	rBV	3606473	5157098	22.52%	4.896%
12	18.186	2580	2584	2594	rBV	379818	741505	3.24%	0.704%
13	19.421	2789	2794	2808	rBV	636802	1293540	5.65%	1.228%
14	19.863	2863	2869	2880	rBV	18353598	22901932	100.00%	21.740%
15	21.098	3075	3079	3090	rBV	305596	586373	2.56%	0.557%
16	21.386	3123	3128	3140	rBV2	4081282	5752664	25.12%	5.461%
17	21.515	3145	3150	3159	rBV	1118262	1830631	7.99%	1.738%
18	23.833	3537	3544	3554	rVB2	2761377	5674903	24.78%	5.387%




Sum of corrected areas: 105342910

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
Data File : BP011823.D
Acq On : 27 Sep 2022 19:30
Operator : CG/JU
Sample : N4839-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
5592-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

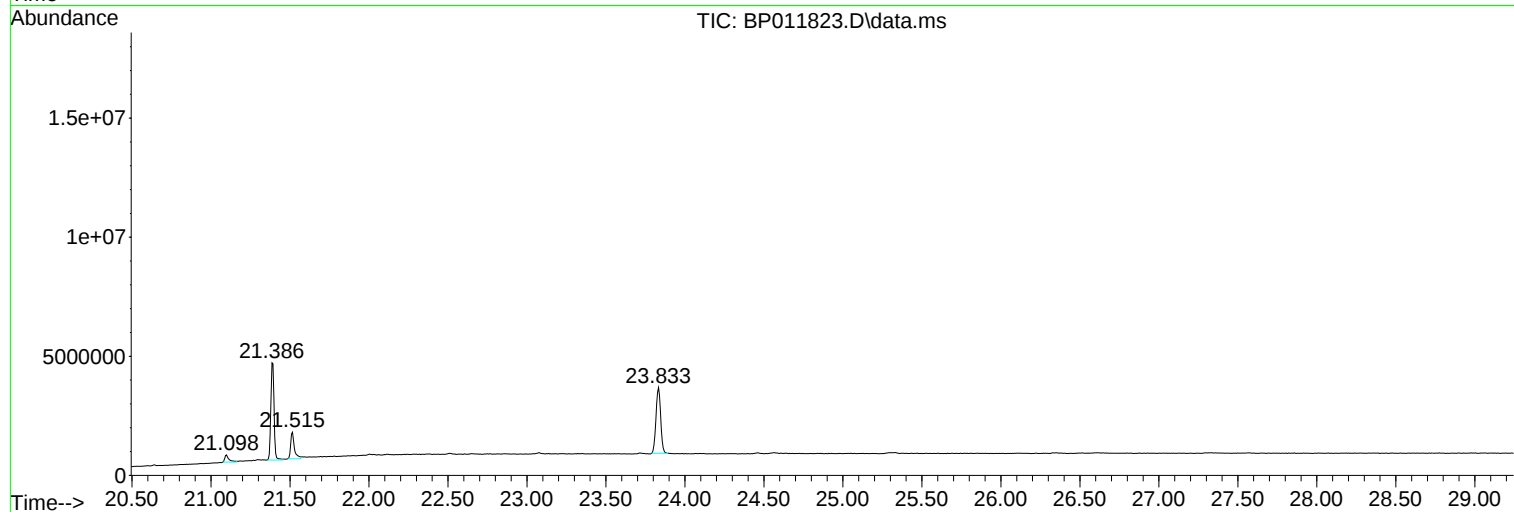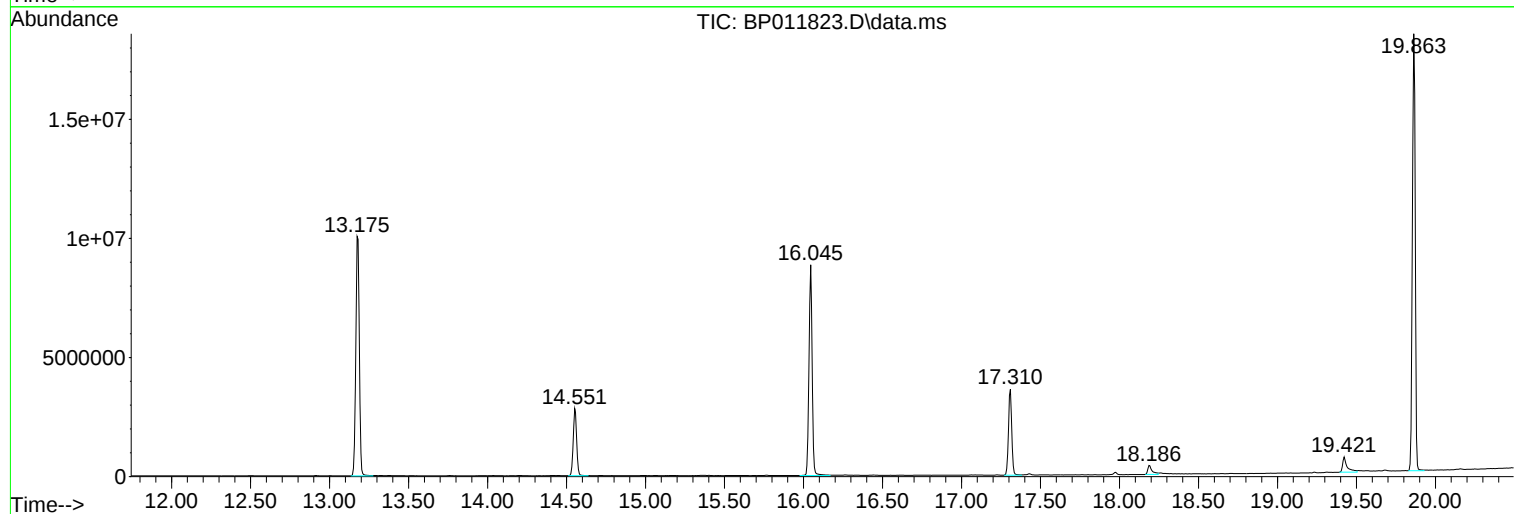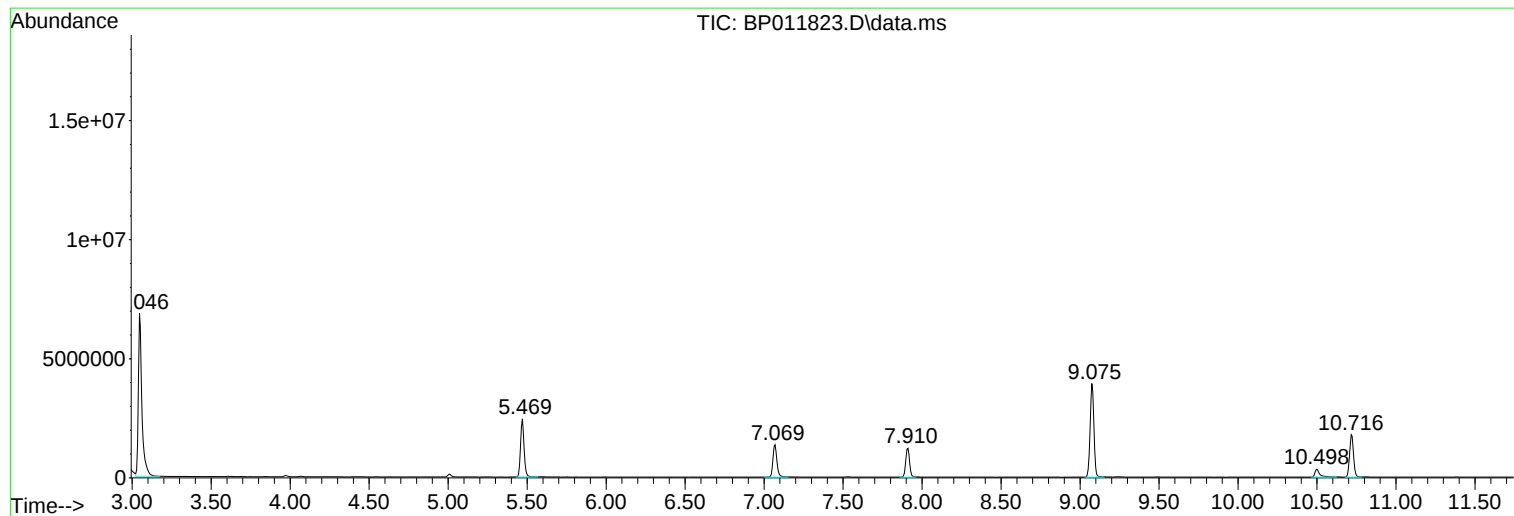

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
Data File : BP011823.D
Acq On : 27 Sep 2022 19:30
Operator : CG/JU
Sample : N4839-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
5592-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
Data File : BP011823.D
Acq On : 27 Sep 2022 19:30
Operator : CG/JU
Sample : N4839-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
5592-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------