


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
 Data File : BP011807.D
 Acq On : 27 Sep 2022 09:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 28 02:03:33 2022

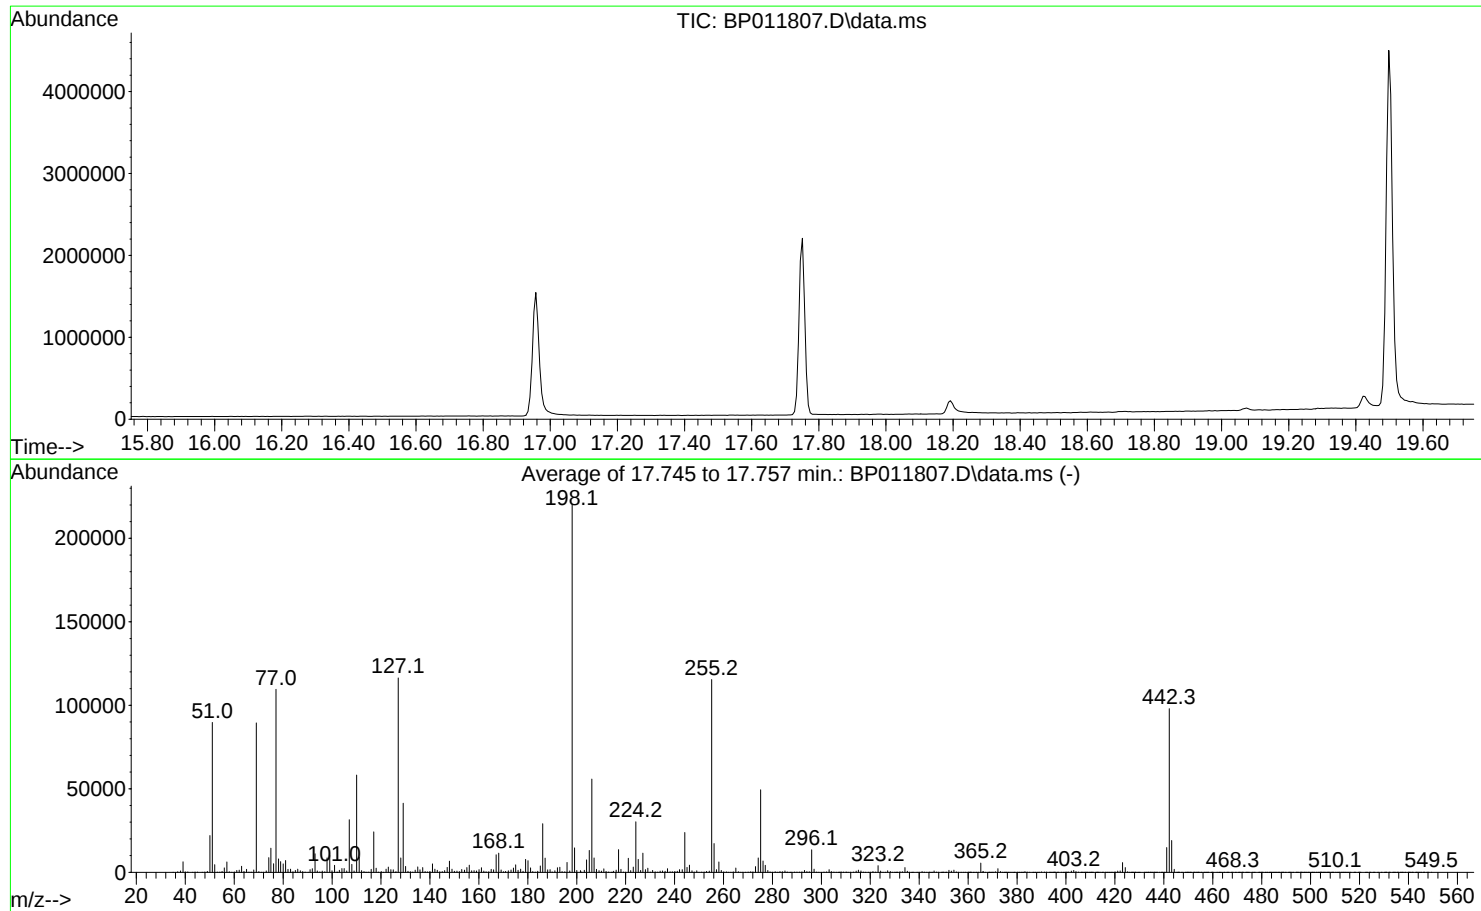




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2500

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	40.7	89757	PASS
68	69	0.00	2	1.6	1447	PASS
69	198	0.00	100	40.6	89409	PASS
70	69	0.00	2	0.5	408	PASS
127	198	10	80	52.8	116355	PASS
197	198	0.00	2	0.4	777	PASS
198	198	100	100	100.0	220309	PASS
199	198	5	9	6.6	14588	PASS
275	198	10	60	22.4	49430	PASS
365	198	1	100	2.5	5472	PASS
441	198	0.01	100	6.7	14841	PASS
442	442	100	100	100.0	98024	PASS
443	442	15	24	19.4	18987	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
 Data File : BP011807.D
 Acq On : 27 Sep 2022 09:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 28 06:56:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:03:33 2022
 Response via : Initial Calibration

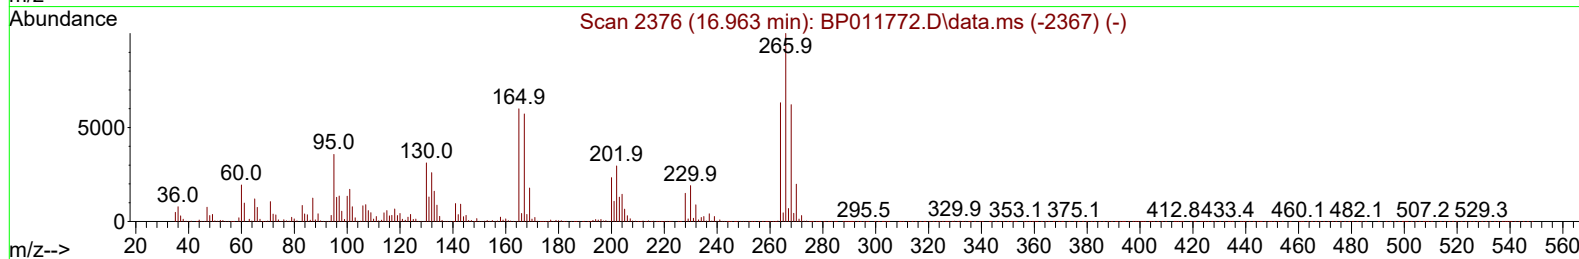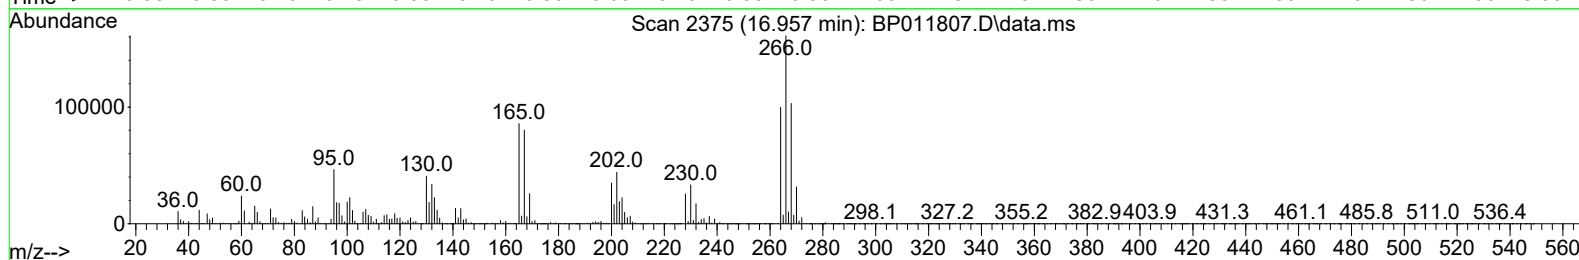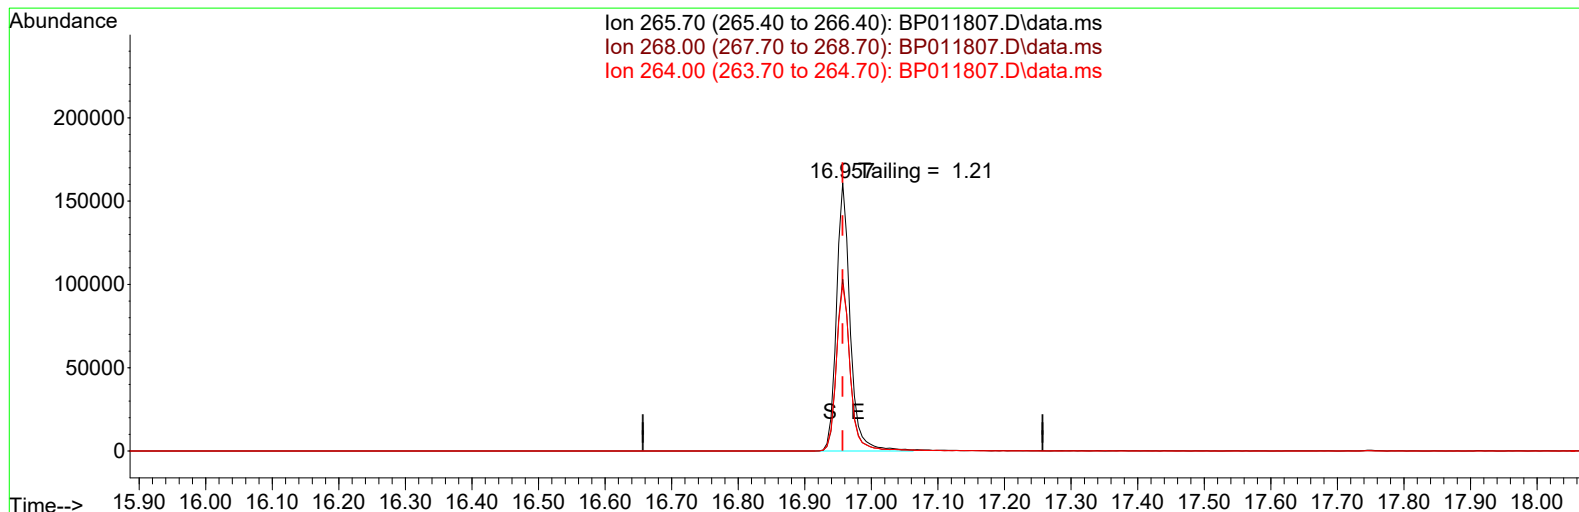

TIC: BP011807.D\data.ms

(70) Pentachlorophenol (C)

16.957min (-0.000) 1331873.36 ng


response 229667

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	63.97
264.00	63.20	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092722\
 Data File : BP011807.D
 Acq On : 27 Sep 2022 09:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 28 06:56:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:03:33 2022
 Response via : Initial Calibration

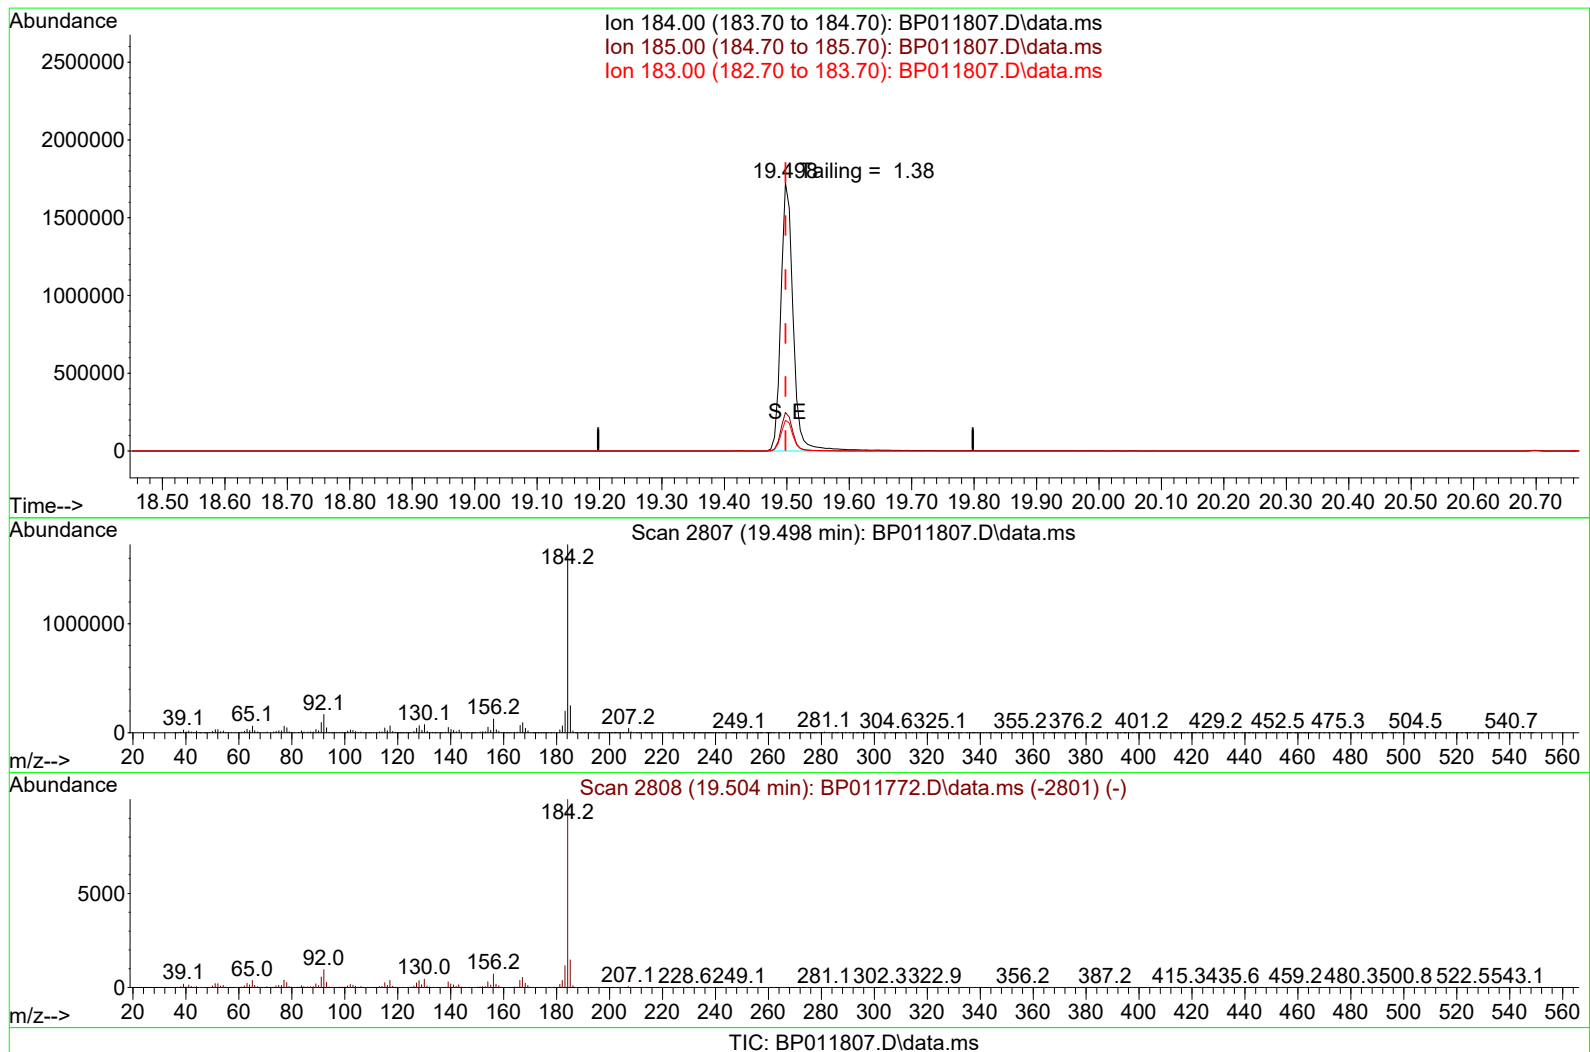

TIC: BP011807.D\data.ms

(77) Benzidine

19.498min (-0.000) 463422.63 ng

response 2383443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.38
183.00	11.60	11.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/27/2022	BNA_P	<u>BP011807.D</u>
Compound Name	Response	Retention Time
DDT	845104	20.698
DDD	5726	20.321
DDE	1410	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7136	852240	0.84

Instrument :
BNA_P
ClientSampleId :
DFTPP