
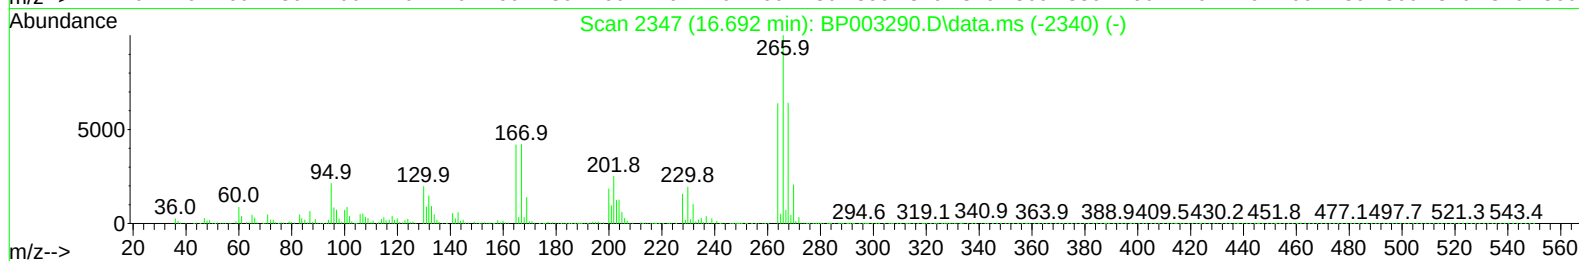
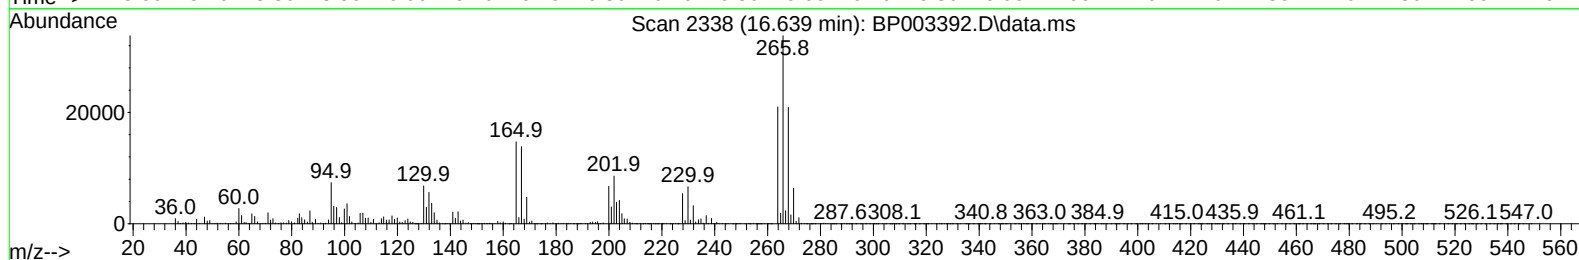


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092820\
 Data File : BP003392.D
 Acq On : 28 Sep 2020 13:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 05:43:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 28 17:55:44 2020
 Response via : Initial Calibration

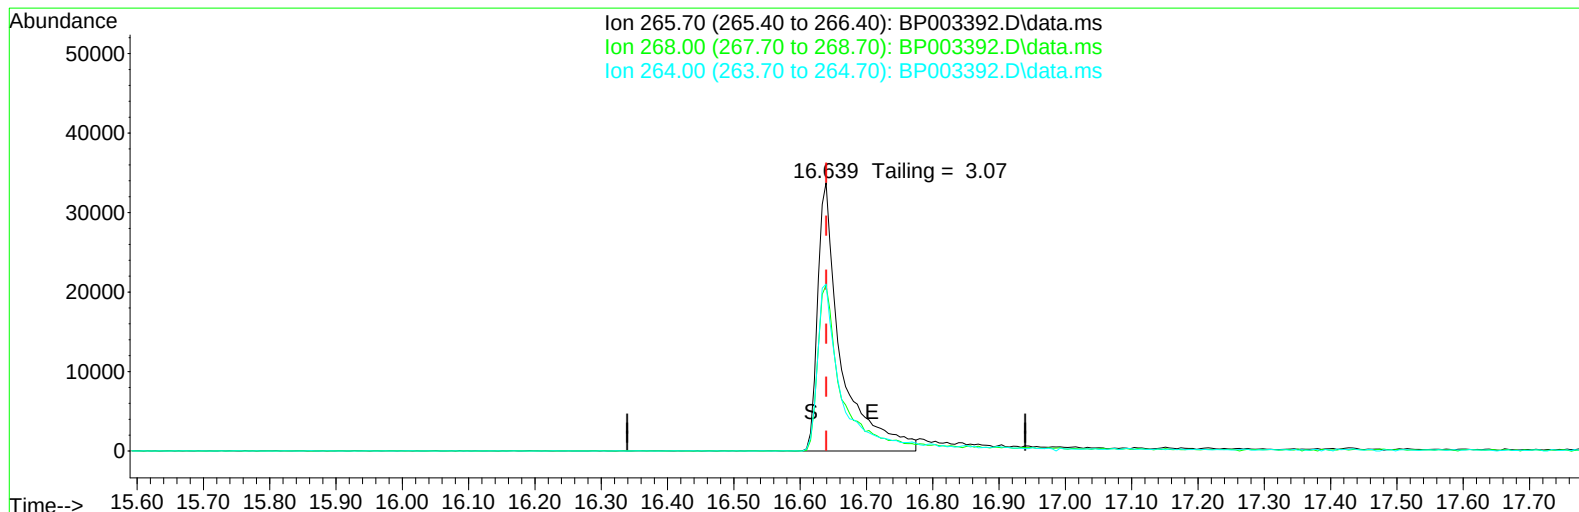

TIC: BP003392.D\data.ms

(70) Pentachlorophenol (C)




16.639min (-0.000) 533046.57 ng

response 82556

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	61.86
264.00	63.30	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092820\
Data File : BP003392.D
Acq On : 28 Sep 2020 13:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 05:43:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 17:55:44 2020
Response via : Initial Calibration

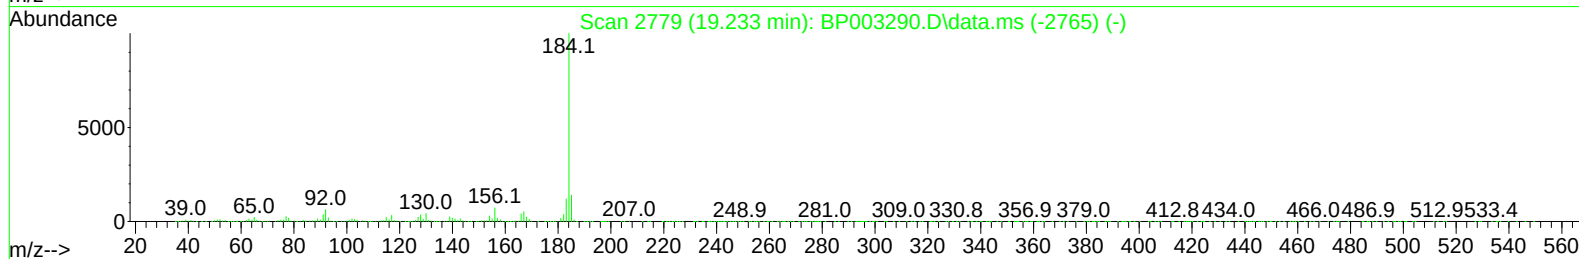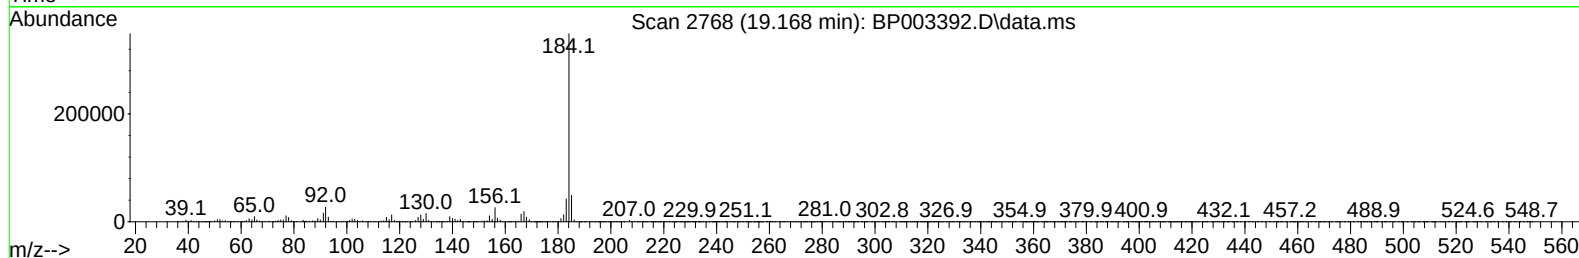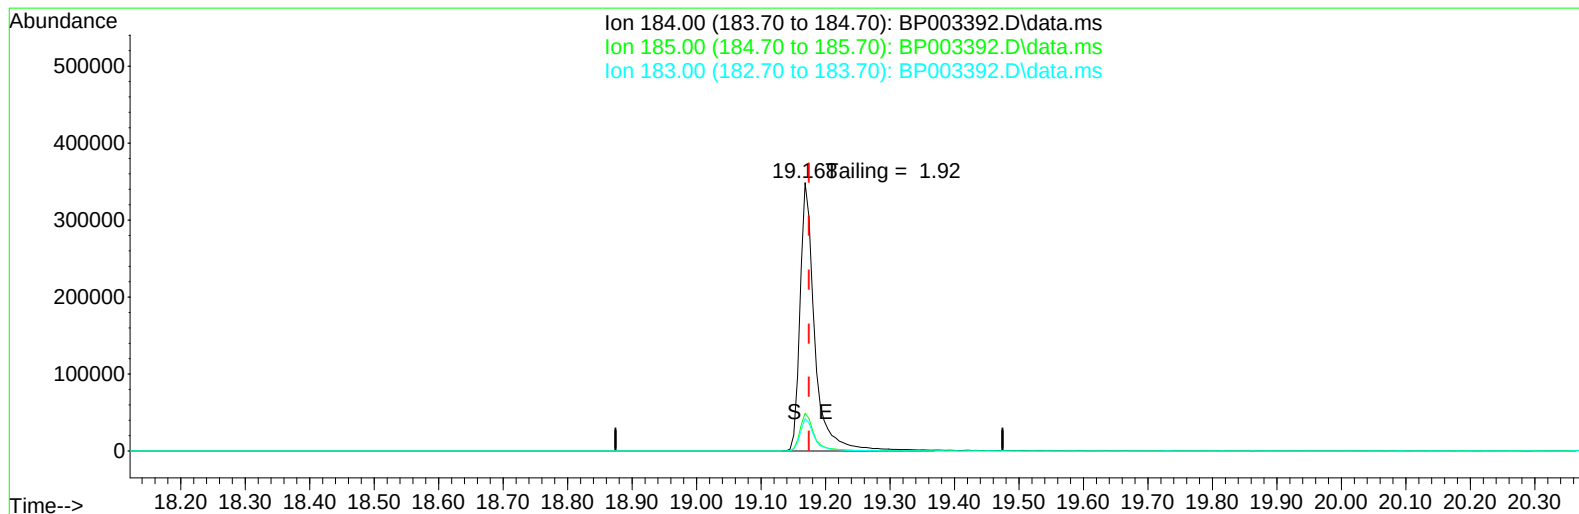

TIC: BP003392.D\data.ms

(77) Benzidine**19.168min (-0.006) 67491.34 ng****response 554599**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.06
183.00	12.00	12.14
0.00	0.00	0.00