


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092820\
 Data File : BP003392.D
 Acq On : 28 Sep 2020 13:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 28 17:55:44 2020

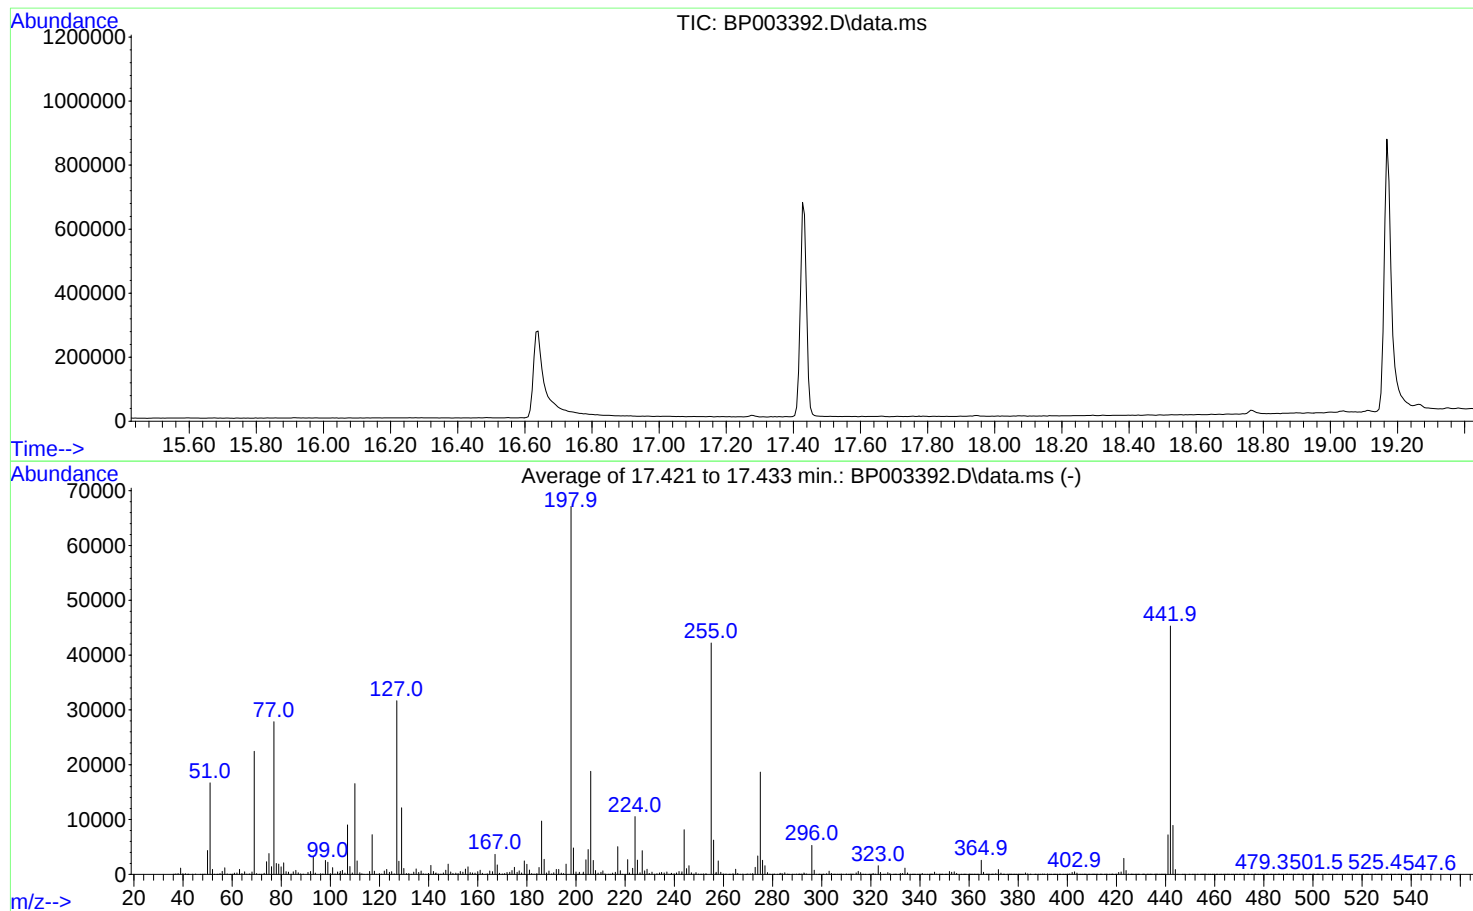

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.9	16703	PASS
68	69	0.00	2	2.0	439	PASS
69	198	0.00	100	33.4	22440	PASS
70	69	0.00	2	0.7	149	PASS
127	198	10	80	47.2	31674	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67115	PASS
199	198	5	9	7.2	4829	PASS
275	198	10	60	27.8	18652	PASS
365	198	1	100	3.8	2572	PASS
441	198	0.01	100	10.7	7212	PASS
442	198	50	100	67.5	45295	PASS
443	442	15	24	19.7	8945	PASS