

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092920\
 Data File : BP003406.D
 Acq On : 29 Sep 2020 19:03
 Operator : CG/JU
 Sample : L4154-08DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 B-5(5-7)DL

Manual Integrations
 APPROVED

mohammad
 10/1/2020 1:30:27 PM

Quant Time: Sep 30 01:19:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 28 17:55:44 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.546	152	74818	20.00	ng	0.00
21) Naphthalene-d8	10.322	136	328082	20.00	ng	# 0.00
39) Acenaphthene-d10	14.198	164	213544	20.00	ng	-0.01
64) Phenanthrene-d10	16.957	188	486806	20.00	ng	# 0.00
76) Chrysene-d12	21.063	240	615939	20.00	ng	-0.01
86) Perylene-d12	23.257	264	759168	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.163	112	79441	18.54	ng	0.00
7) Phenol-d6	6.752	99	105853	18.53	ng	0.00
23) Nitrobenzene-d5	8.699	82	70267	12.58	ng	0.00
42) 2,4,6-Tribromophenol	15.704	330	40006	12.28	ng	0.00
45) 2-Fluorobiphenyl	12.816	172	160486	10.99	ng	0.00
79) Terphenyl-d14	19.539	244	291339	9.86	ng	-0.01
Target Compounds						Qvalue
49) Acenaphthylene	13.922	152	74560	3.70	ng	98
52) Acenaphthene	14.263	154	34019	2.77	ng	98
58) Fluorene	15.257	166	49423	3.20	ng	98
71) Phenanthrene	16.998	178	807053	30.47	ng	100
72) Anthracene	17.092	178	219481	8.41	ng	99
73) Carbazole	17.369	167	88834	3.58	ng	100
75) Fluoranthene	18.986	202	1395860	41.91	ng	99
78) Pyrene	19.339	202	1241316	32.32	ng	100
81) Benzo(a)anthracene	21.045	228	783955	19.69	ng	99
83) Chrysene	21.098	228	657826	17.20	ng	98
87) Indeno(1,2,3-cd)pyrene	25.474	276	506744	8.81	ng	95
88) Benzo(b)fluoranthene	22.598	252	1045752m	21.81	ng	
89) Benzo(k)fluoranthene	22.633	252	313924m	6.83	ng	
90) Benzo(a)pyrene	23.157	252	783002	17.32	ng	97
91) Dibenzo(a,h)anthracene	25.468	278	137808m	2.90	ng	
92) Benzo(g,h,i)perylene	26.156	276	463726	9.78	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092920\
Data File : BP003406.D
Acq On : 29 Sep 2020 19:03
Operator : CG/JU
Sample : L4154-08DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-5(5-7)DL

Manual Integrations
APPROVED

mohammad
10/1/2020 1:30:27 PM

Quant Time: Sep 30 01:19:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 17:55:44 2020
Response via : Initial Calibration

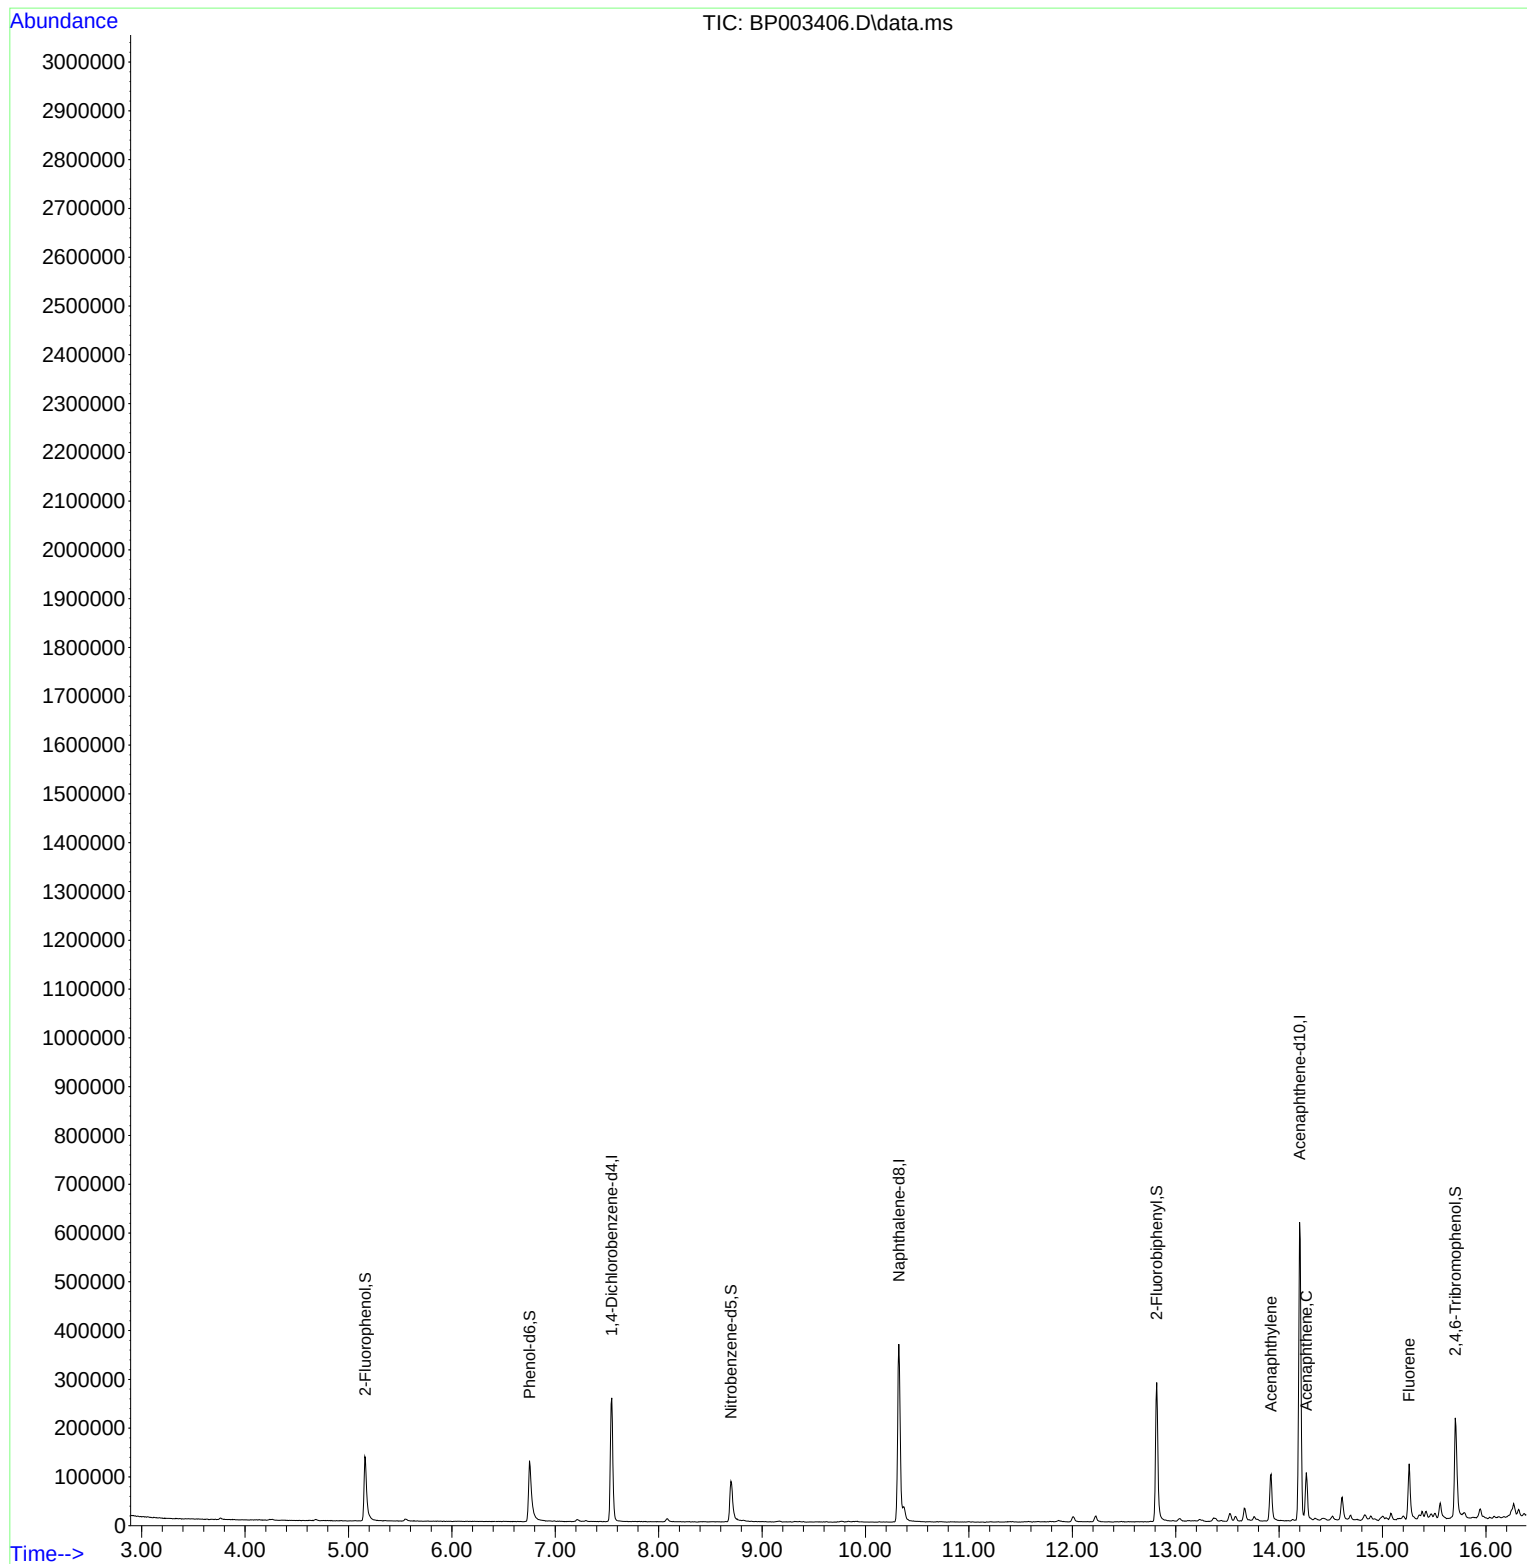

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092920\
Data File : BP003406.D
Acq On : 29 Sep 2020 19:03
Operator : CG/JU
Sample : L4154-08DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-5(5-7)DL

Manual Integrations
APPROVED

mohammad
10/1/2020 1:30:27 PM

Quant Time: Sep 30 01:19:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 17:55:44 2020
Response via : Initial Calibration

