
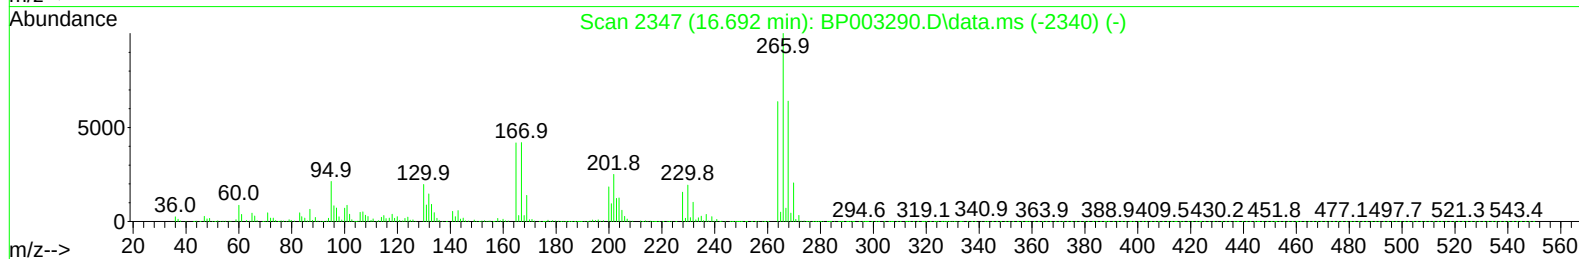
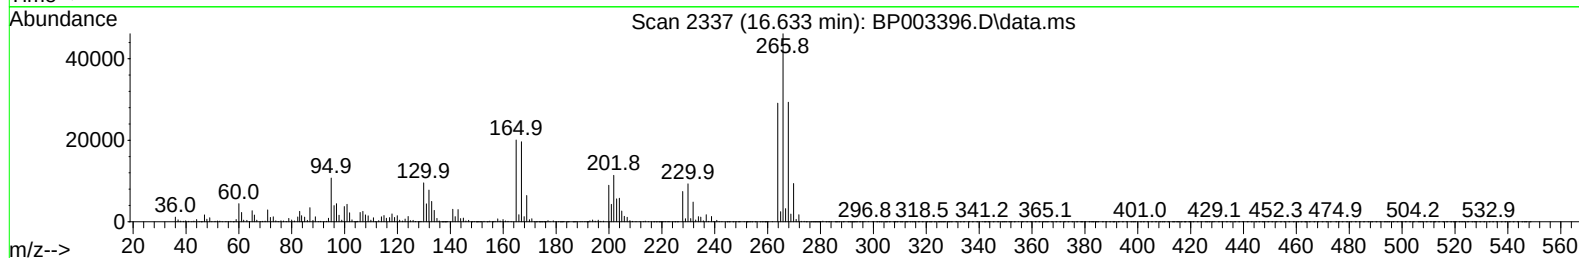


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092920\
Data File : BP003396.D
Acq On : 29 Sep 2020 12:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 05:37:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 17:55:44 2020
Response via : Initial Calibration

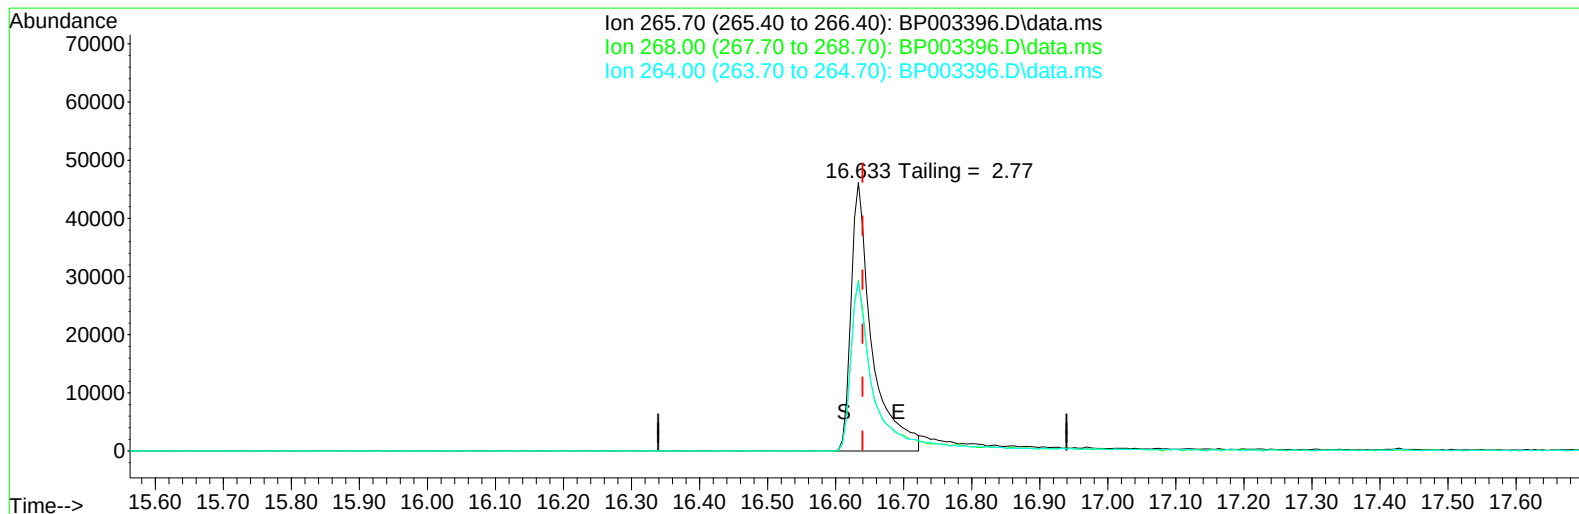

TIC: BP003396.D\data.ms

(70) Pentachlorophenol (C)




16.633min (-0.006) 751207.18 ng

response 91052

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.61
264.00	63.30	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092920\
Data File : BP003396.D
Acq On : 29 Sep 2020 12:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 05:37:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 17:55:44 2020
Response via : Initial Calibration

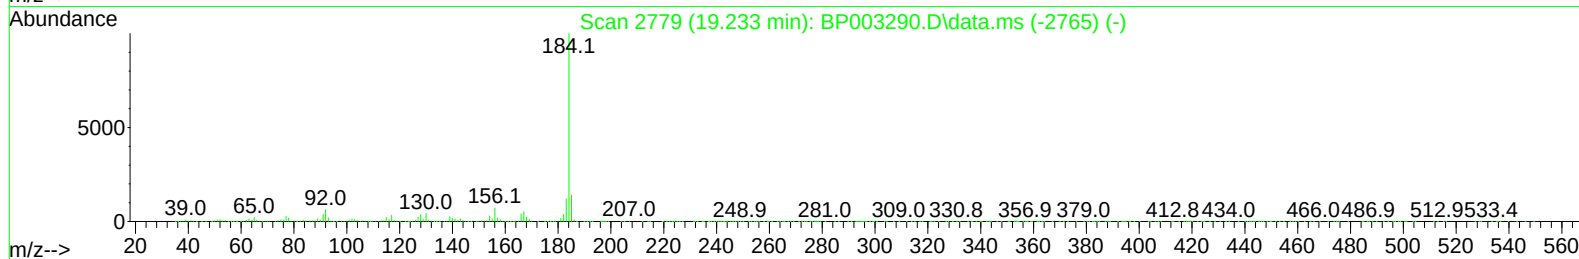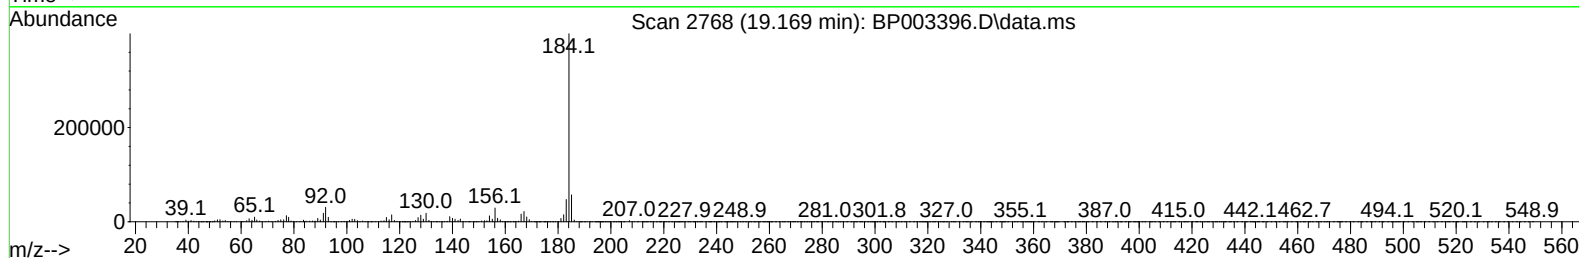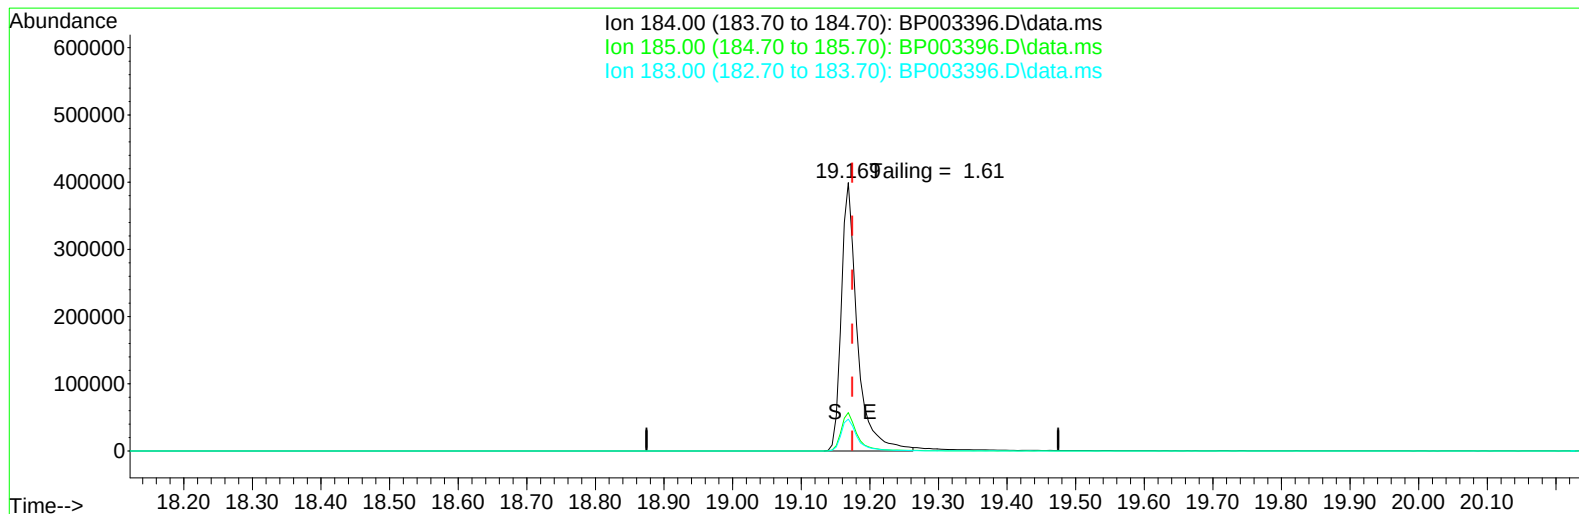

TIC: BP003396.D\data.ms

(77) Benzidine

19.169min (-0.006) 409806.70 ng m

response 635381

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.33
183.00	12.00	11.86
0.00	0.00	0.00