
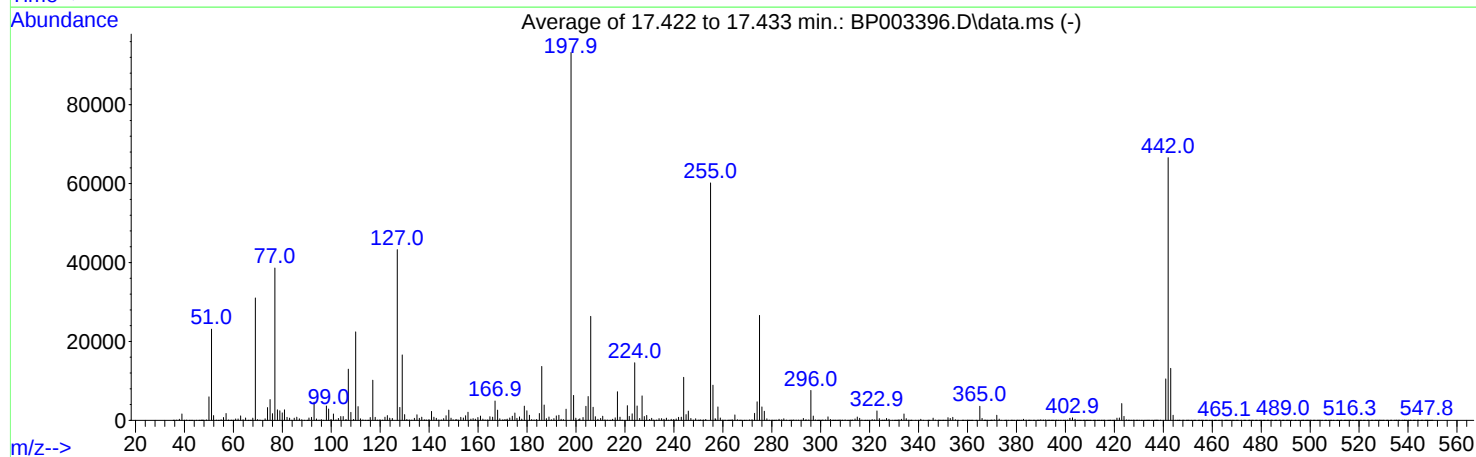


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092920\
 Data File : BP003396.D
 Acq On : 29 Sep 2020 12:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 28 17:55:44 2020

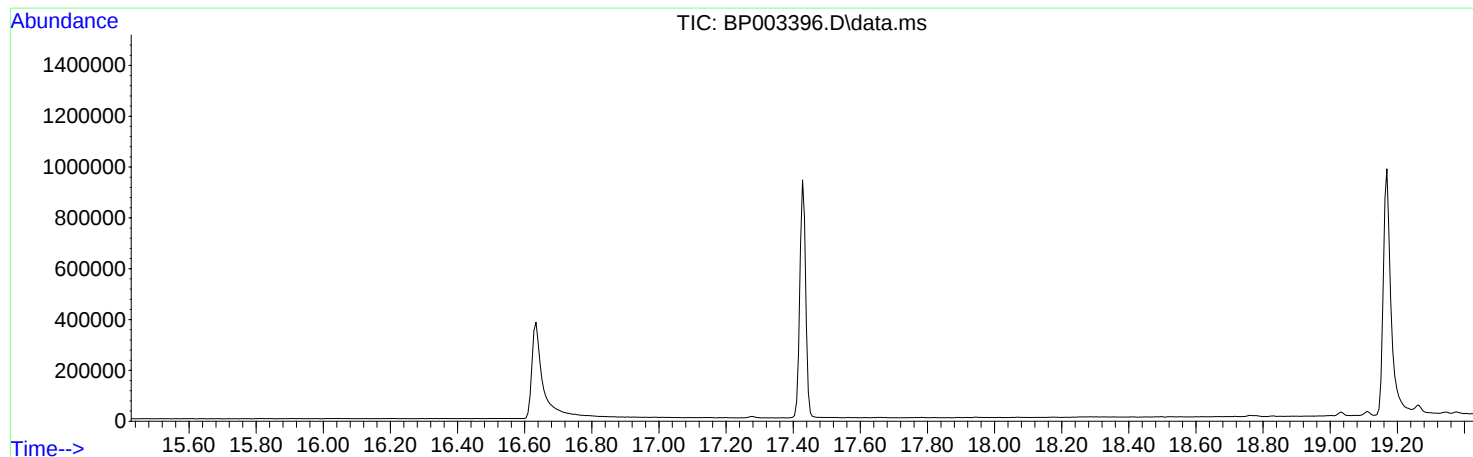

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.8	23107	PASS
68	69	0.00	2	1.8	562	PASS
69	198	0.00	100	33.3	31024	PASS
70	69	0.00	2	0.6	192	PASS
127	198	10	80	46.4	43272	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93229	PASS
199	198	5	9	6.8	6323	PASS
275	198	10	60	28.6	26623	PASS
365	198	1	100	3.8	3578	PASS
441	198	0.01	100	11.3	10501	PASS
442	198	50	100	71.4	66587	PASS
443	442	15	24	19.8	13195	PASS