
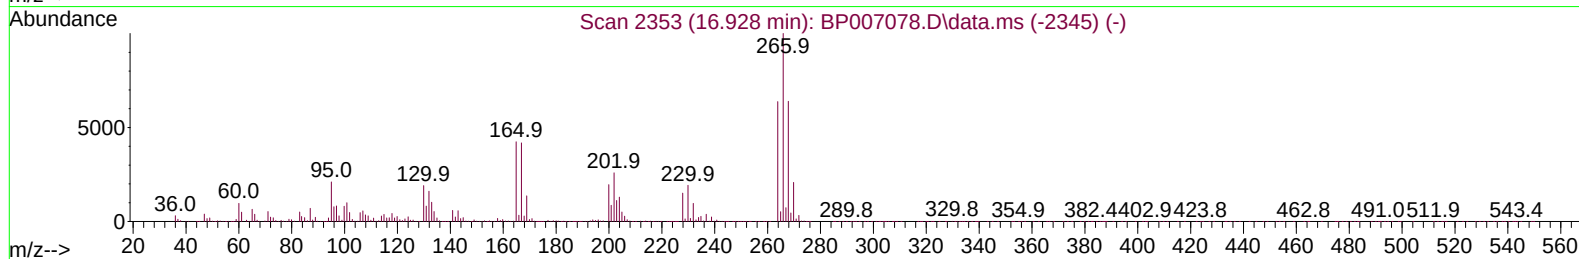
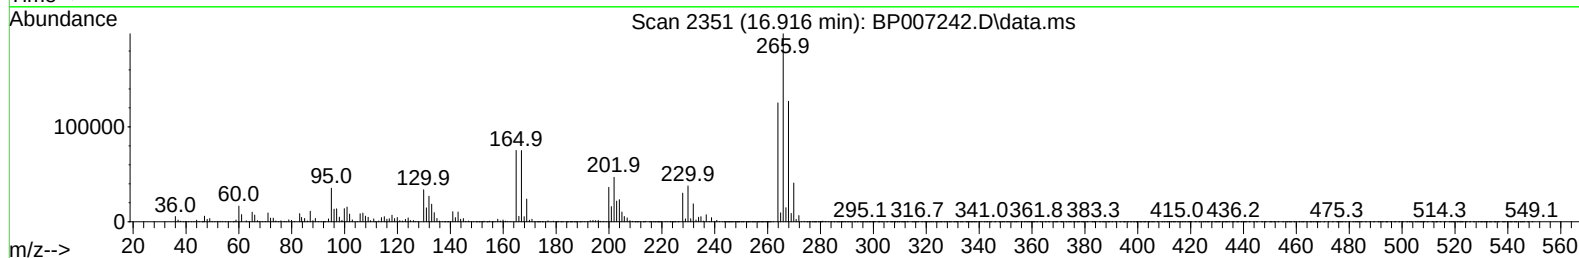


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092921\
Data File : BP007242.D
Acq On : 29 Sep 2021 12:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 14:42:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 23 11:17:25 2021
Response via : Initial Calibration

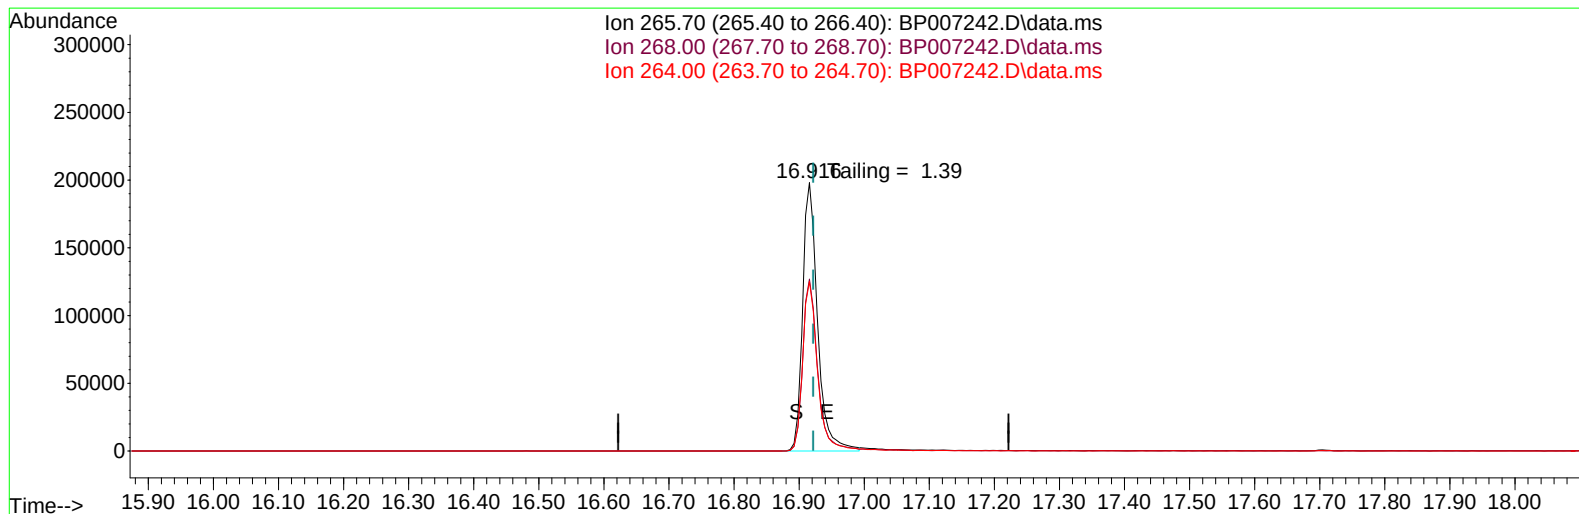

TIC: BP007242.D\data.ms

(70) Pentachlorophenol (C)




16.916min (-0.006) 425260.32 ng

response 323094

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.09
264.00	62.90	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092921\
 Data File : BP007242.D
 Acq On : 29 Sep 2021 12:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 14:42:36 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

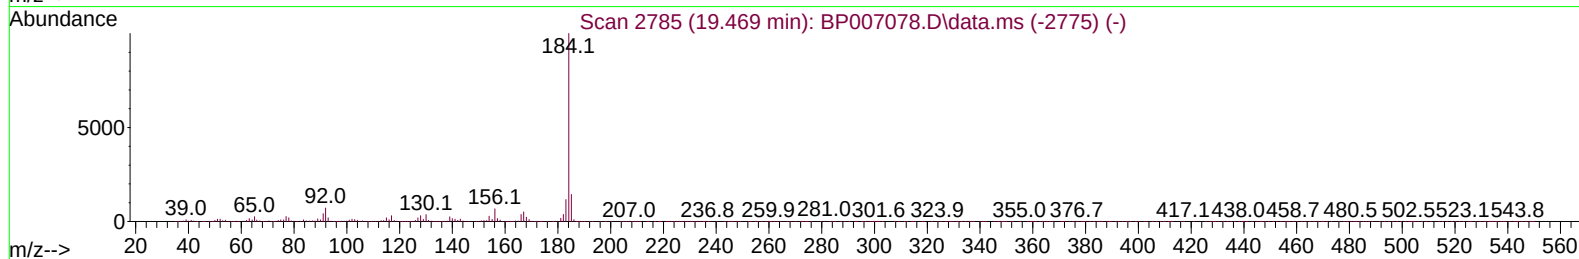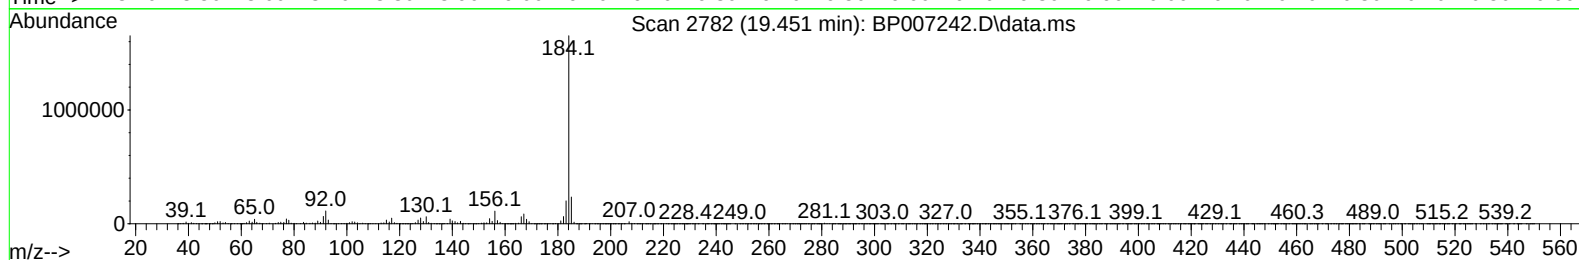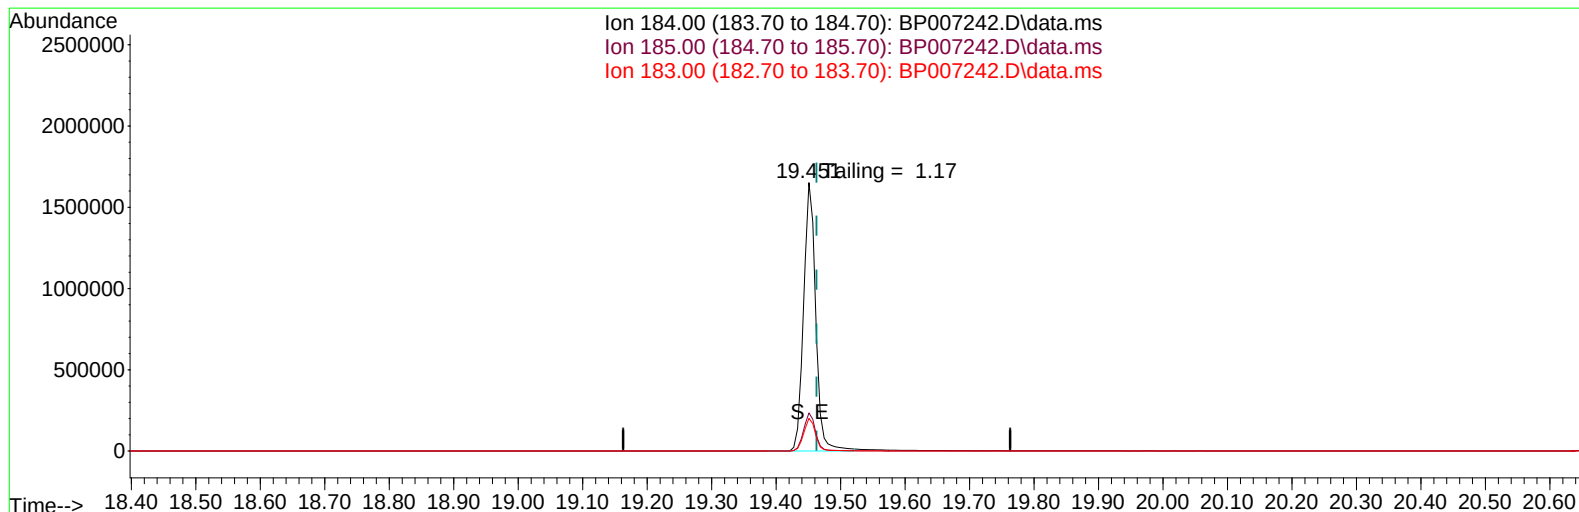

TIC: BP007242.D\data.ms

(77) Benzidine

19.451min (-0.012) 2972951.78 ng

response 2192723

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.22
183.00	11.90	12.18
0.00	0.00	0.00