

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP092921\  
 Data File : BP007244.D  
 Acq On : 29 Sep 2021 14:02  
 Operator : CG/JU  
 Sample : PB139459BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 PB139459BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP092121.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007244.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.452       | 396           | 402         | 416          | rBV      | 2919962        | 4336311       | 38.08%          | 9.287%        |
| 2         | 7.052       | 666           | 674         | 696          | rBV      | 3195415        | 5204697       | 45.70%          | 11.147%       |
| 3         | 7.875       | 807           | 814         | 823          | rBV      | 577248         | 879084        | 7.72%           | 1.883%        |
| 4         | 9.040       | 1003          | 1012        | 1035         | rBV      | 1643946        | 2807087       | 24.65%          | 6.012%        |
| 5         | 10.675      | 1280          | 1290        | 1310         | rBV      | 658700         | 1165756       | 10.24%          | 2.497%        |
| 6         | 13.134      | 1700          | 1708        | 1725         | rBV      | 4493241        | 6824511       | 59.92%          | 14.616%       |
| 7         | 14.510      | 1934          | 1942        | 1954         | rBV      | 1194682        | 1820190       | 15.98%          | 3.898%        |
| 8         | 16.004      | 2188          | 2196        | 2221         | rBV      | 3561926        | 5596611       | 49.14%          | 11.986%       |
| 9         | 17.263      | 2403          | 2410        | 2423         | rBV      | 1326192        | 1986176       | 17.44%          | 4.254%        |
| 10        | 19.822      | 2839          | 2845        | 2854         | rBV      | 9542744        | 11388569      | 100.00%         | 24.390%       |
| 11        | 21.351      | 3100          | 3105        | 3111         | rBV      | 1735131        | 2300659       | 20.20%          | 4.927%        |
| 12        | 23.763      | 3509          | 3515        | 3524         | rVB2     | 1141868        | 2383783       | 20.93%          | 5.105%        |




Sum of corrected areas: 46693434

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP092921\  
Data File : BP007244.D  
Acq On : 29 Sep 2021 14:02  
Operator : CG/JU  
Sample : PB139459BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB139459BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP092121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

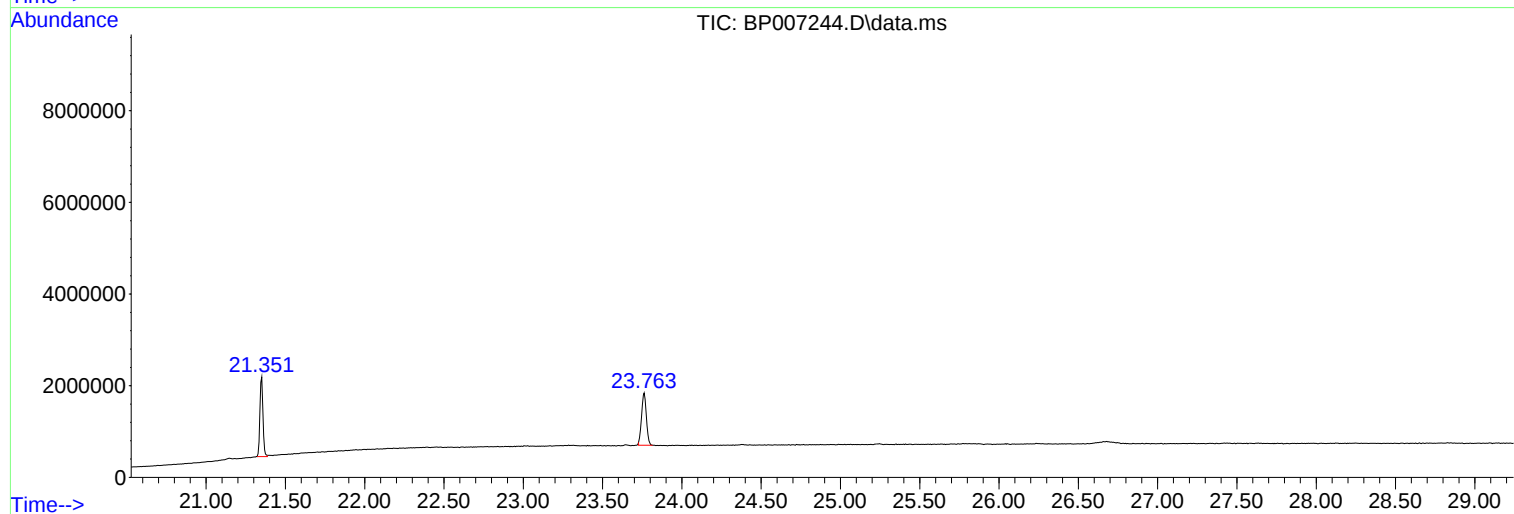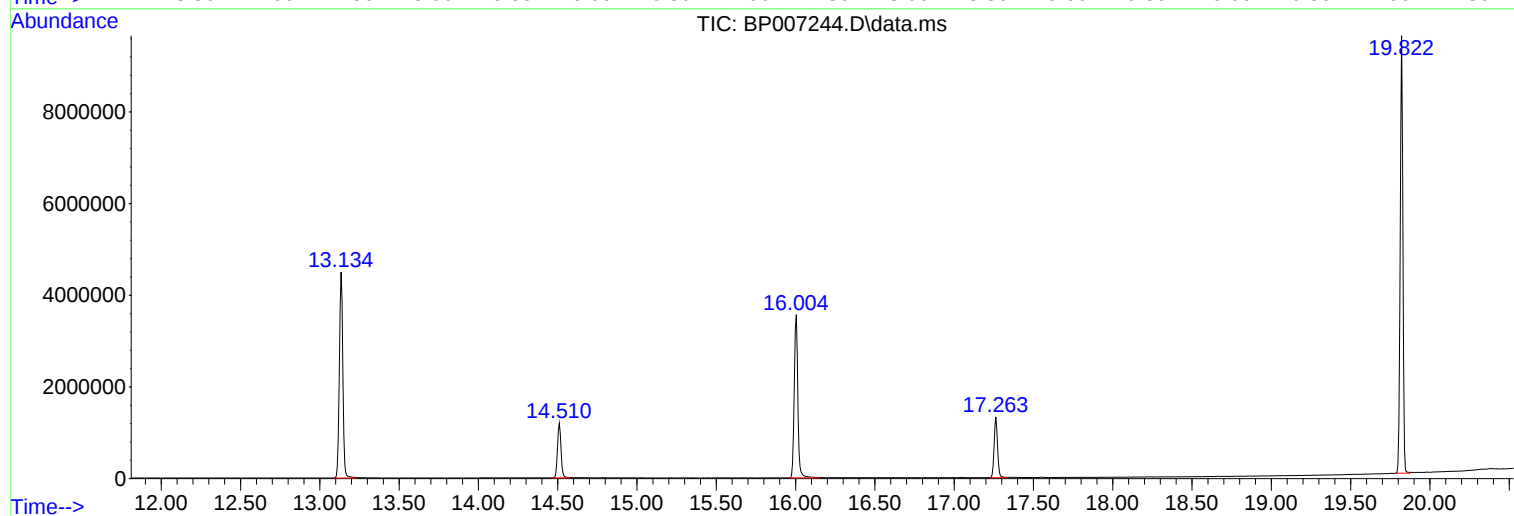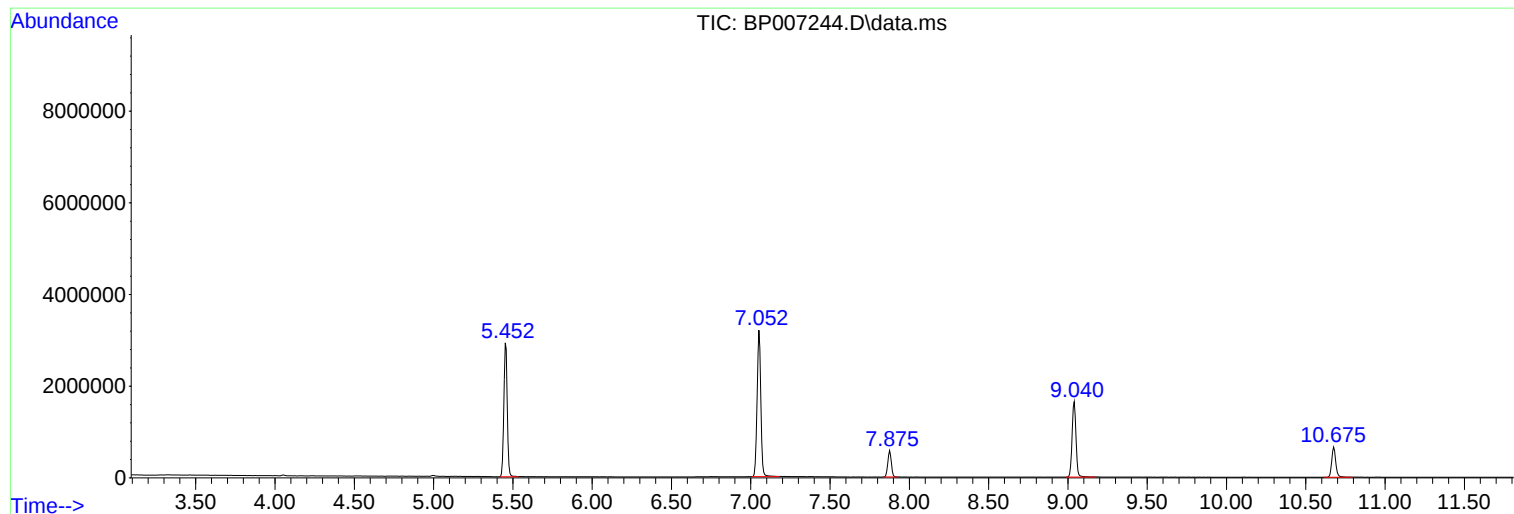

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP092921\  
Data File : BP007244.D  
Acq On : 29 Sep 2021 14:02  
Operator : CG/JU  
Sample : PB139459BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB139459BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP092121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP092921\  
Data File : BP007244.D  
Acq On : 29 Sep 2021 14:02  
Operator : CG/JU  
Sample : PB139459BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB139459BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP092121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|