
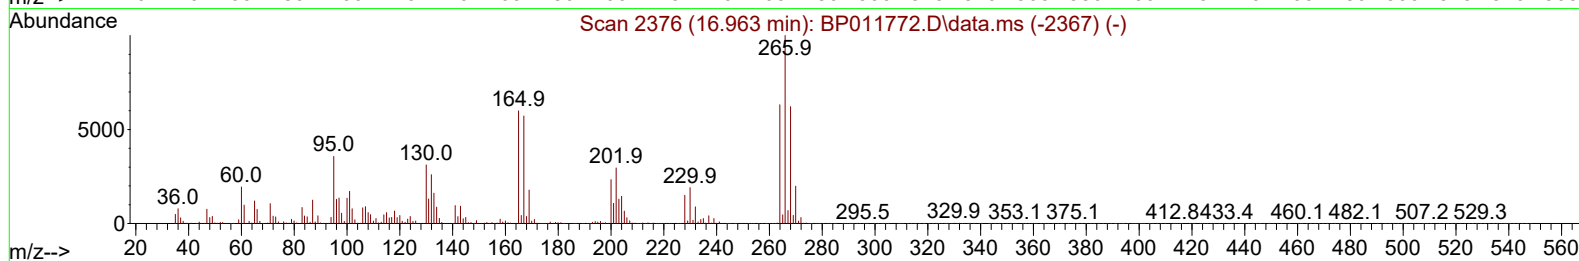
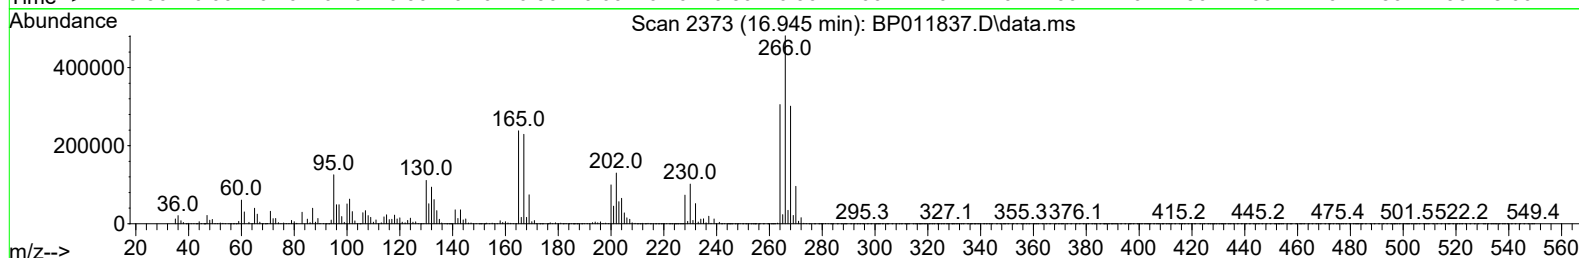


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092922\
Data File : BP011837.D
Acq On : 29 Sep 2022 09:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 05:07:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:03:33 2022
Response via : Initial Calibration

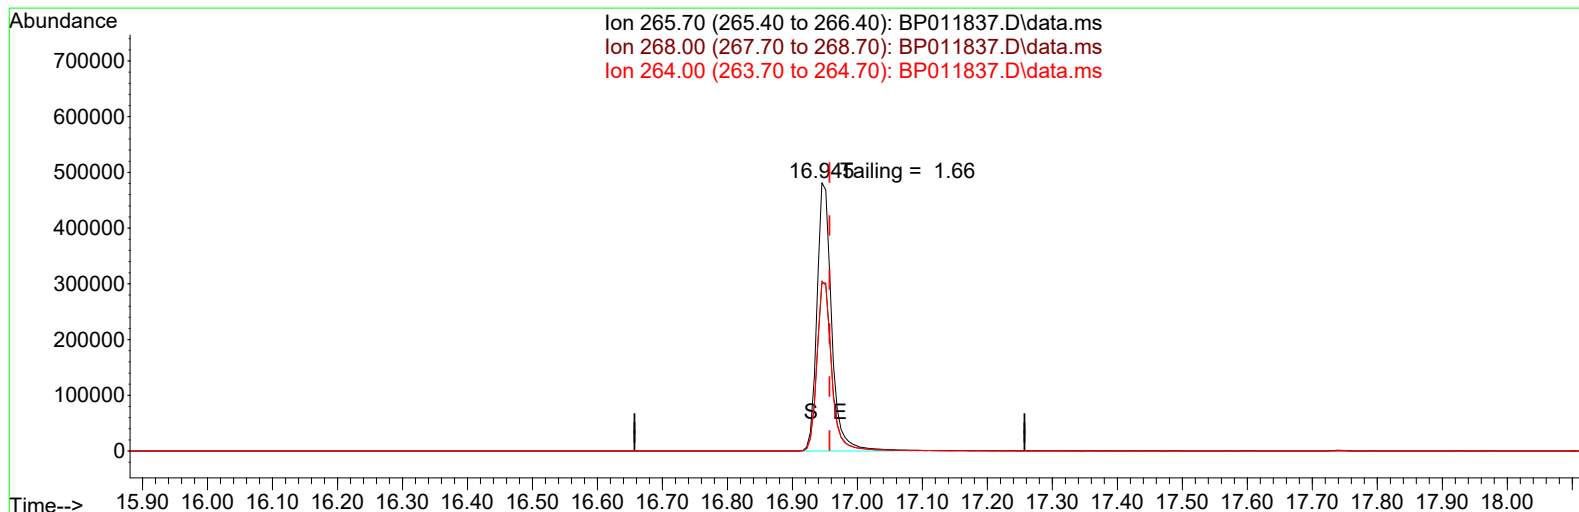

TIC: BP011837.D\data.ms

(70) Pentachlorophenol (C)




16.945min (-0.012) 5469267.93 ng

response 761749

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	62.53
264.00	63.20	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092922\
Data File : BP011837.D
Acq On : 29 Sep 2022 09:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 05:07:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:03:33 2022
Response via : Initial Calibration

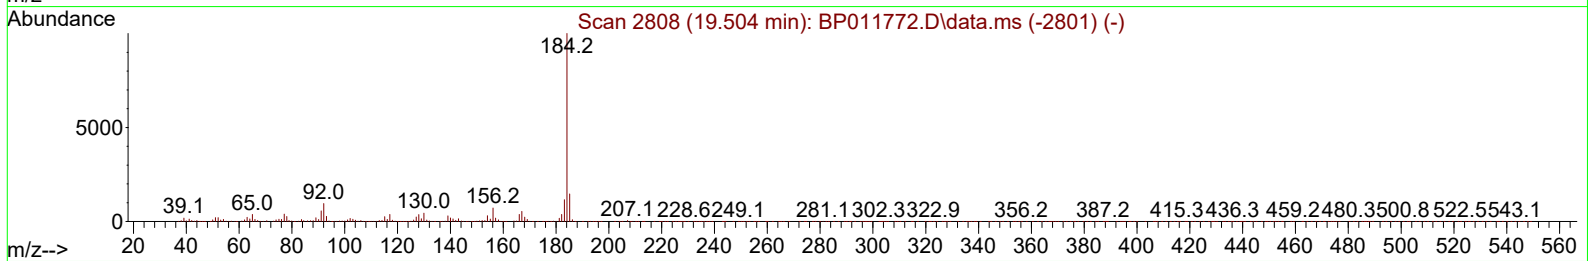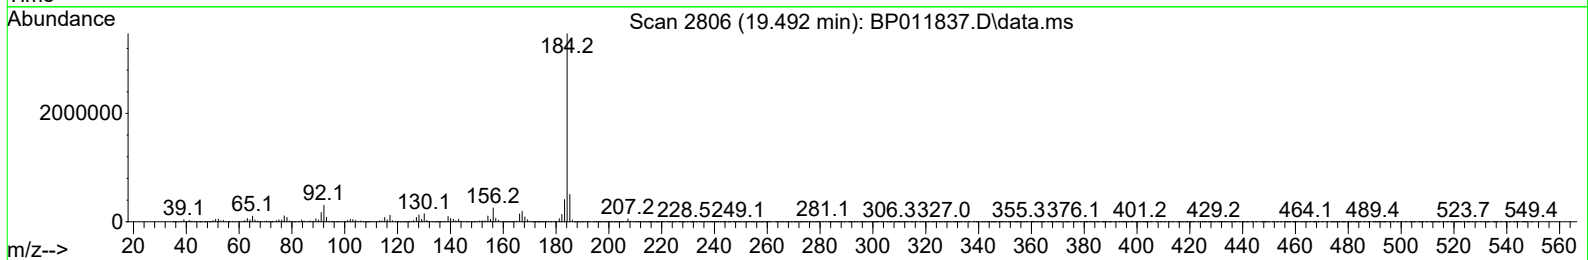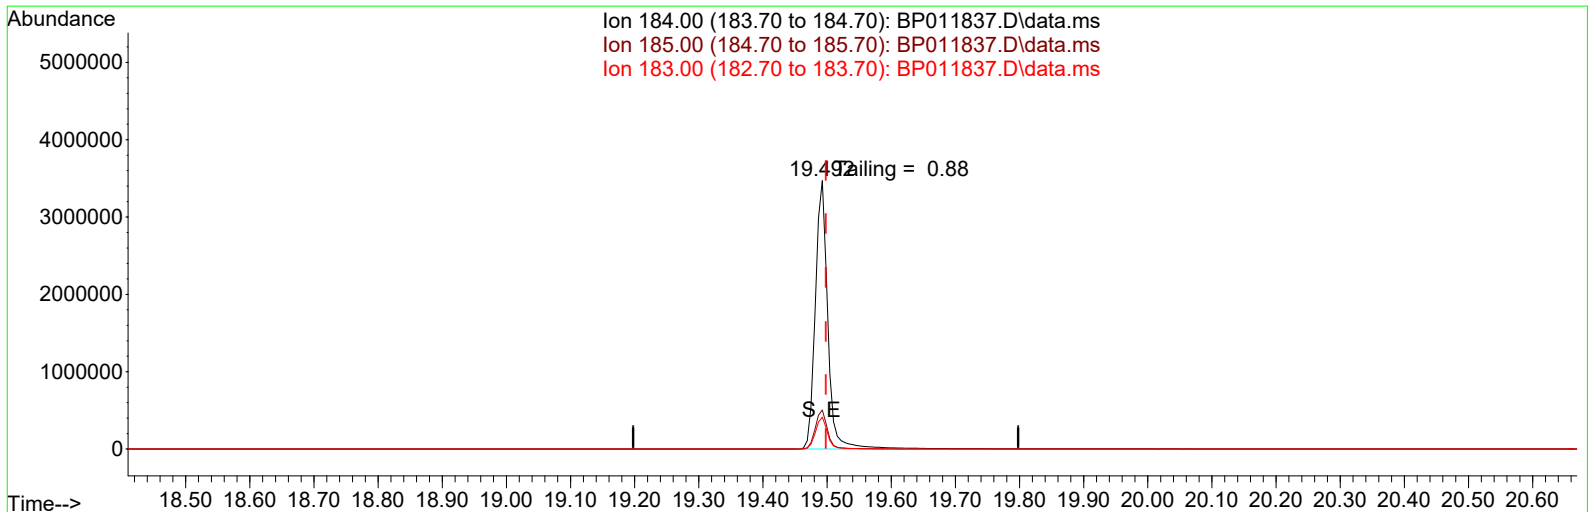

TIC: BP011837.D\data.ms

(77) Benzidine**19.492min (-0.006) 3426582.12 ng****response 4721730**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.54
183.00	11.60	11.86
0.00	0.00	0.00