


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092922\
 Data File : BP011837.D
 Acq On : 29 Sep 2022 09:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 28 02:03:33 2022

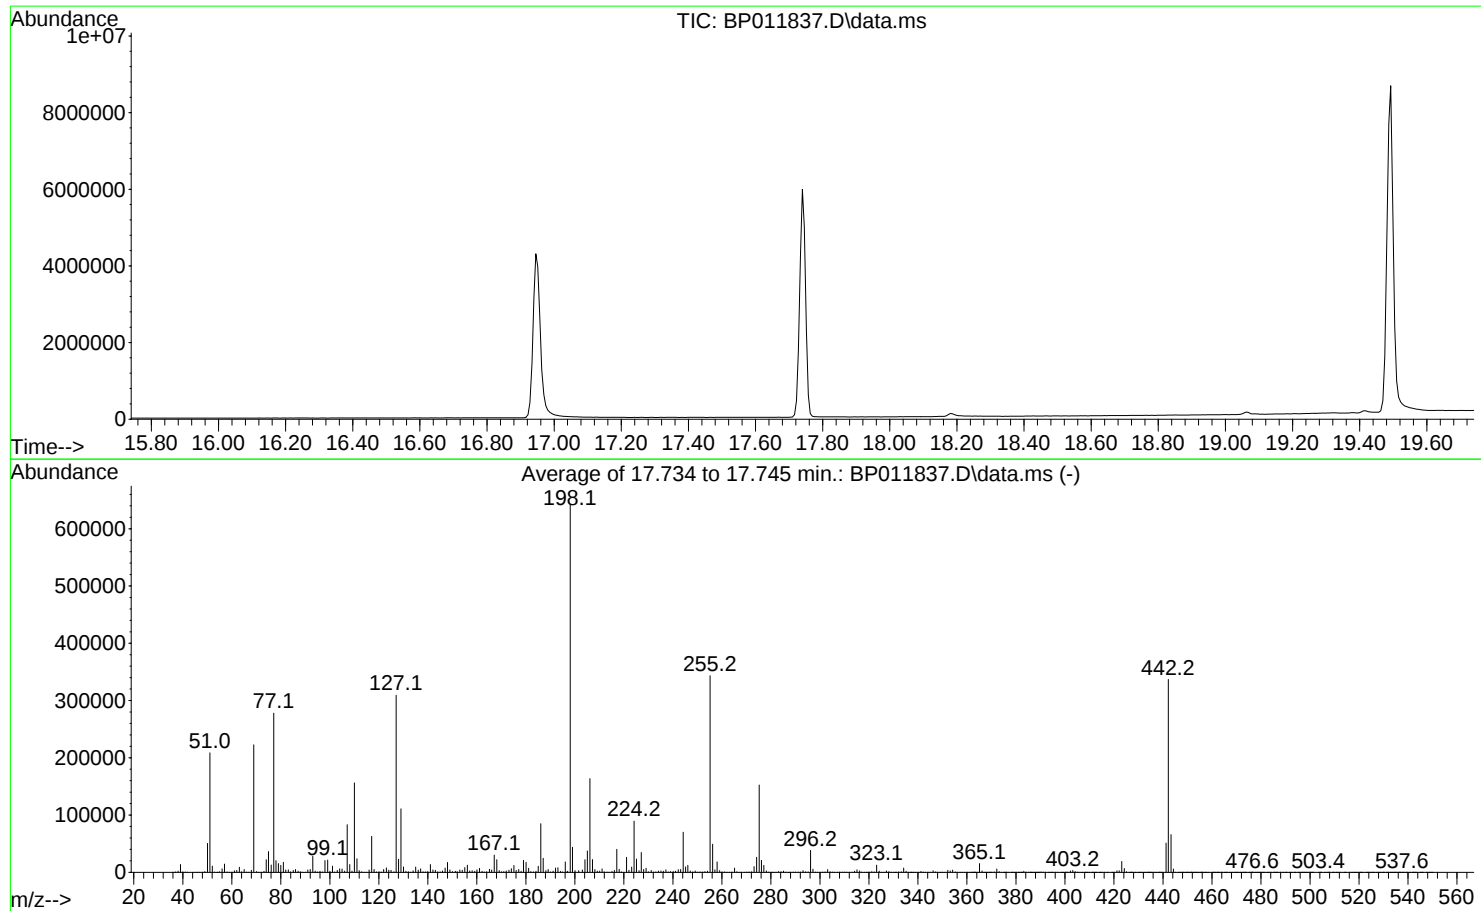


AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	208581	PASS
68	69	0.00	2	1.6	3587	PASS
69	198	0.00	100	34.6	222514	PASS
70	69	0.00	2	0.5	1202	PASS
127	198	10	80	48.1	309321	PASS
197	198	0.00	2	0.3	1842	PASS
198	198	100	100	100.0	642512	PASS
199	198	5	9	6.8	43810	PASS
275	198	10	60	23.7	152582	PASS
365	198	1	100	2.4	15318	PASS
441	198	0.01	100	7.9	50925	PASS
442	442	100	100	100.0	336807	PASS
443	442	15	24	19.5	65763	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092922\
 Data File : BP011837.D
 Acq On : 29 Sep 2022 09:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 30 05:07:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:03:33 2022
 Response via : Initial Calibration

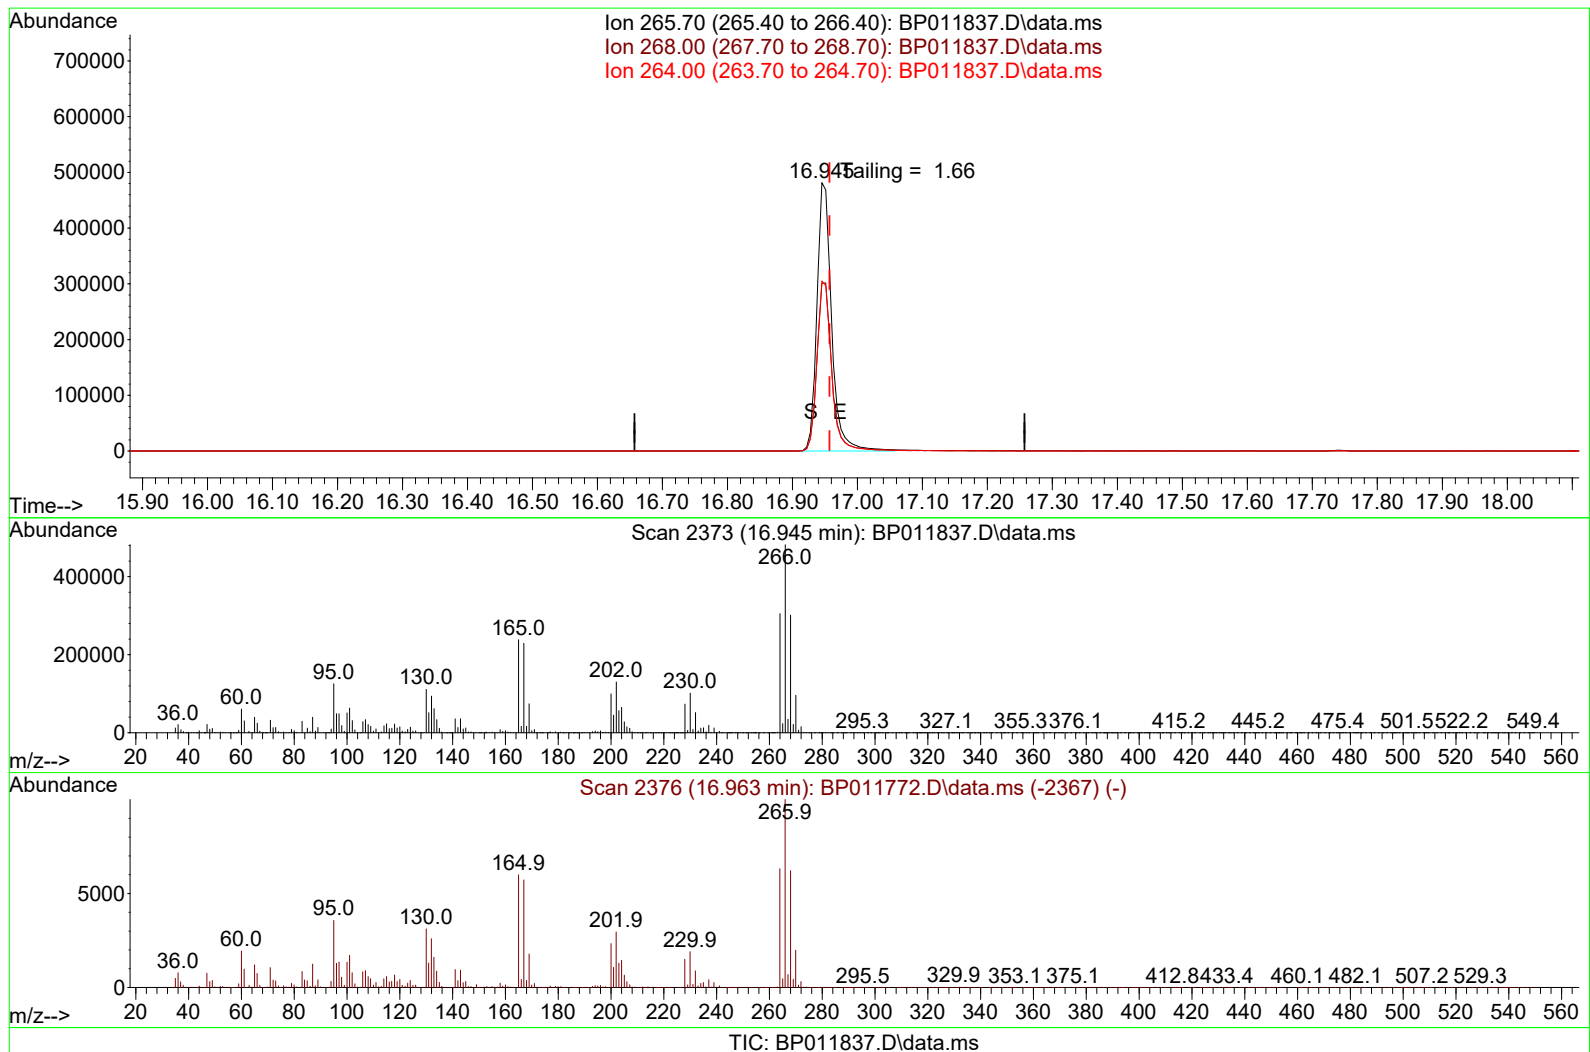

TIC: BP011837.D\data.ms

(70) Pentachlorophenol (C)

16.945min (-0.012) 5469267.93 ng




response 761749

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	62.53
264.00	63.20	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092922\
Data File : BP011837.D
Acq On : 29 Sep 2022 09:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 30 05:07:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:03:33 2022
Response via : Initial Calibration

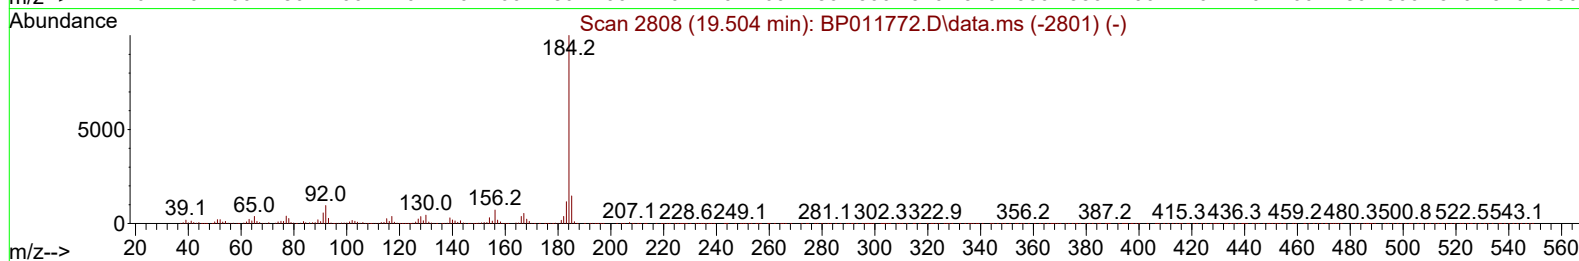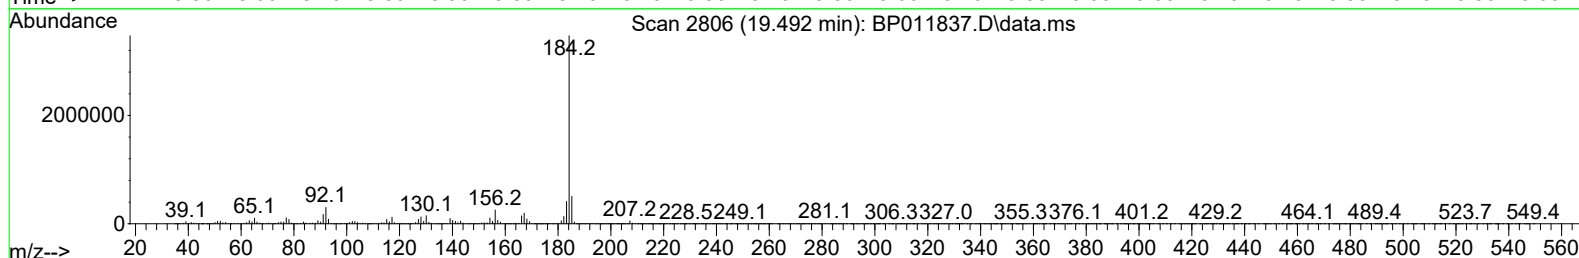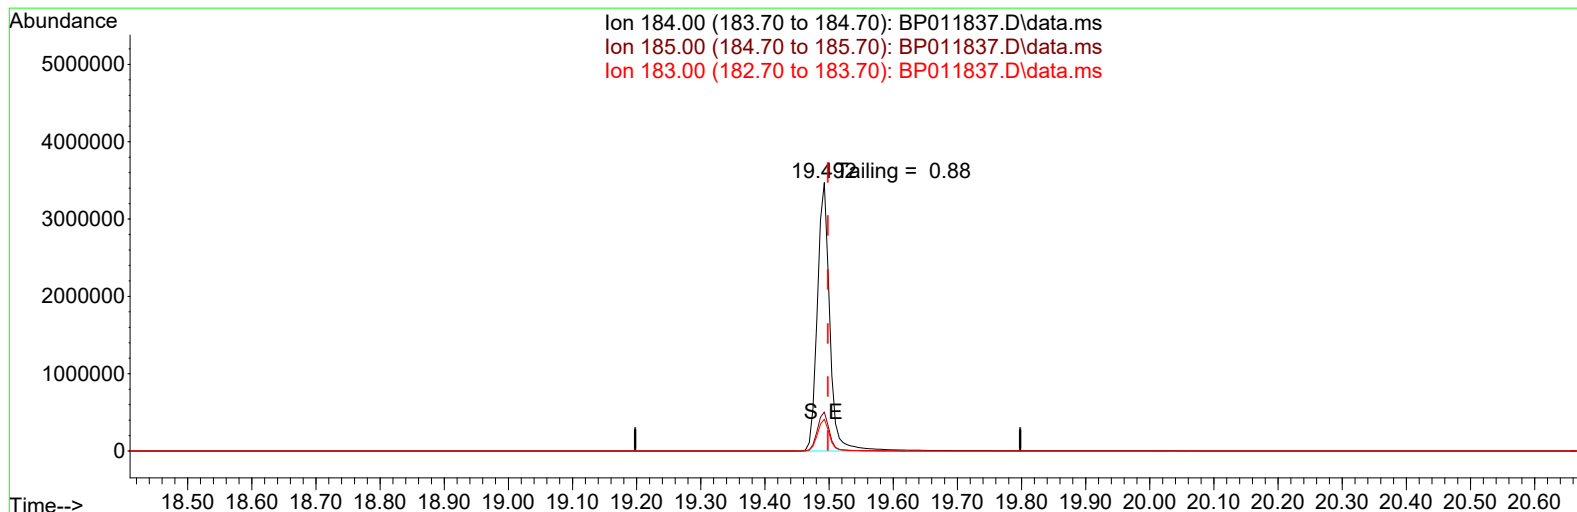

TIC: BP011837.D\data.ms

(77) Benzidine

19.492min (-0.006) 3426582.12 ng

response 4721730

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.54
183.00	11.60	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/29/2022	BNA_P	<u>BP011837.D</u>
Compound Name	Response	Retention Time
DDT	2125984	20.686
DDD	74986	20.257
DDE	6845	19.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
81831	2207815	3.71

Instrument :
BNA_P
ClientSampleId :
DFTPP