
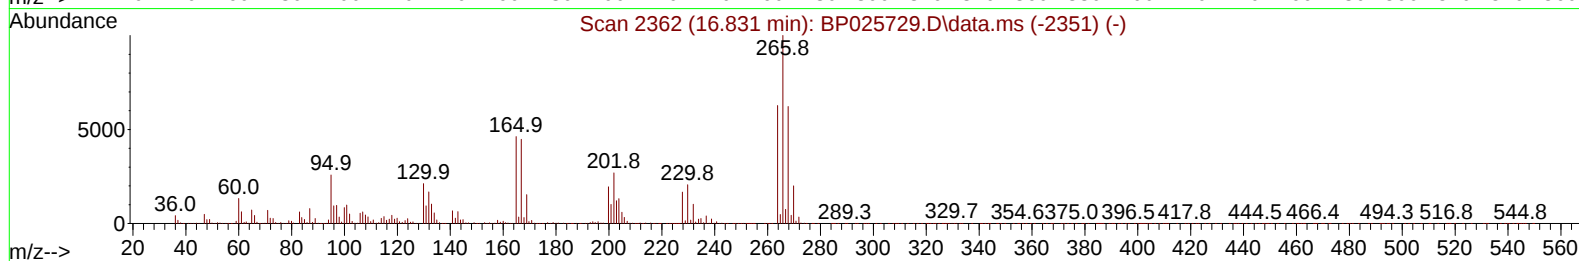
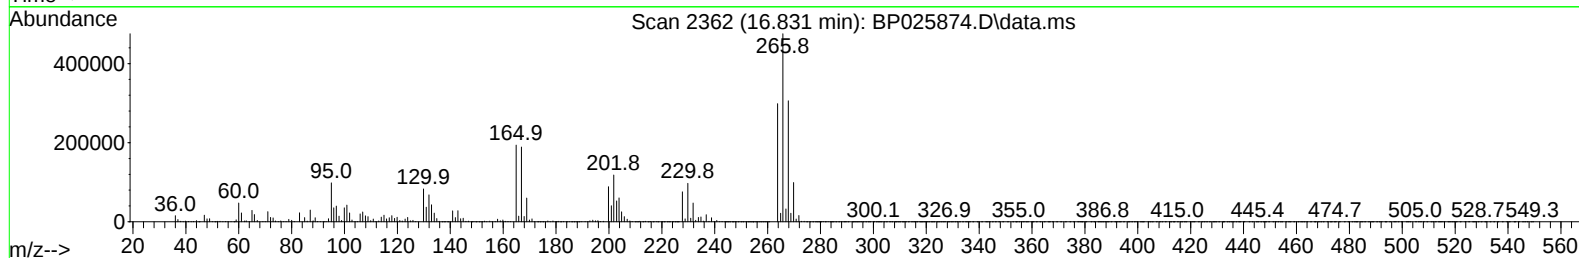


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092925\
Data File : BP025874.D
Acq On : 29 Sep 2025 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 12:06:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

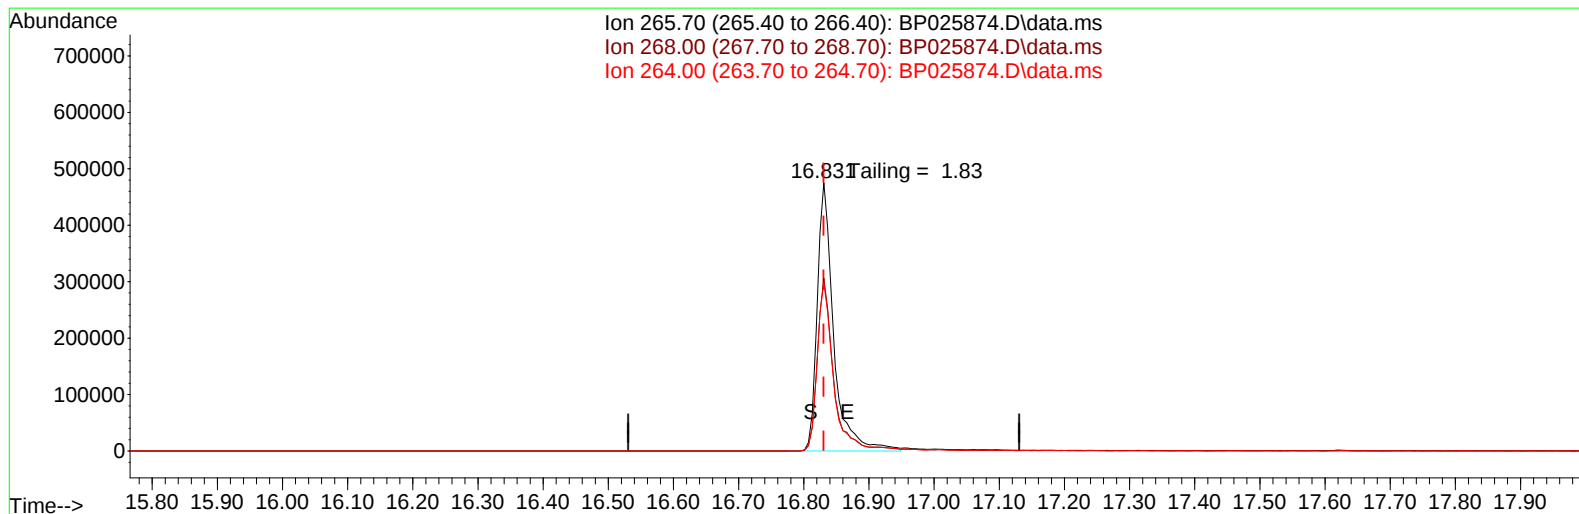

TIC: BP025874.D\data.ms

(70) Pentachlorophenol (C)




16.831min (+ 0.000) 45846.44 ng

response 845567

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.31
264.00	62.70	62.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092925\
Data File : BP025874.D
Acq On : 29 Sep 2025 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 12:06:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

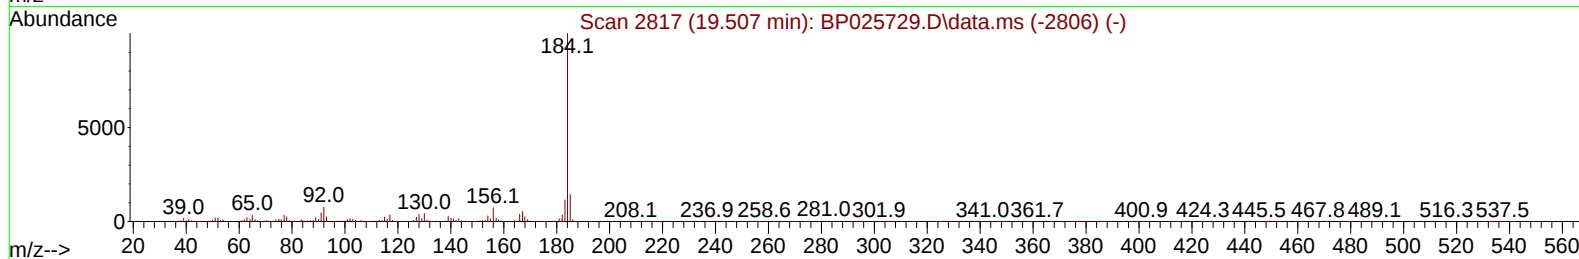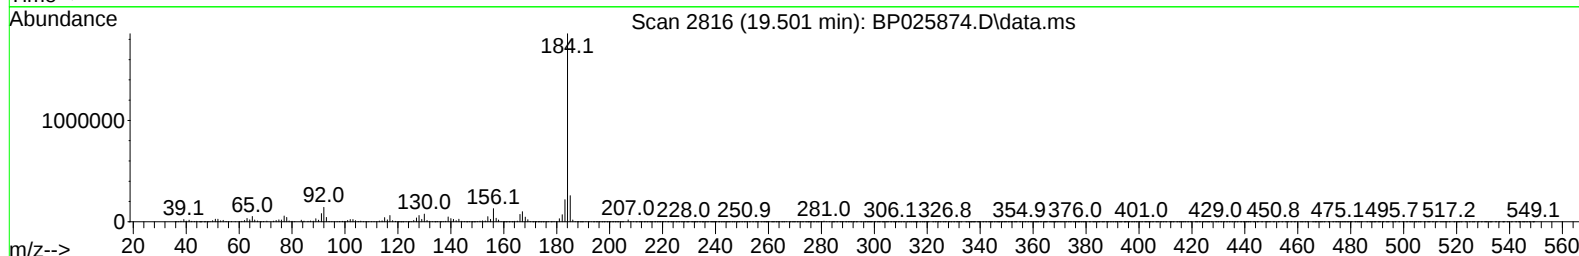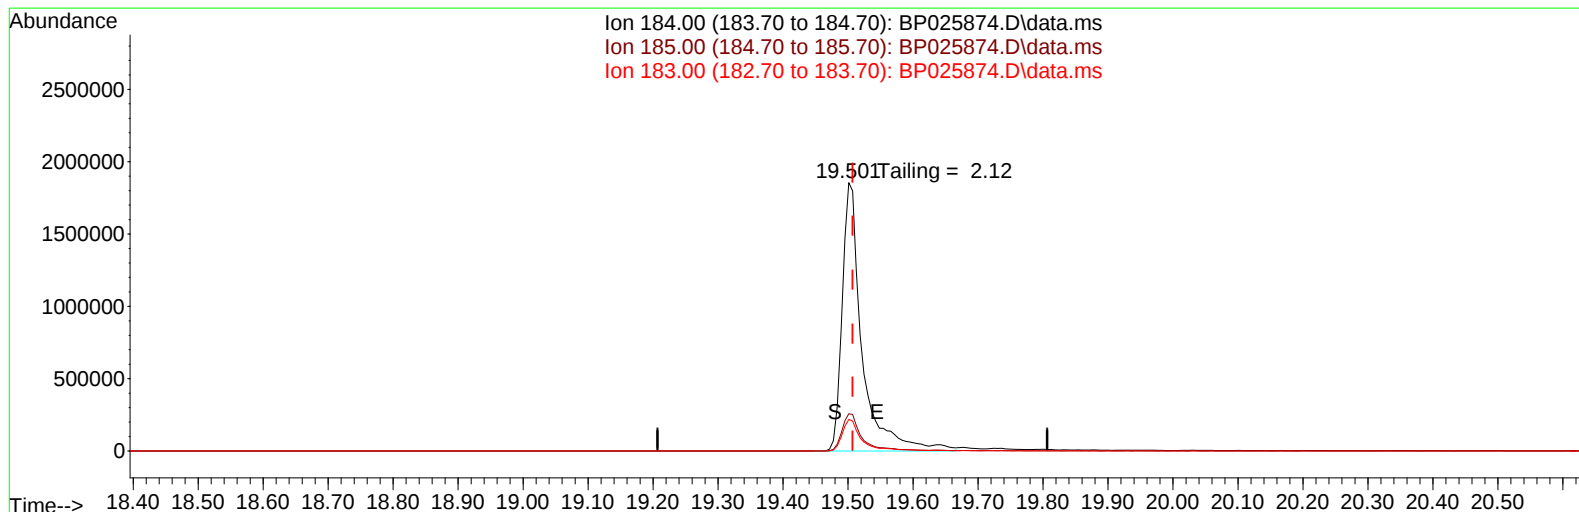

TIC: BP025874.D\data.ms

(77) Benzidine

19.501min (-0.006) 31908.41 ng

response 3894366

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.90
183.00	11.50	11.77
0.00	0.00	0.00