

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
 Data File : BP003427.D
 Acq On : 30 Sep 2020 22:53
 Operator : CG/JU
 Sample : L4172-04DL 2X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 B-6(11-13)DL

Manual Integrations
 APPROVED

mohammad
 10/1/2020 1:33:51 PM

Quant Time: Oct 01 02:18:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 30 17:14:02 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.540	152	118579	20.00	ng	0.00
21) Naphthalene-d8	10.316	136	502494	20.00	ng	# 0.00
39) Acenaphthene-d10	14.198	164	322729	20.00	ng	0.00
64) Phenanthrene-d10	16.963	188	698246	20.00	ng	# 0.02
76) Chrysene-d12	21.145	240	605972	20.00	ng	0.08
86) Perylene-d12	23.586	264	615531m	20.00	ng	0.33
System Monitoring Compounds						
5) 2-Fluorophenol	5.158	112	276845	40.77	ng	0.00
7) Phenol-d6	6.746	99	377117	41.66	ng	0.00
23) Nitrobenzene-d5	8.693	82	226772	26.51	ng	0.00
42) 2,4,6-Tribromophenol	15.710	330	152547	30.99	ng	0.02
45) 2-Fluorobiphenyl	12.810	172	514675	23.32	ng	0.00
79) Terphenyl-d14	19.563	244	661660	22.75	ng	0.03
Target Compounds						Qvalue
31) Naphthalene	10.369	128	222507	8.38	ng	99
37) 2-Methylnaphthalene	11.998	142	45748	2.38	ng	97
49) Acenaphthylene	13.916	152	116667	3.83	ng	99
50) Dimethylphthalate	13.657	163	95746	3.72	ng	98
52) Acenaphthene	14.257	154	76207	4.11	ng	98
55) Dibenzofuran	14.598	168	111412	3.77	ng	95
58) Fluorene	15.251	166	139004	5.95	ng	98
71) Phenanthrene	17.004	178	1445981	38.06	ng	99
72) Anthracene	17.098	178	408003	10.90	ng	100
73) Carbazole	17.381	167	168737	4.74	ng	98
75) Fluoranthene	19.010	202	1966781	41.17	ng	99
78) Pyrene	19.363	202	1659907	43.92	ng	99
81) Benzo(a)anthracene	21.127	228	917910	23.43	ng	# 92
83) Chrysene	21.180	228	616782m	16.39	ng	
87) Indeno(1,2,3-cd)pyrene	26.315	276	536695m	11.50	ng	
88) Benzo(b)fluoranthene	22.839	252	1341887	34.52	ng	# 95
89) Benzo(k)fluoranthene	23.457	252	1266614m	34.00	ng	
90) Benzo(a)pyrene	23.457	252	1174971	32.06	ng	# 84
91) Dibenzo(a,h)anthracene	26.492	278	469801m	12.20	ng	
92) Benzo(g,h,i)perylene	26.315	276	540817m	14.07	ng	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
Data File : BP003427.D
Acq On : 30 Sep 2020 22:53
Operator : CG/JU
Sample : L4172-04DL 2X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-6(11-13)DL

Manual Integrations
APPROVED

mohammad
10/1/2020 1:33:51 PM

Quant Time: Oct 01 02:18:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 30 17:14:02 2020
Response via : Initial Calibration

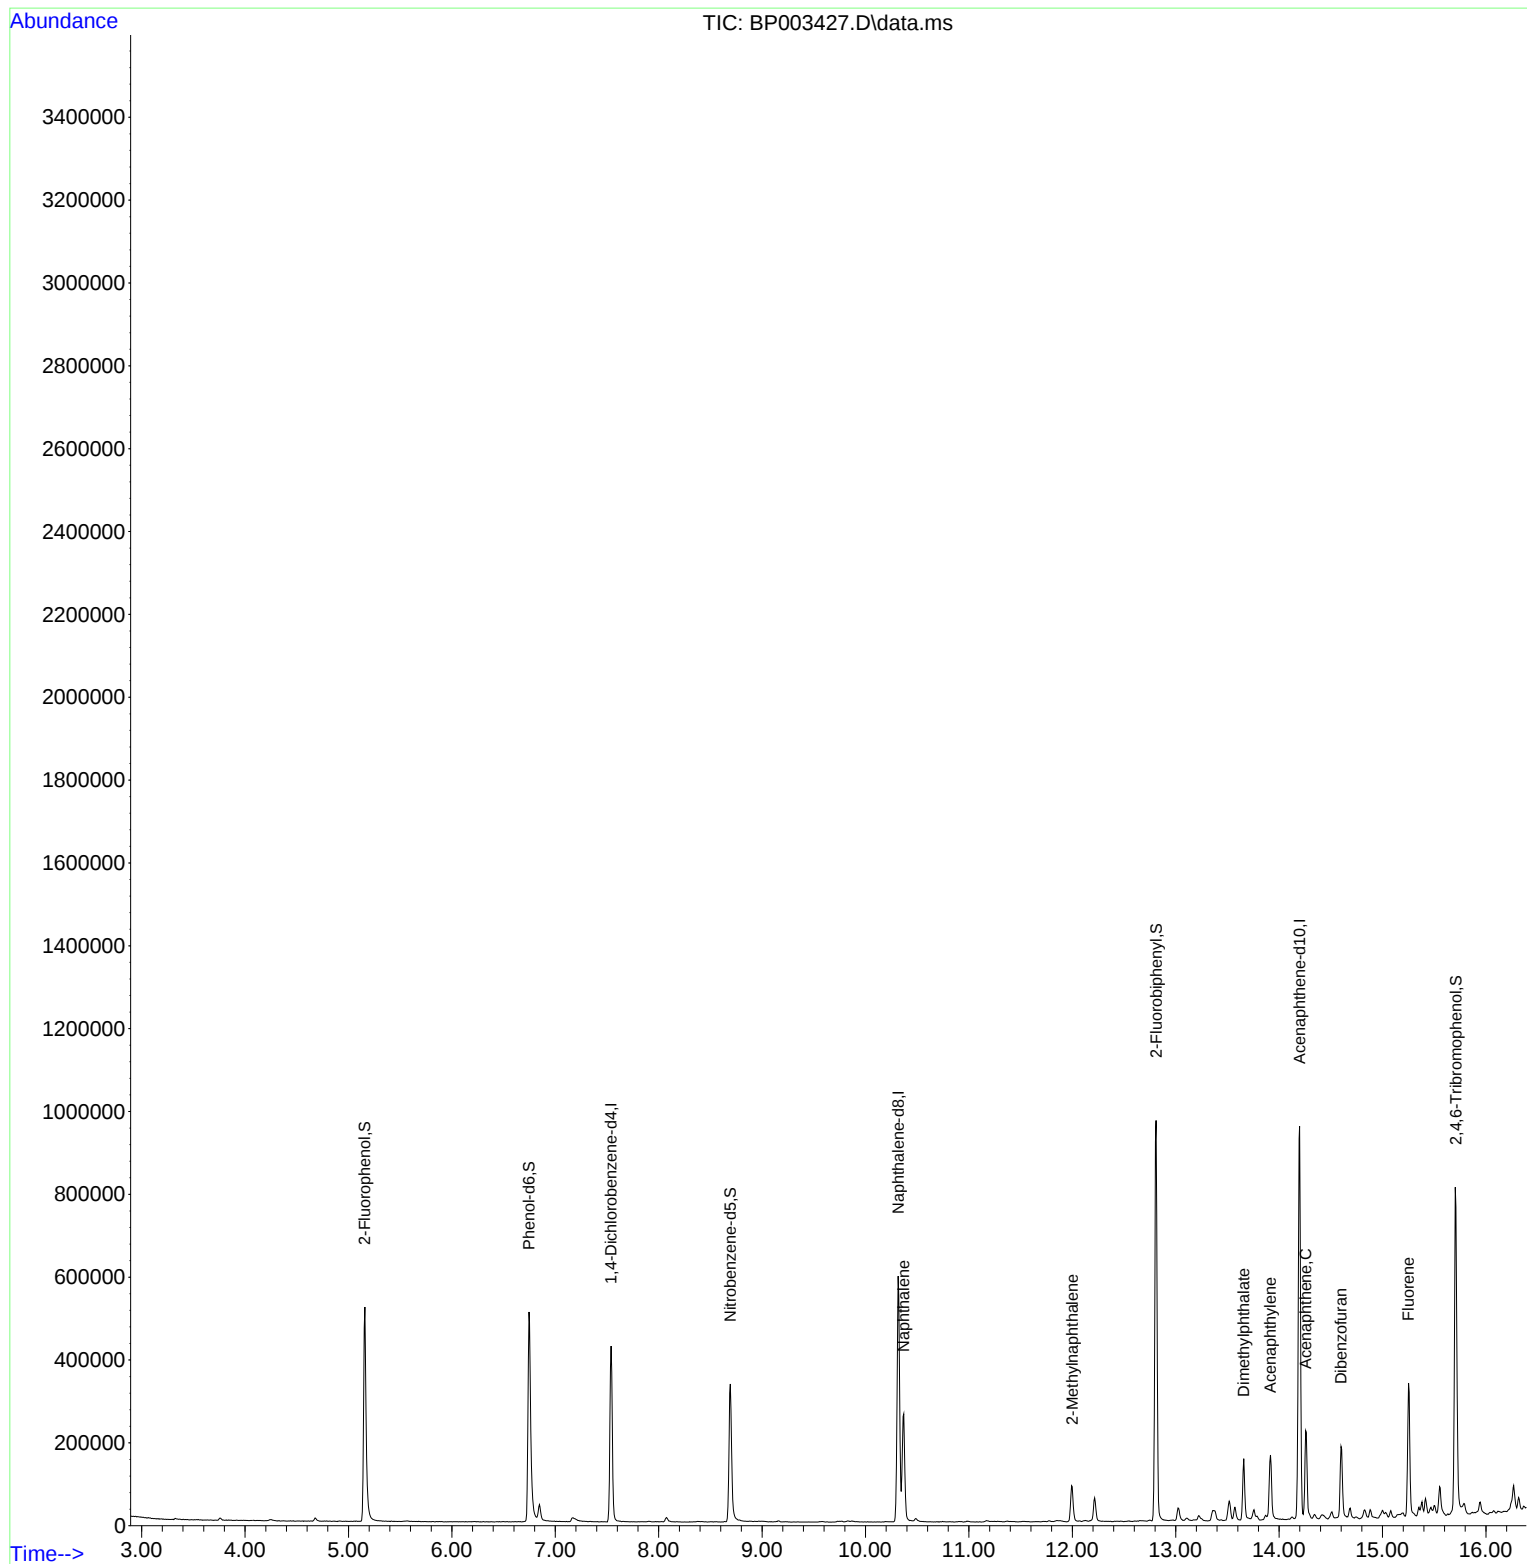

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
Data File : BP003427.D
Acq On : 30 Sep 2020 22:53
Operator : CG/JU
Sample : L4172-04DL 2X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-6(11-13)DL

Manual Integrations
APPROVED

mohammad
10/1/2020 1:33:51 PM

Quant Time: Oct 01 02:18:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 30 17:14:02 2020
Response via : Initial Calibration

