

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
 Data File : BP003428.D
 Acq On : 30 Sep 2020 23:27
 Operator : CG/JU
 Sample : L4172-02DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 B-6(7-9)DL

Manual Integrations
 APPROVED

Quant Time: Oct 01 06:24:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 30 17:14:02 2020
 Response via : Initial Calibration

mohammad

10/1/2020 1:33:54 PM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.540	152	103801	20.00	ng	0.00
21) Naphthalene-d8	10.316	136	444890	20.00	ng	# 0.00
39) Acenaphthene-d10	14.198	164	287976	20.00	ng	0.00
64) Phenanthrene-d10	16.957	188	659508	20.00	ng	# 0.01
76) Chrysene-d12	21.145	240	627309	20.00	ng	0.08
86) Perylene-d12	23.580	264	616828m	20.00	ng	0.32
System Monitoring Compounds						
5) 2-Fluorophenol	5.158	112	121152	20.38	ng	0.00
7) Phenol-d6	6.752	99	159565	20.14	ng	0.01
23) Nitrobenzene-d5	8.693	82	93482	12.34	ng	0.00
42) 2,4,6-Tribromophenol	15.710	330	68098	15.50	ng	0.02
45) 2-Fluorobiphenyl	12.810	172	229275	11.64	ng	0.00
79) Terphenyl-d14	19.563	244	336853	11.19	ng	0.03
Target Compounds						Qvalue
31) Naphthalene	10.369	128	49701	2.11	ng	98
52) Acenaphthene	14.257	154	56282	3.40	ng	98
55) Dibenzofuran	14.604	168	56650	2.15	ng	95
58) Fluorene	15.251	166	75207	3.61	ng	99
71) Phenanthrene	17.004	178	1002727	27.94	ng	99
72) Anthracene	17.092	178	259382	7.33	ng	99
73) Carbazole	17.381	167	135975	4.05	ng	99
75) Fluoranthene	19.010	202	1416051	31.39	ng	99
78) Pyrene	19.363	202	1128253	28.84	ng	100
81) Benzo(a)anthracene	21.127	228	625468	15.42	ng	# 94
83) Chrysene	21.174	228	479809m	12.32	ng	
88) Benzo(b)fluoranthene	22.845	252	947471	24.32	ng	# 94
89) Benzo(k)fluoranthene	23.463	252	887630m	23.78	ng	
90) Benzo(a)pyrene	23.463	252	819011	22.30	ng	# 85
91) Dibenzo(a,h)anthracene	26.333	278	291893m	7.57	ng	
92) Benzo(g,h,i)perylene	26.315	276	381219m	9.90	ng	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
Data File : BP003428.D
Acq On : 30 Sep 2020 23:27
Operator : CG/JU
Sample : L4172-02DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-6(7-9)DL

Manual Integrations
APPROVED

Quant Time: Oct 01 06:24:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 30 17:14:02 2020
Response via : Initial Calibration

mohammad

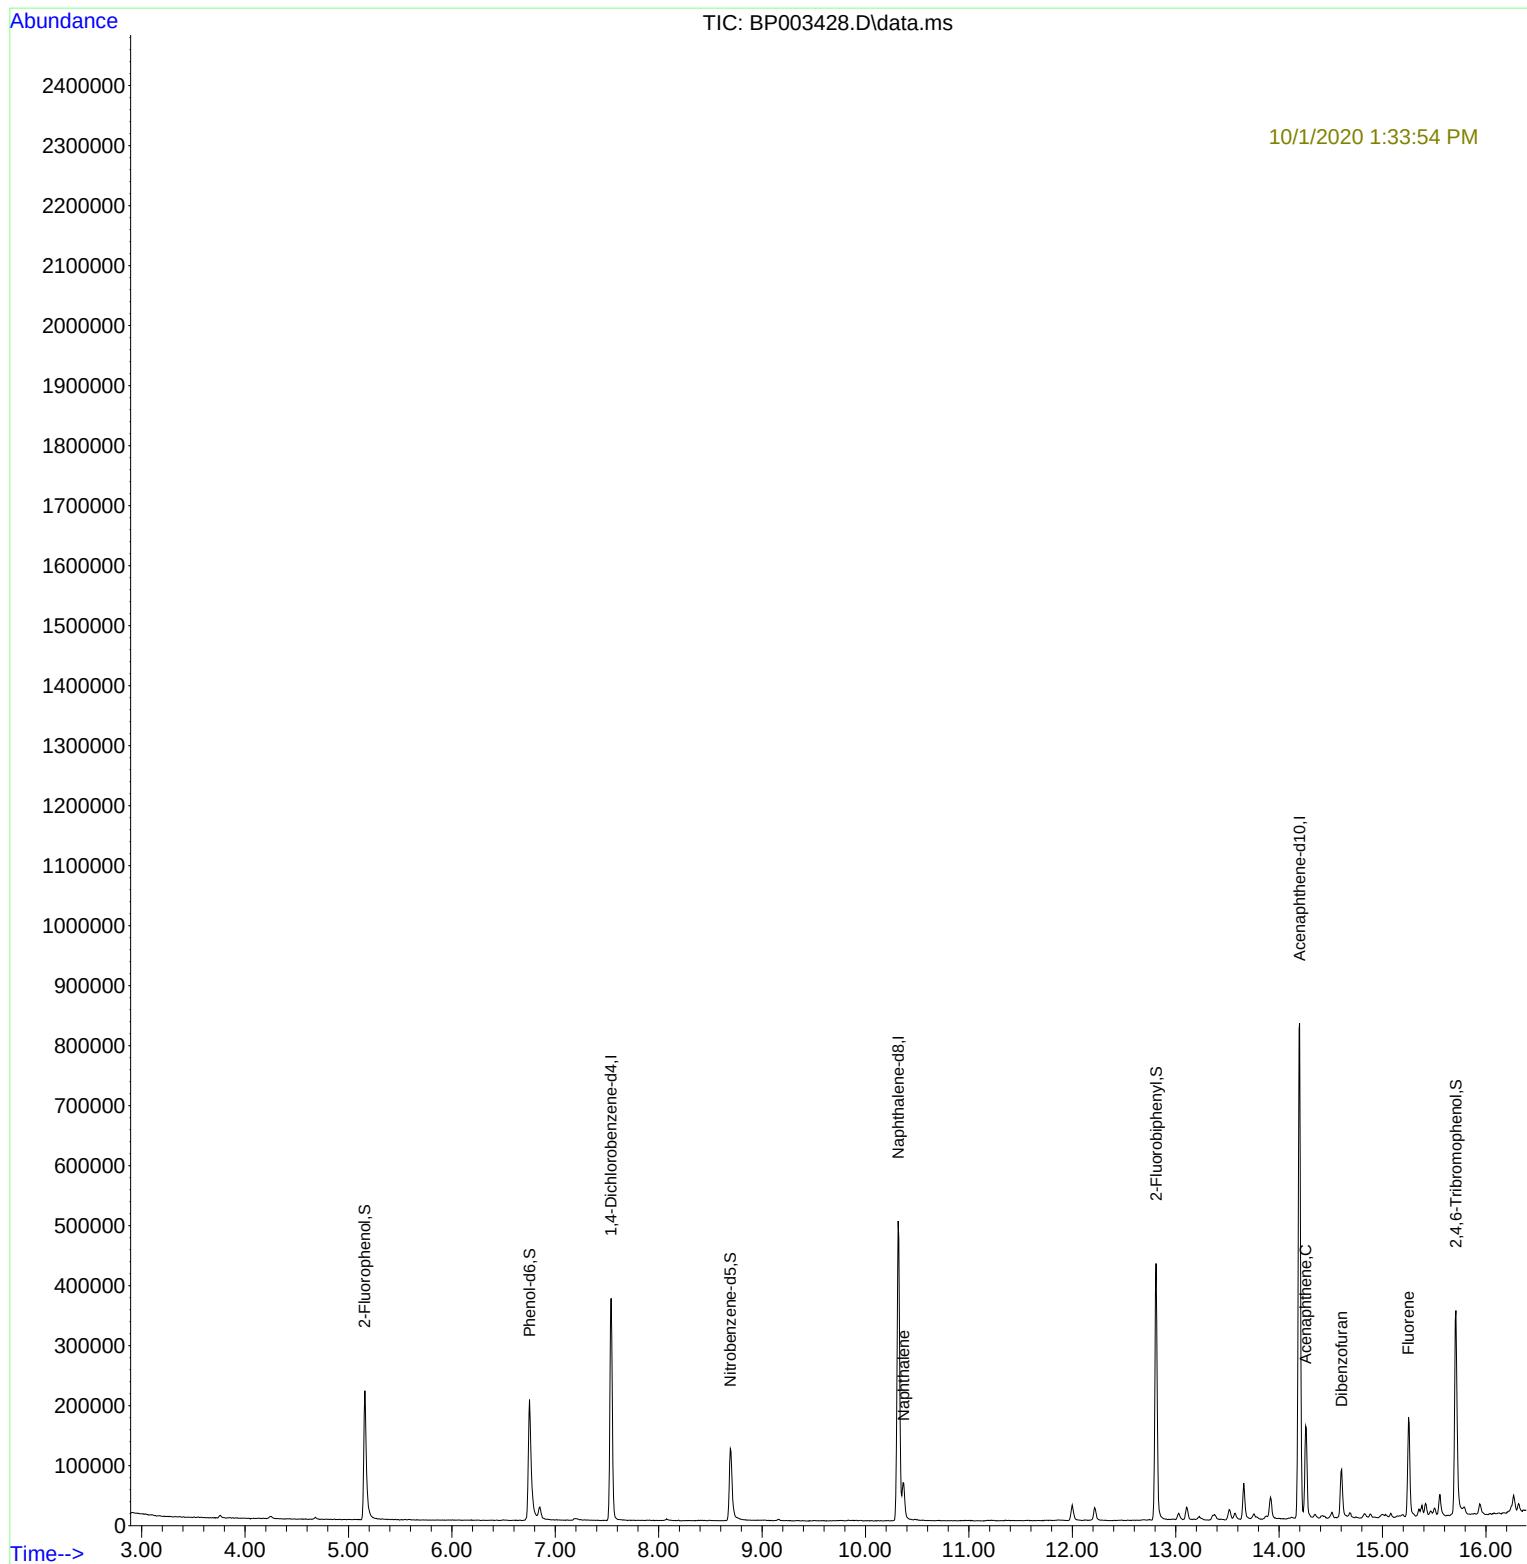

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
Data File : BP003428.D
Acq On : 30 Sep 2020 23:27
Operator : CG/JU
Sample : L4172-02DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-6(7-9)DL

Manual Integrations
APPROVED

Quant Time: Oct 01 06:24:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 30 17:14:02 2020
Response via : Initial Calibration

mohammad

