

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
 Data File : BP003432.D
 Acq On : 01 Oct 2020 01:43
 Operator : CG/JU
 Sample : L4193-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 B-12(13-14)

Manual Integrations
 APPROVED

mohammad
 10/1/2020 1:34:10 PM

Quant Time: Oct 01 04:08:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 30 17:14:02 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.540	152	98546	20.00	ng	0.00
21) Naphthalene-d8	10.316	136	423094	20.00	ng	# 0.00
39) Acenaphthene-d10	14.192	164	269066	20.00	ng	0.00
64) Phenanthrene-d10	16.963	188	592805	20.00	ng	# 0.02
76) Chrysene-d12	21.163	240	537550	20.00	ng	0.10
86) Perylene-d12	23.686	264	557316m	20.00	ng	0.43
System Monitoring Compounds						
5) 2-Fluorophenol	5.158	112	540642	95.80	ng	0.00
7) Phenol-d6	6.746	99	715834	95.16	ng	0.00
23) Nitrobenzene-d5	8.693	82	459568	63.81	ng	0.00
42) 2,4,6-Tribromophenol	15.710	330	312867	76.24	ng	0.02
45) 2-Fluorobiphenyl	12.810	172	1093738	59.45	ng	0.00
79) Terphenyl-d14	19.575	244	1601231	62.06	ng	0.04
Target Compounds						Qvalue
49) Acenaphthylene	13.916	152	120022	4.73	ng	98
50) Dimethylphthalate	13.657	163	99562	4.63	ng	100
58) Fluorene	15.251	166	44482	2.28	ng	# 99
71) Phenanthrene	17.004	178	1184143	36.71	ng	99
72) Anthracene	17.098	178	381973	12.02	ng	99
73) Carbazole	17.386	167	82802	2.74	ng	98
75) Fluoranthene	19.016	202	2798800	69.01	ng	99
78) Pyrene	19.375	202	2814915	83.97	ng	99
81) Benzo(a)anthracene	21.163	228	1325193	38.14	ng	# 94
83) Chrysene	21.192	228	1363114m	40.83	ng	
88) Benzo(b)fluoranthene	22.904	252	2400132m	68.20	ng	
89) Benzo(k)fluoranthene	23.510	252	2460314m	72.94	ng	
90) Benzo(a)pyrene	23.510	252	2450440m	73.84	ng	
92) Benzo(g,h,i)perylene	26.421	276	1065980m	30.63	ng	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
Data File : BP003432.D
Acq On : 01 Oct 2020 01:43
Operator : CG/JU
Sample : L4193-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-12(13-14)

Manual Integrations
APPROVED

mohammad
10/1/2020 1:34:10 PM

Quant Time: Oct 01 04:08:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 30 17:14:02 2020
Response via : Initial Calibration

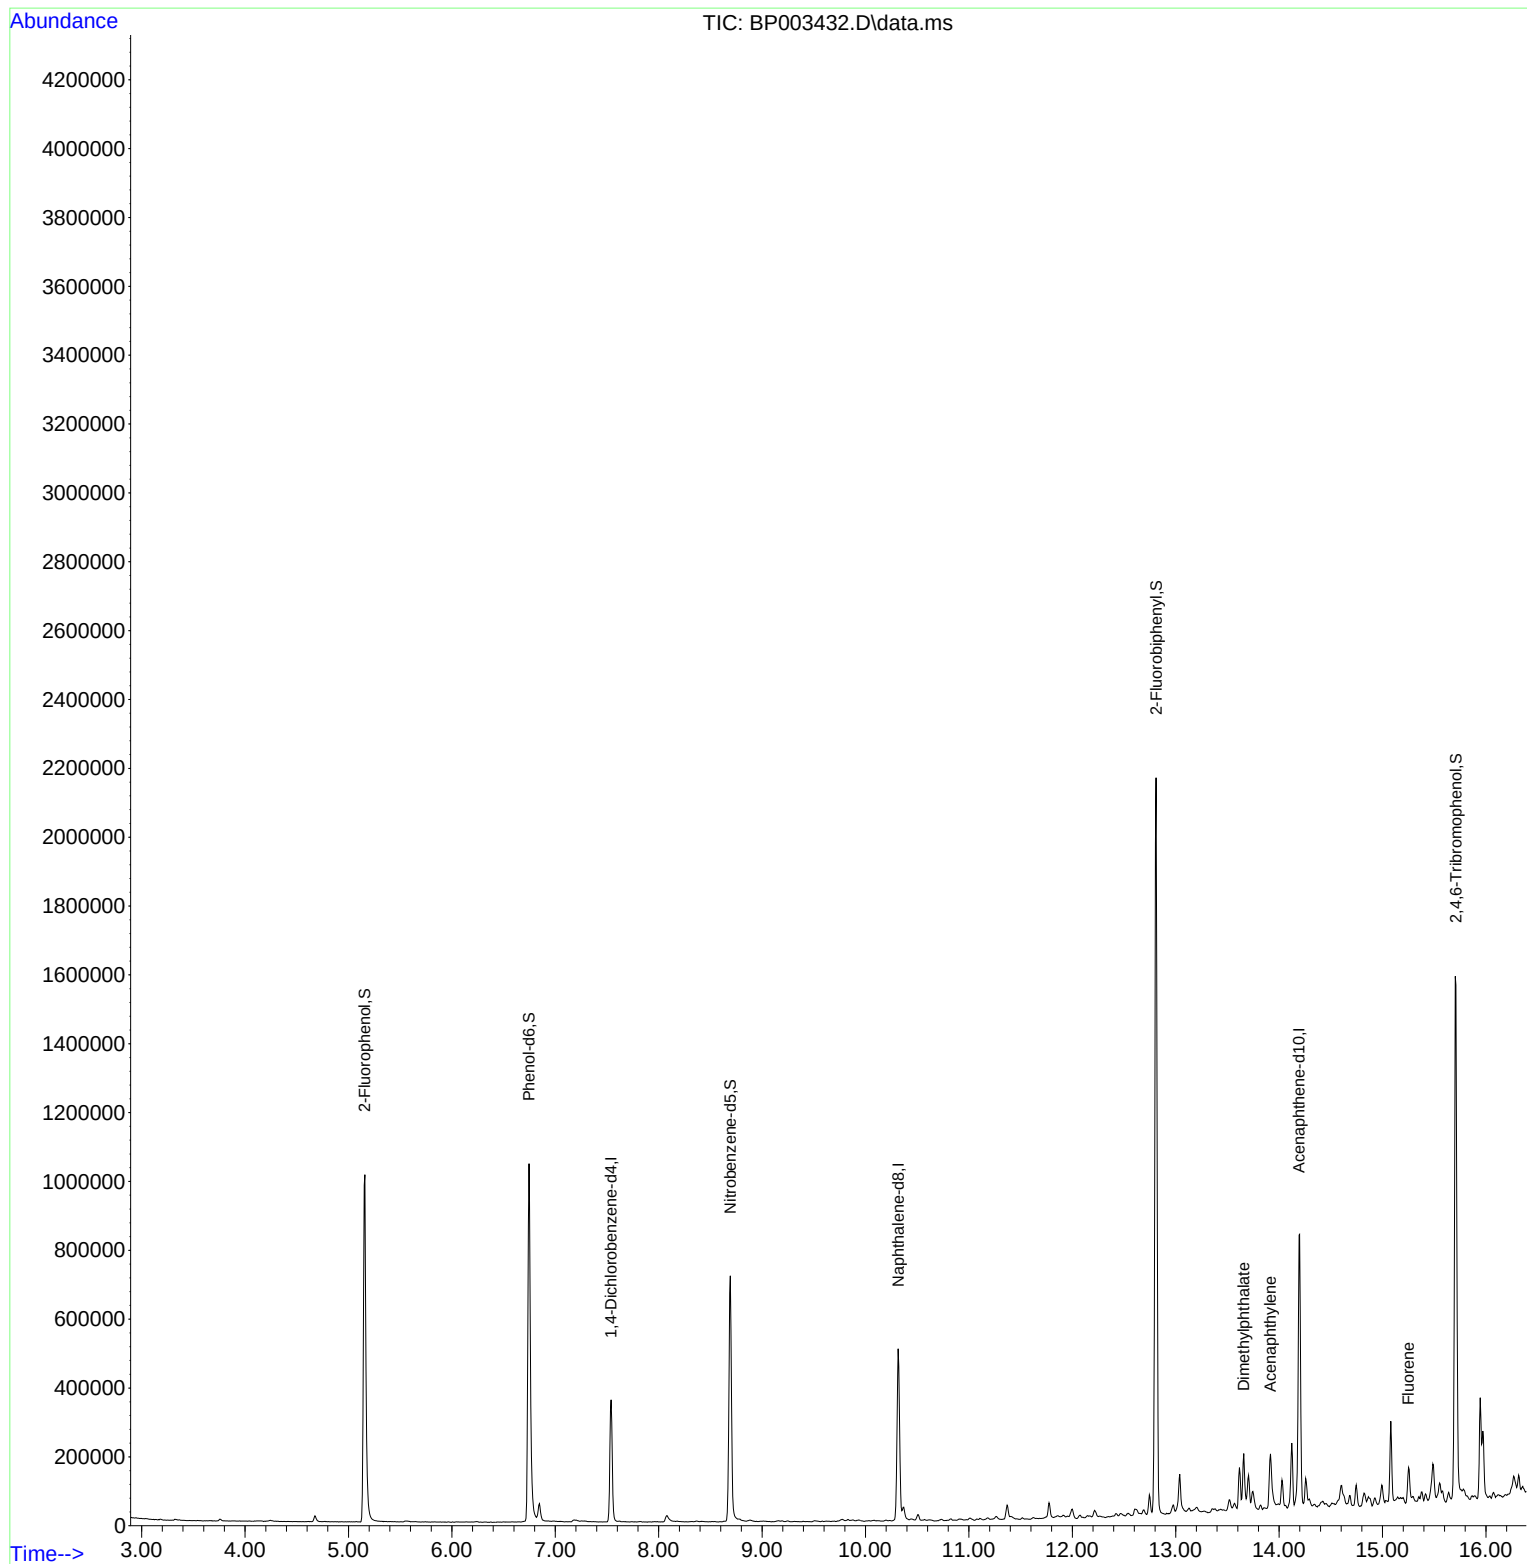

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
Data File : BP003432.D
Acq On : 01 Oct 2020 01:43
Operator : CG/JU
Sample : L4193-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-12(13-14)

Manual Integrations
APPROVED

mohammad
10/1/2020 1:34:10 PM

Quant Time: Oct 01 04:08:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 30 17:14:02 2020
Response via : Initial Calibration

