
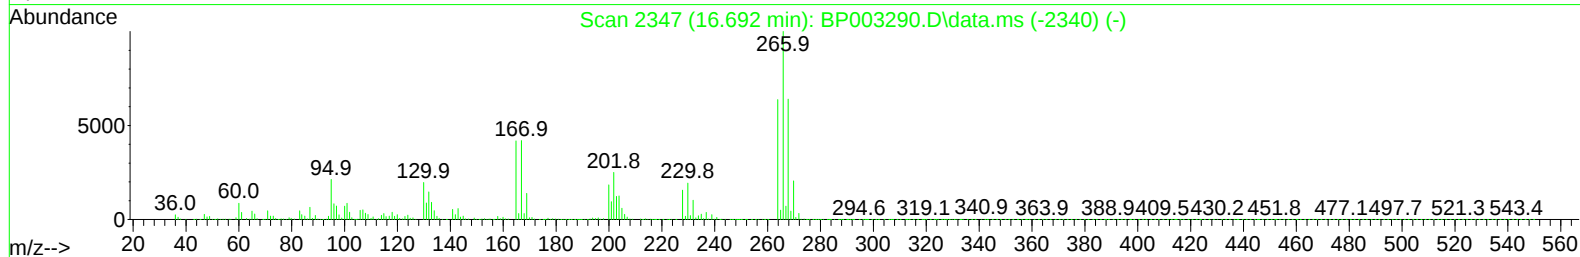
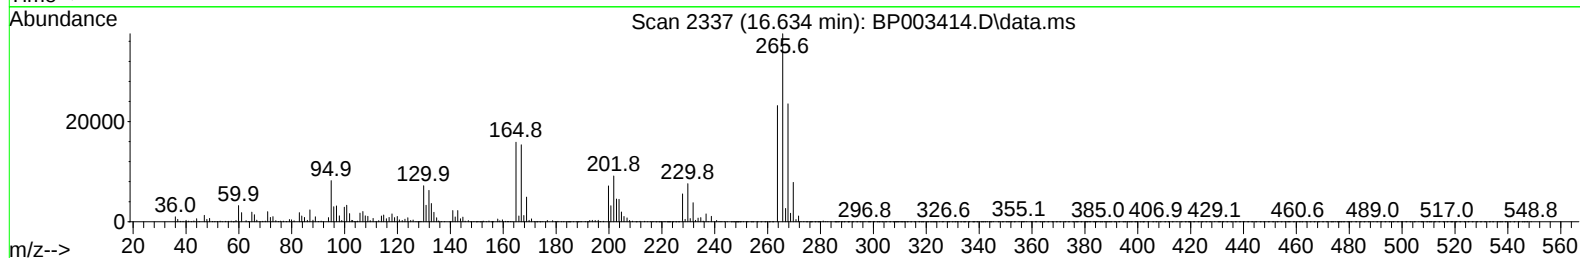


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
Data File : BP003414.D
Acq On : 30 Sep 2020 15:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 18:41:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 30 17:14:02 2020
Response via : Initial Calibration

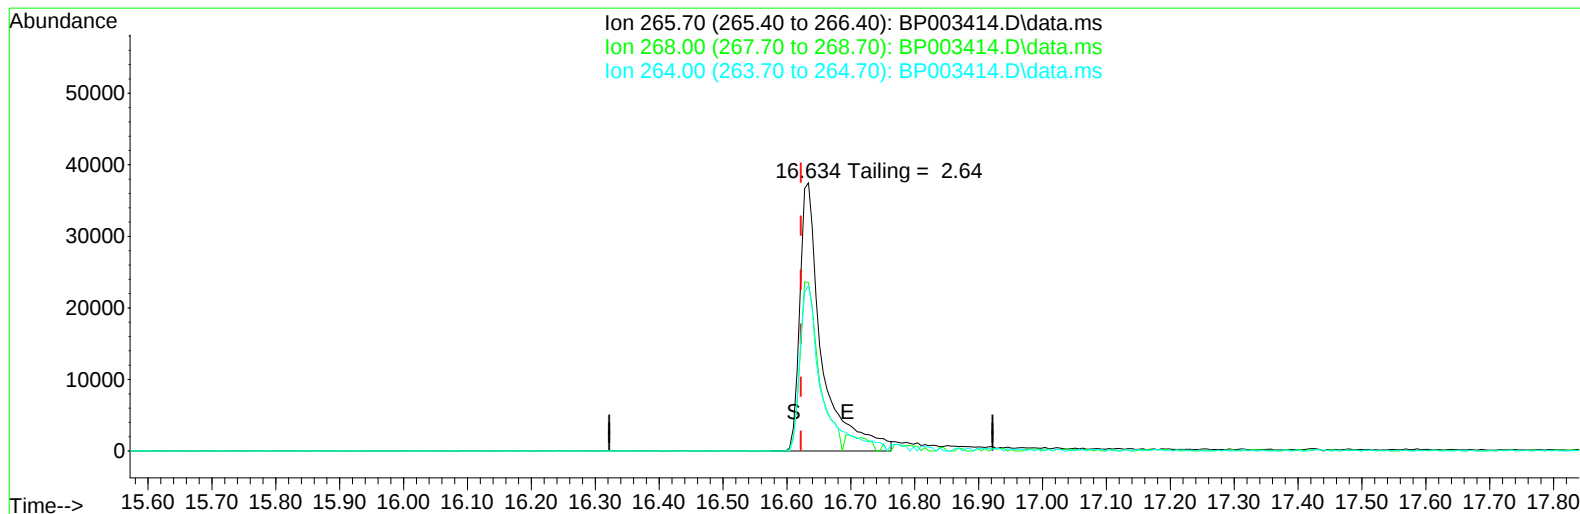

TIC: BP003414.D\data.ms

(70) Pentachlorophenol (C)




16.634min (+ 0.012) 498758.23 ng

response 94038

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	67.28
264.00	63.30	61.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
Data File : BP003414.D
Acq On : 30 Sep 2020 15:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 18:41:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 30 17:14:02 2020
Response via : Initial Calibration

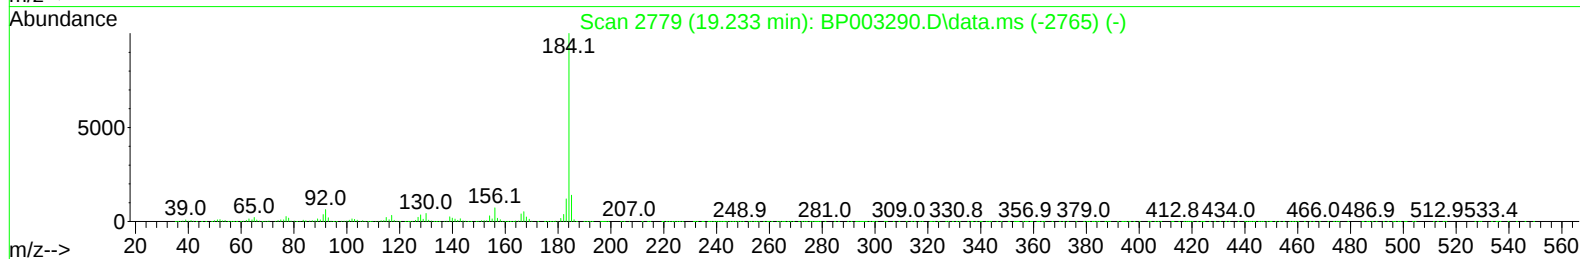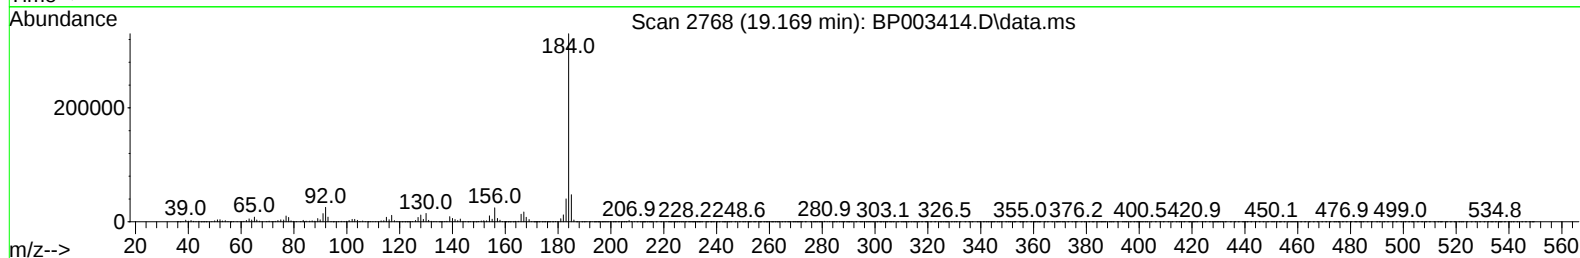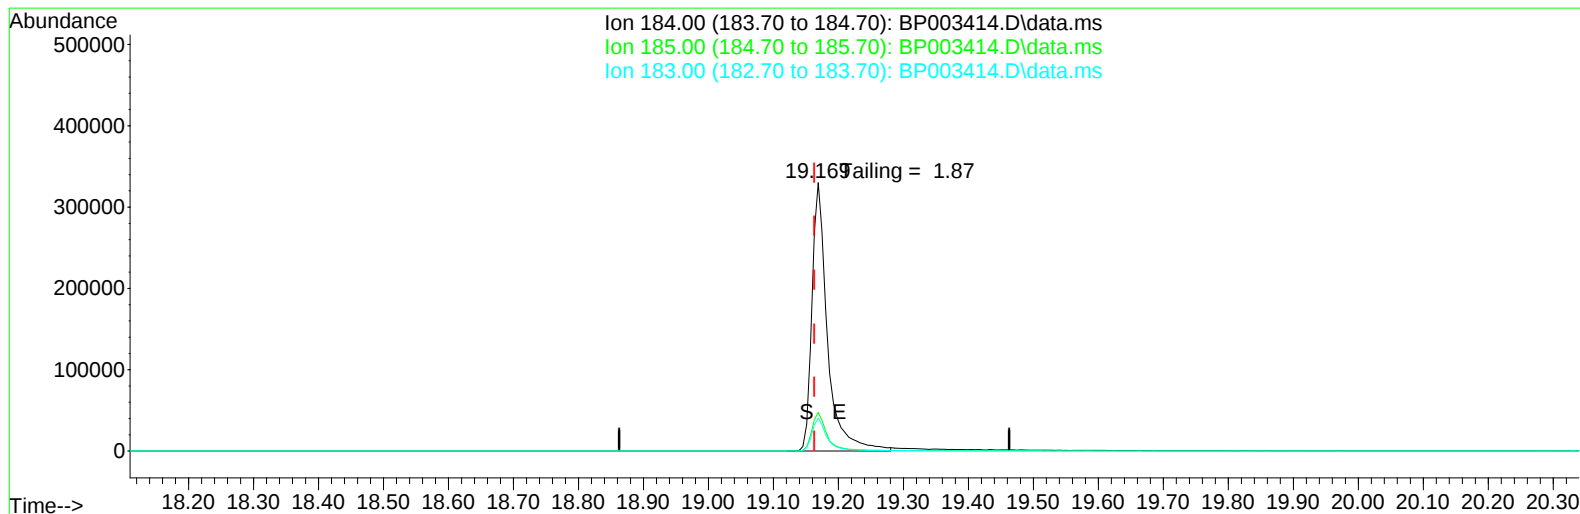

TIC: BP003414.D\data.ms

(77) Benzidine**19.169min (+ 0.006) 219935.89 ng****response 559236**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.36
183.00	12.00	12.21
0.00	0.00	0.00