
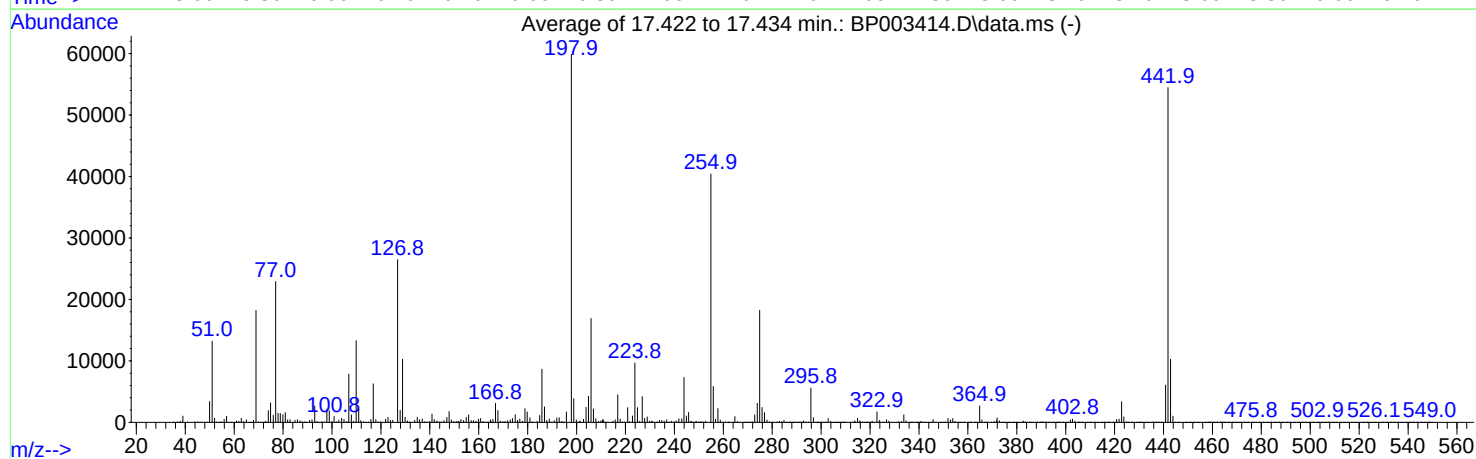


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093020\
 Data File : BP003414.D
 Acq On : 30 Sep 2020 15:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 01 10:05:32 2020

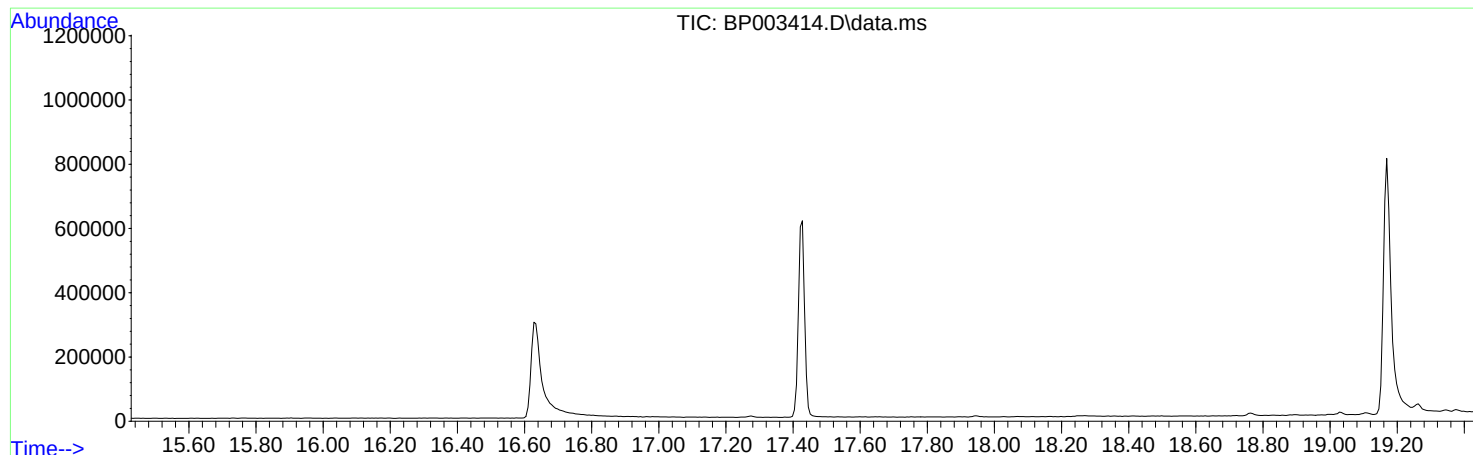

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.0	13192	PASS
68	69	0.00	2	1.8	337	PASS
69	198	0.00	100	30.5	18225	PASS
70	69	0.00	2	0.5	87	PASS
127	198	10	80	44.2	26479	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59851	PASS
199	198	5	9	6.5	3862	PASS
275	198	10	60	30.5	18230	PASS
365	198	1	100	4.5	2671	PASS
441	198	0.01	100	10.1	6064	PASS
442	198	50	100	91.0	54456	PASS
443	442	15	24	18.8	10254	PASS