

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093024\
 Data File : BP022114.D
 Acq On : 30 Sep 2024 16:00
 Operator : RC/JU
 Sample : PB163716BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK716

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	35	39	45	rVB	21592	29044	1.23%	0.136%
2	3.628	105	109	128	rBV	247401	385336	16.37%	1.803%
3	3.958	160	165	170	rBV	5697	8118	0.34%	0.038%
4	4.416	242	243	253	rVB6	2618	4484	0.19%	0.021%
5	6.881	654	662	672	rBV	312633	500130	21.24%	2.340%
6	7.040	681	689	700	rVB	214373	362980	15.42%	1.698%
7	7.240	715	723	733	rBV	333939	522204	22.18%	2.443%
8	7.699	794	801	810	rBV	320794	495897	21.06%	2.320%
9	8.398	912	920	931	rBV	364827	601455	25.54%	2.814%
10	8.840	987	995	1003	rBV	279733	477902	20.30%	2.236%
11	9.551	1105	1116	1124	rBV	255962	424096	18.01%	1.984%
12	10.087	1197	1207	1219	rBV	369881	641848	27.26%	3.003%
13	10.463	1263	1271	1279	rBV	378116	619812	26.32%	2.900%
14	10.587	1284	1292	1308	rBV	318414	600606	25.51%	2.810%
15	12.051	1534	1541	1547	rBV4	5068	10466	0.44%	0.049%
16	13.716	1816	1824	1834	rBV	698084	995298	42.27%	4.656%
17	14.004	1864	1873	1888	rBV	690976	1062219	45.11%	4.970%
18	14.145	1894	1897	1906	rVB10	3365	7239	0.31%	0.034%
19	14.316	1918	1926	1935	rBV	601426	875084	37.17%	4.094%
20	14.522	1954	1961	1978	rBV	242781	458074	19.46%	2.143%
21	14.728	1994	1996	2009	rVB	2696	5979	0.25%	0.028%
22	15.322	2090	2097	2108	rBV	846842	1381758	58.69%	6.465%
23	15.439	2111	2117	2128	rBV	317772	427159	18.14%	1.998%
24	15.563	2134	2138	2143	rVB6	4066	6869	0.29%	0.032%
25	16.769	2335	2343	2348	rBV10	4109	9030	0.38%	0.042%
26	17.110	2396	2401	2410	rBV	811299	1145329	48.64%	5.358%
27	17.204	2411	2417	2433	rVB	1147161	1586576	67.38%	7.423%
28	17.510	2465	2469	2472	rBV6	2603	3790	0.16%	0.018%
29	18.057	2557	2562	2569	rBV9	11119	21350	0.91%	0.100%
30	19.139	2742	2746	2750	rVB2	11072	15907	0.68%	0.074%
31	19.216	2755	2759	2764	rBV3	15410	23743	1.01%	0.111%
32	19.598	2817	2824	2835	rBV2	1283714	2021733	85.87%	9.459%
33	21.539	3149	3154	3165	rVB2	1035705	1553513	65.98%	7.268%
34	24.598	3665	3674	3687	rVB	790932	2354524	100.00%	11.016%
35	24.815	3703	3711	3724	rVB	676543	1734893	73.68%	8.117%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093024\
Data File : BP022114.D
Acq On : 30 Sep 2024 16:00
Operator : RC/JU
Sample : PB163716BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK716

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 21374445

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093024\
Data File : BP022114.D
Acq On : 30 Sep 2024 16:00
Operator : RC/JU
Sample : PB163716BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK716

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

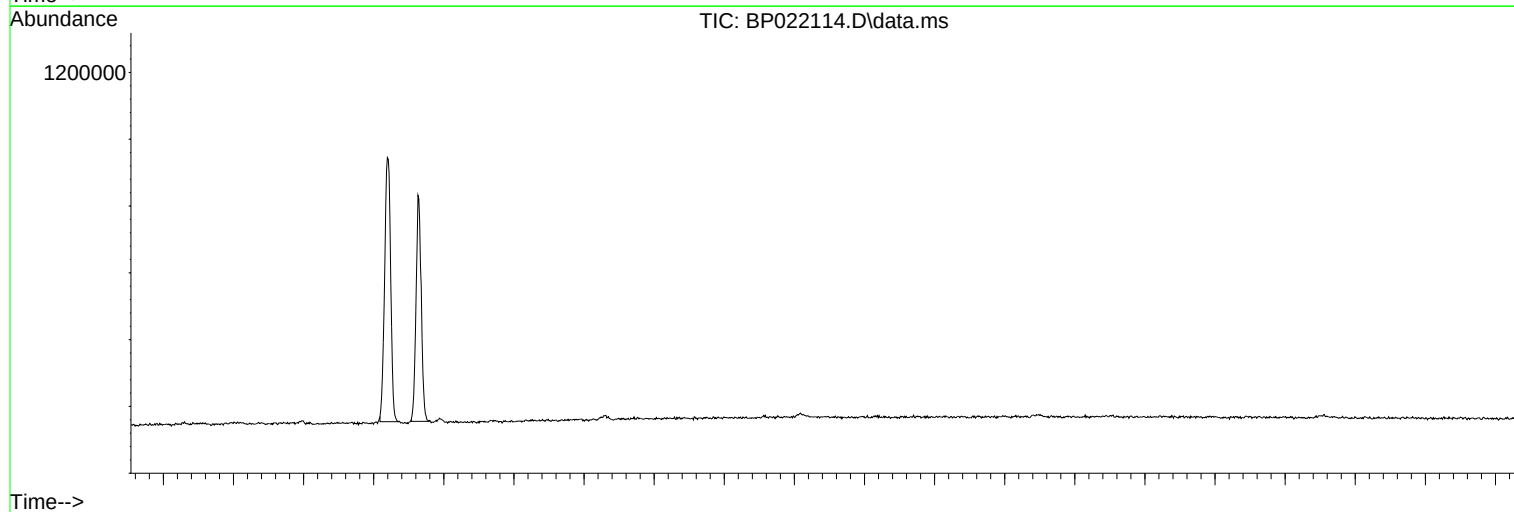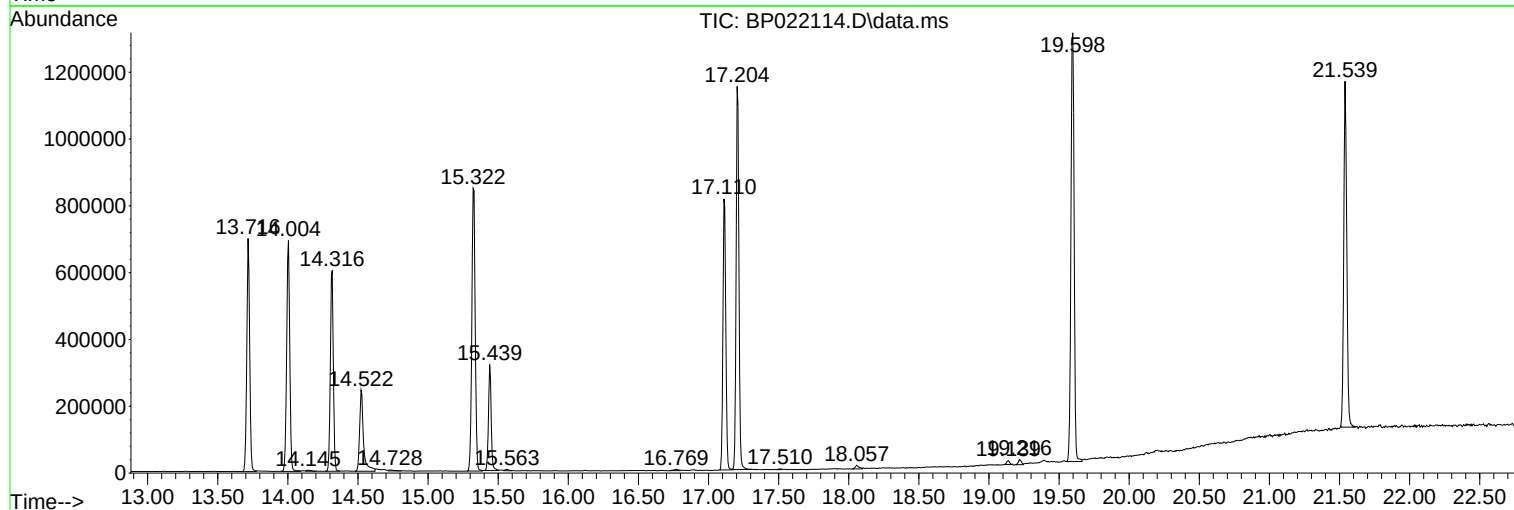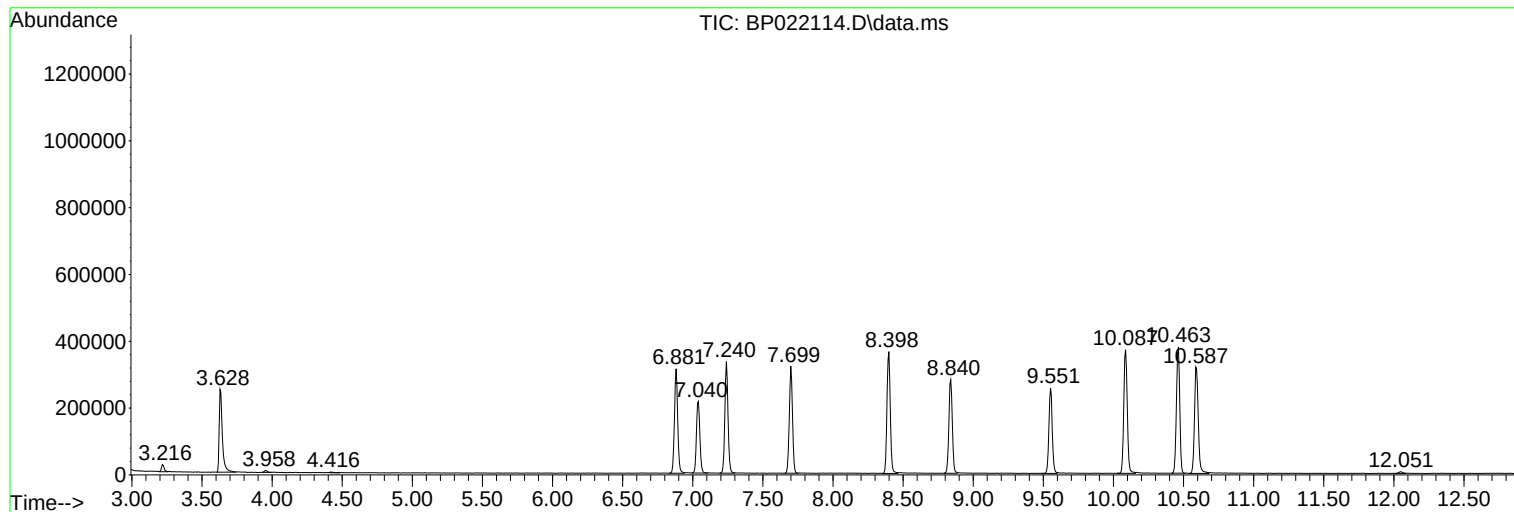

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093024\
Data File : BP022114.D
Acq On : 30 Sep 2024 16:00
Operator : RC/JU
Sample : PB163716BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK716

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093024\
Data File : BP022114.D
Acq On : 30 Sep 2024 16:00
Operator : RC/JU
Sample : PB163716BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK716

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc