

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093024\
 Data File : BP022127.D
 Acq On : 01 Oct 2024 01:31
 Operator : RC/JU
 Sample : PB163565BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK565

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	49	rVB	28363	40189	1.30%	0.137%
2	3.634	105	110	125	rBV	324829	503348	16.28%	1.716%
3	3.958	160	165	173	rVB	7875	11709	0.38%	0.040%
4	6.881	655	662	672	rBV	396145	649535	21.01%	2.214%
5	7.040	681	689	700	rBV	294062	479080	15.50%	1.633%
6	7.240	716	723	733	rBV	411664	672329	21.75%	2.292%
7	7.699	794	801	816	rVB	432910	686910	22.22%	2.342%
8	8.399	913	920	931	rBV	497558	805913	26.07%	2.747%
9	8.840	987	995	1010	rBV	370797	656149	21.22%	2.237%
10	9.551	1109	1116	1126	rBV	332965	561293	18.15%	1.913%
11	10.087	1198	1207	1226	rBV	531427	873593	28.25%	2.978%
12	10.457	1262	1270	1283	rVB	518266	902802	29.20%	3.078%
13	10.593	1285	1293	1309	rBV	469938	816046	26.39%	2.782%
14	12.045	1532	1540	1546	rBV3	6517	14146	0.46%	0.048%
15	13.710	1815	1823	1838	rBV	900459	1334484	43.16%	4.549%
16	13.998	1864	1872	1880	rBV2	929278	1447451	46.82%	4.934%
17	14.310	1917	1925	1935	rBV	895616	1319177	42.67%	4.497%
18	14.528	1955	1962	1985	rBV	306509	652217	21.09%	2.223%
19	15.316	2090	2096	2104	rBV	1376958	1895086	61.29%	6.460%
20	15.433	2110	2116	2125	rBV	395475	564265	18.25%	1.924%
21	15.563	2133	2138	2143	rVB7	5951	11148	0.36%	0.038%
22	15.898	2191	2195	2199	rBV6	1704	3247	0.11%	0.011%
23	16.751	2336	2340	2341	rBV3	3785	4901	0.16%	0.017%
24	17.098	2393	2399	2410	rBV	1231029	1732836	56.05%	5.907%
25	17.204	2410	2417	2429	rVV	1264612	2140417	69.23%	7.297%
26	18.039	2554	2559	2565	rBV9	7046	15325	0.50%	0.052%
27	19.127	2740	2744	2747	rBV2	19553	25055	0.81%	0.085%
28	19.192	2751	2755	2760	rVV	20475	27333	0.88%	0.093%
29	19.574	2814	2820	2829	rBV	1993297	2729491	88.28%	9.305%
30	21.533	3147	3153	3162	rBV2	1417244	2261854	73.16%	7.711%
31	24.592	3663	3673	3686	rVB	1229618	3091836	100.00%	10.540%
32	24.815	3701	3711	3726	rVB	873710	2405472	77.80%	8.200%




Sum of corrected areas: 29334637

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093024\
Data File : BP022127.D
Acq On : 01 Oct 2024 01:31
Operator : RC/JU
Sample : PB163565BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK565

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

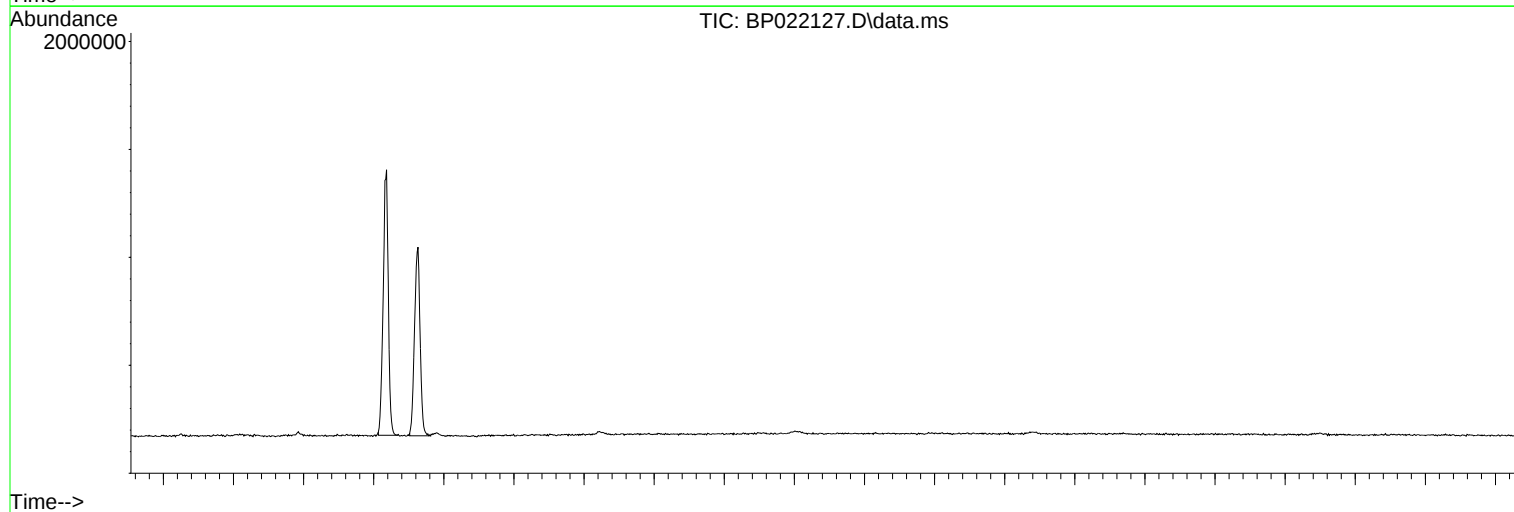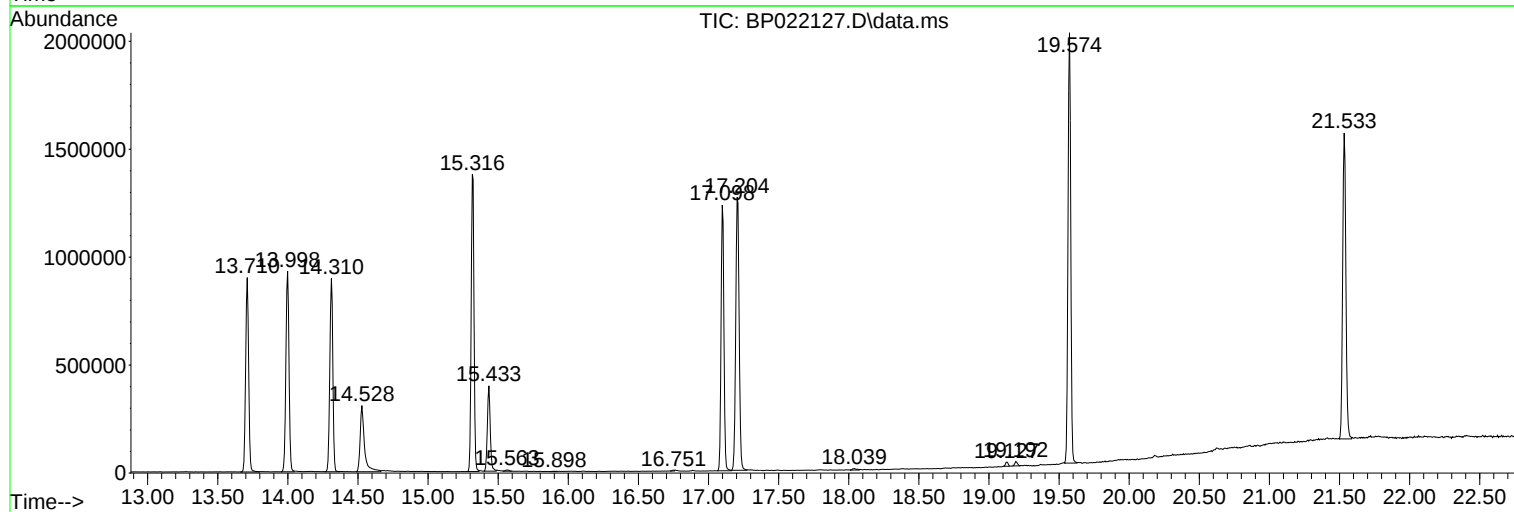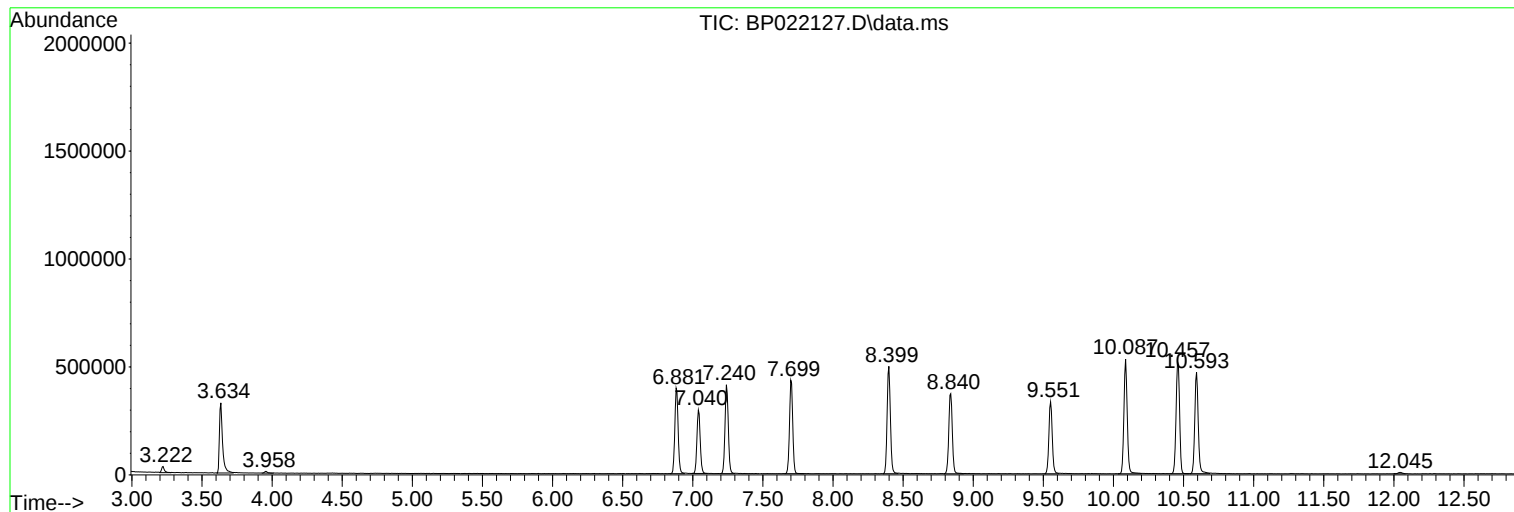

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093024\
Data File : BP022127.D
Acq On : 01 Oct 2024 01:31
Operator : RC/JU
Sample : PB163565BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK565

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093024\
Data File : BP022127.D
Acq On : 01 Oct 2024 01:31
Operator : RC/JU
Sample : PB163565BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK565

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------