

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100120\
 Data File : BP003445.D
 Acq On : 01 Oct 2020 19:21
 Operator : CG/JU
 Sample : L4136-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PAV-B26-092420-0-10

Quant Time: Oct 02 02:51:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 01 10:05:32 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.528	152	99701	20.00	ng	0.00
21) Naphthalene-d8	10.310	136	400202	20.00	ng	# 0.00
39) Acenaphthene-d10	14.192	164	261723	20.00	ng	0.00
64) Phenanthrene-d10	16.945	188	591957	20.00	ng	# 0.00
76) Chrysene-d12	21.051	240	626457	20.00	ng	-0.01
86) Perylene-d12	23.239	264	553685	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.146	112	805113	141.01	ng	0.00
7) Phenol-d6	6.740	99	955985	125.61	ng	0.00
23) Nitrobenzene-d5	8.681	82	771299	113.22	ng	0.00
42) 2,4,6-Tribromophenol	15.698	330	501857	125.72	ng	0.00
45) 2-Fluorobiphenyl	12.804	172	1666965	93.15	ng	0.00
79) Terphenyl-d14	19.533	244	2520986	83.85	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.657	163	54670	2.62	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100120\
Data File : BP003445.D
Acq On : 01 Oct 2020 19:21
Operator : CG/JU
Sample : L4136-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PAV-B26-092420-0-10

Quant Time: Oct 02 02:51:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 10:05:32 2020
Response via : Initial Calibration

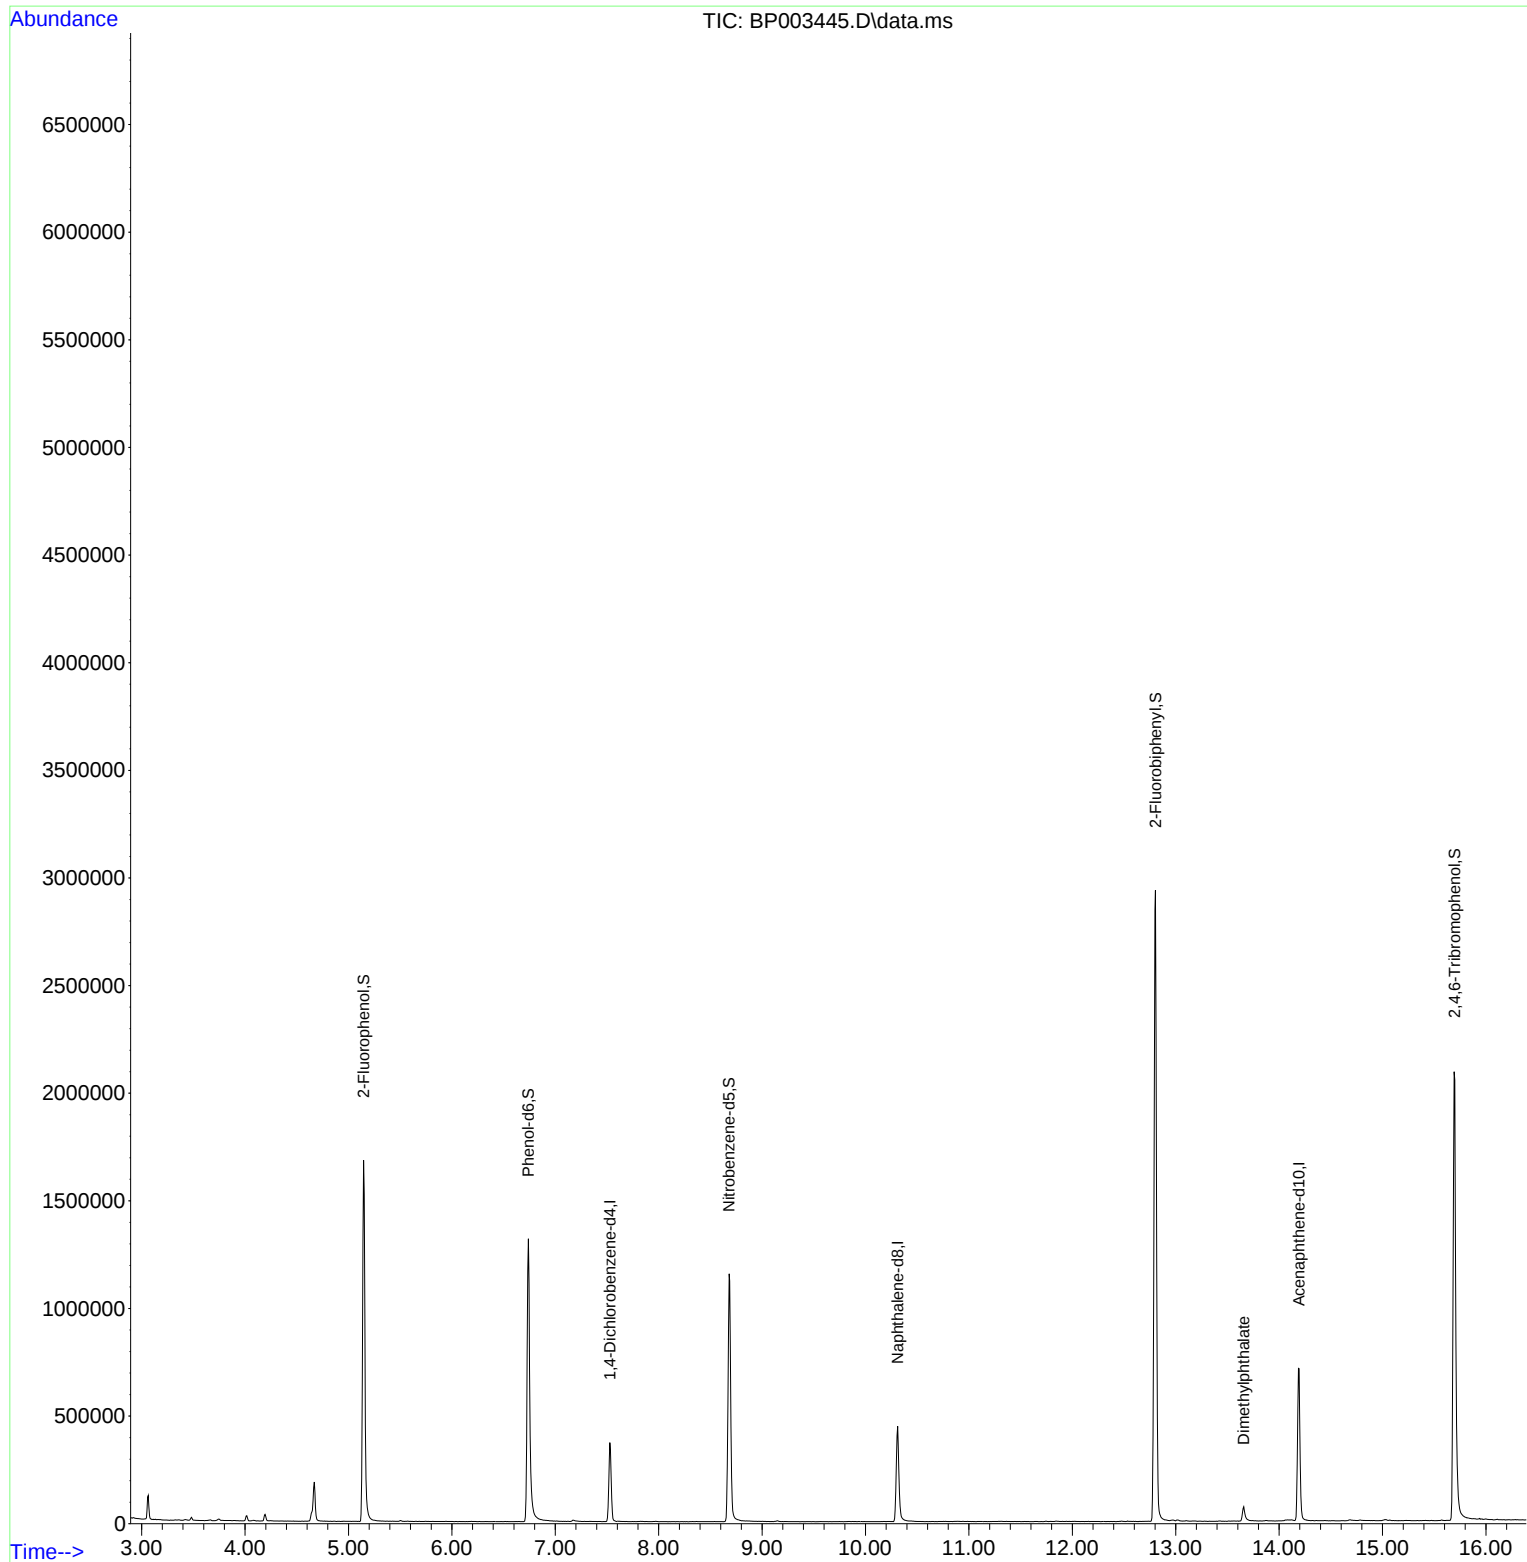

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100120\
Data File : BP003445.D
Acq On : 01 Oct 2020 19:21
Operator : CG/JU
Sample : L4136-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PAV-B26-092420-0-10

Quant Time: Oct 02 02:51:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 10:05:32 2020
Response via : Initial Calibration

