
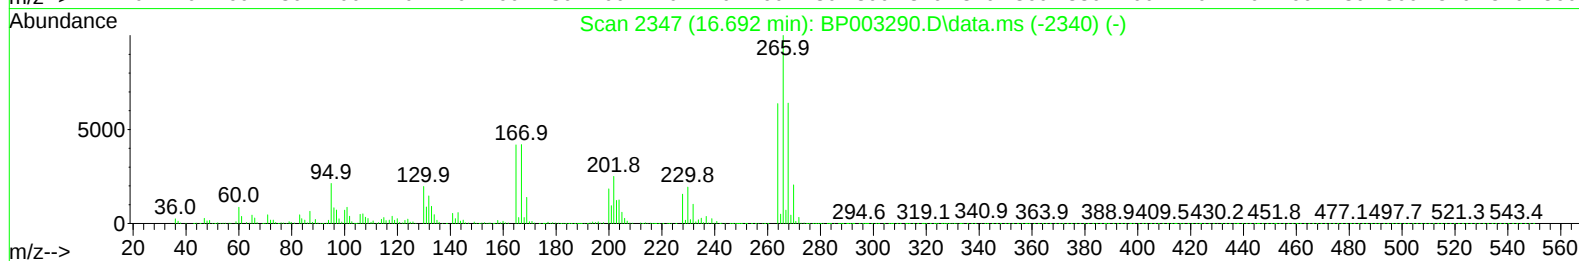
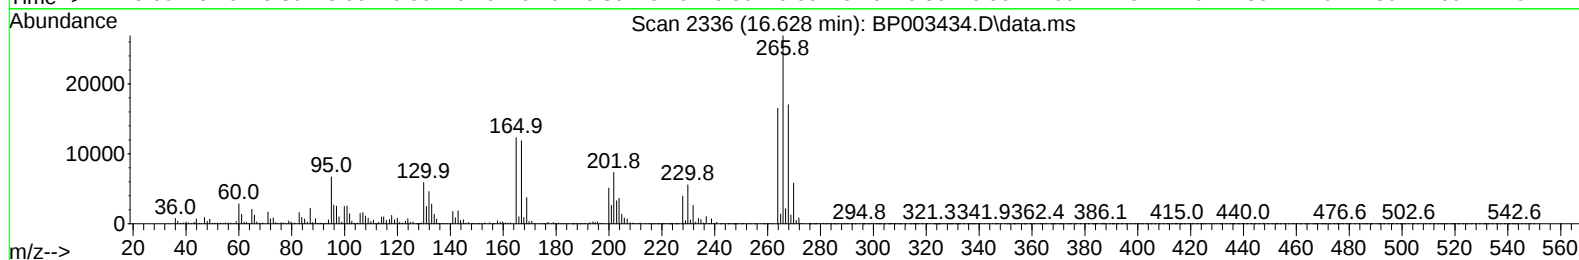


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP100120\  
Data File : BP003434.D  
Acq On : 01 Oct 2020 12:18  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 02 06:26:03 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP091520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 01 10:05:32 2020  
Response via : Initial Calibration

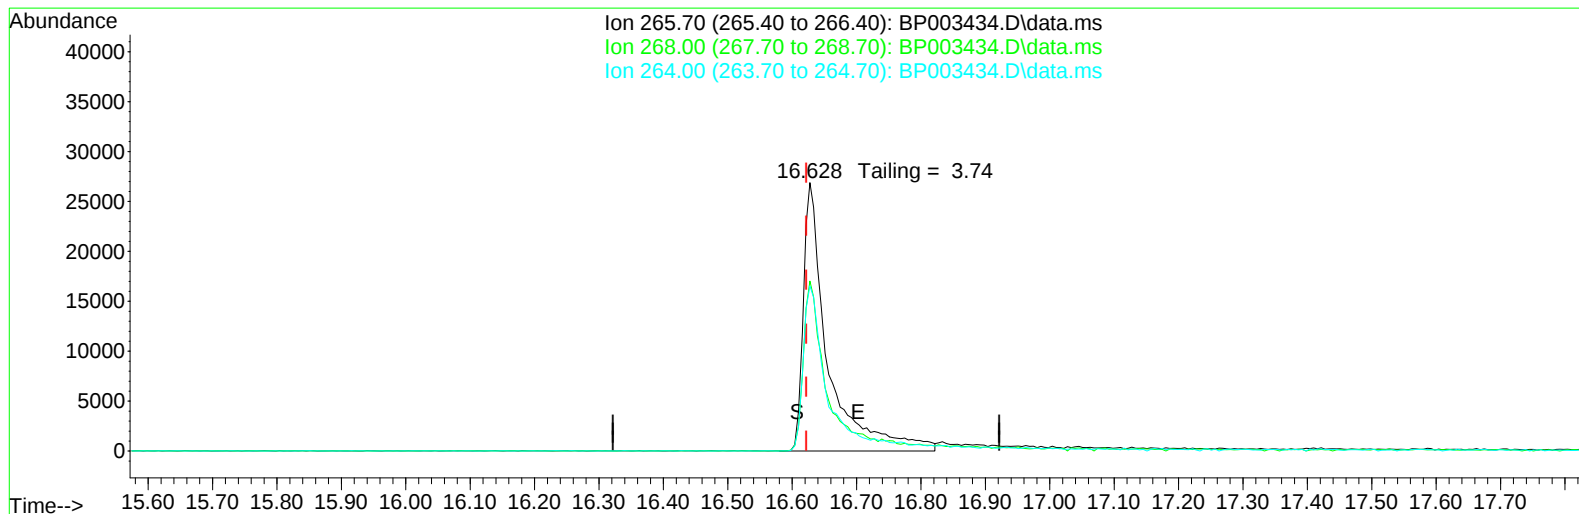

TIC: BP003434.D\data.ms

**(70) Pentachlorophenol (C)**




**16.628min (+ 0.006) 294478.29 ng**

**response 71385**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.90  | 63.31  |
| 264.00 | 63.30  | 61.47  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP100120\  
Data File : BP003434.D  
Acq On : 01 Oct 2020 12:18  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 02 06:26:03 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP091520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 01 10:05:32 2020  
Response via : Initial Calibration

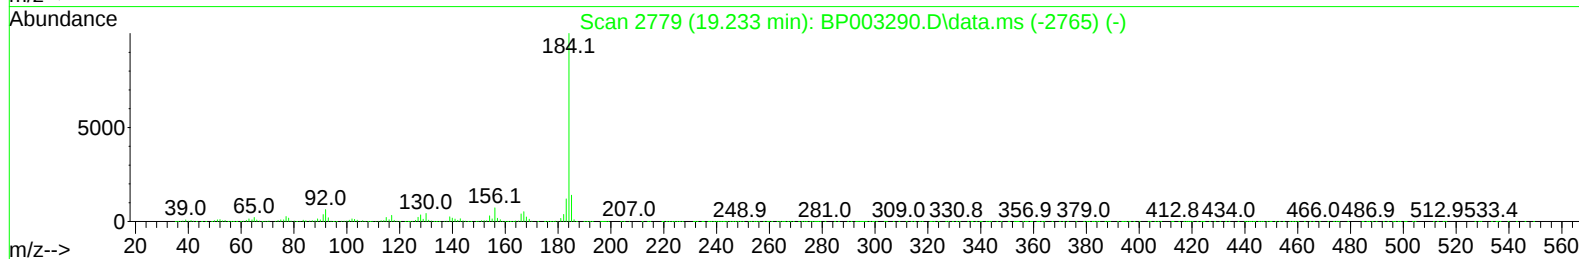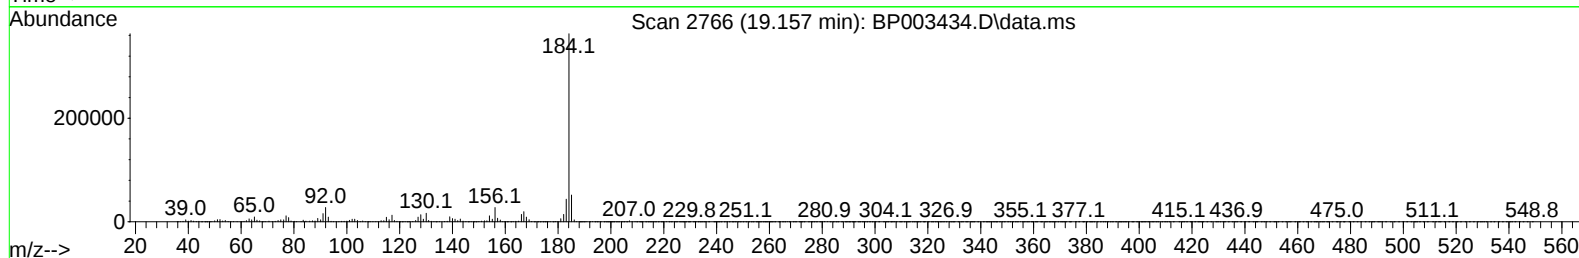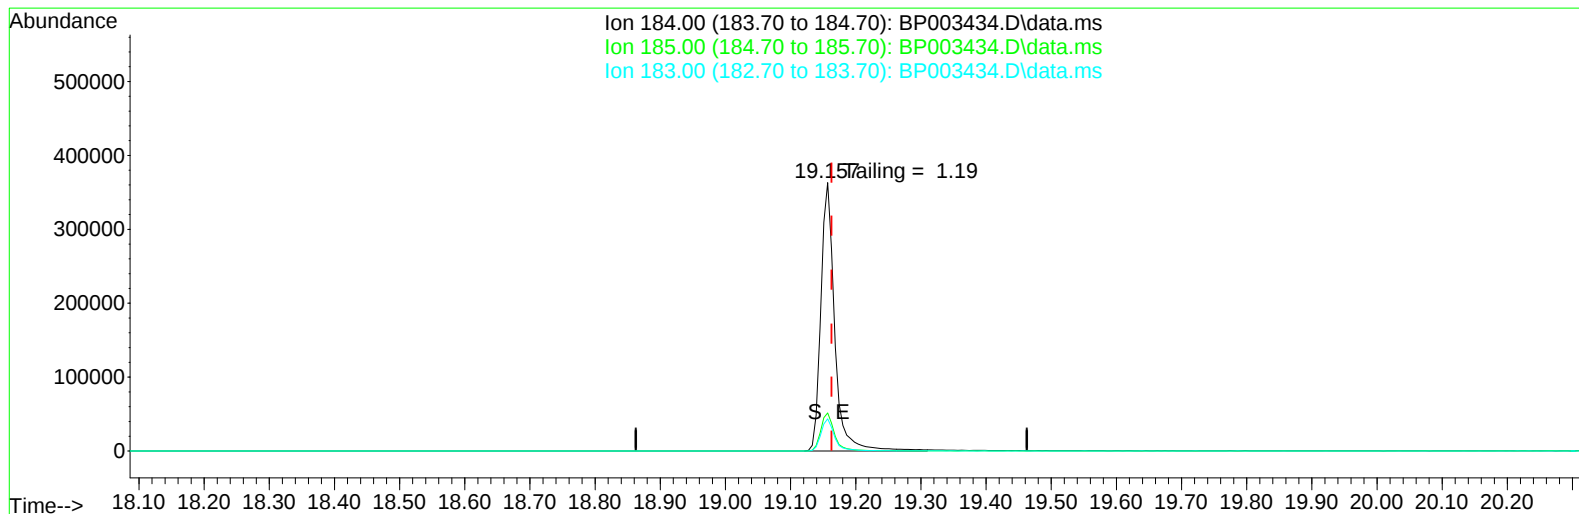

TIC: BP003434.D\data.ms

**(77) Benzidine**

19.157min (-0.006) 266870.02 ng

response 537896

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.18  |
| 183.00 | 12.00  | 12.01  |
| 0.00   | 0.00   | 0.00   |