

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100120\
 Data File : BP003436.D
 Acq On : 01 Oct 2020 14:10
 Operator : CG/JU
 Sample : PB131974BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB131974BL

Quant Time: Oct 01 14:47:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 01 10:05:32 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.528	152	74781	20.00	ng	# 0.00
21) Naphthalene-d8	10.310	136	293208	20.00	ng	# 0.00
39) Acenaphthene-d10	14.187	164	178470	20.00	ng	0.00
64) Phenanthrene-d10	16.945	188	408826	20.00	ng	# 0.00
76) Chrysene-d12	21.051	240	470294	20.00	ng	-0.01
86) Perylene-d12	23.239	264	480892	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.146	112	498217	116.33	ng	0.00
7) Phenol-d6	6.740	99	624242	109.35	ng	0.00
23) Nitrobenzene-d5	8.681	82	414285	83.01	ng	0.00
42) 2,4,6-Tribromophenol	15.698	330	230063	84.52	ng	0.00
45) 2-Fluorobiphenyl	12.804	172	886994	72.69	ng	0.00
79) Terphenyl-d14	19.527	244	1462241	64.78	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100120\
Data File : BP003436.D
Acq On : 01 Oct 2020 14:10
Operator : CG/JU
Sample : PB131974BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131974BL


Quant Time: Oct 01 14:47:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 10:05:32 2020
Response via : Initial Calibration

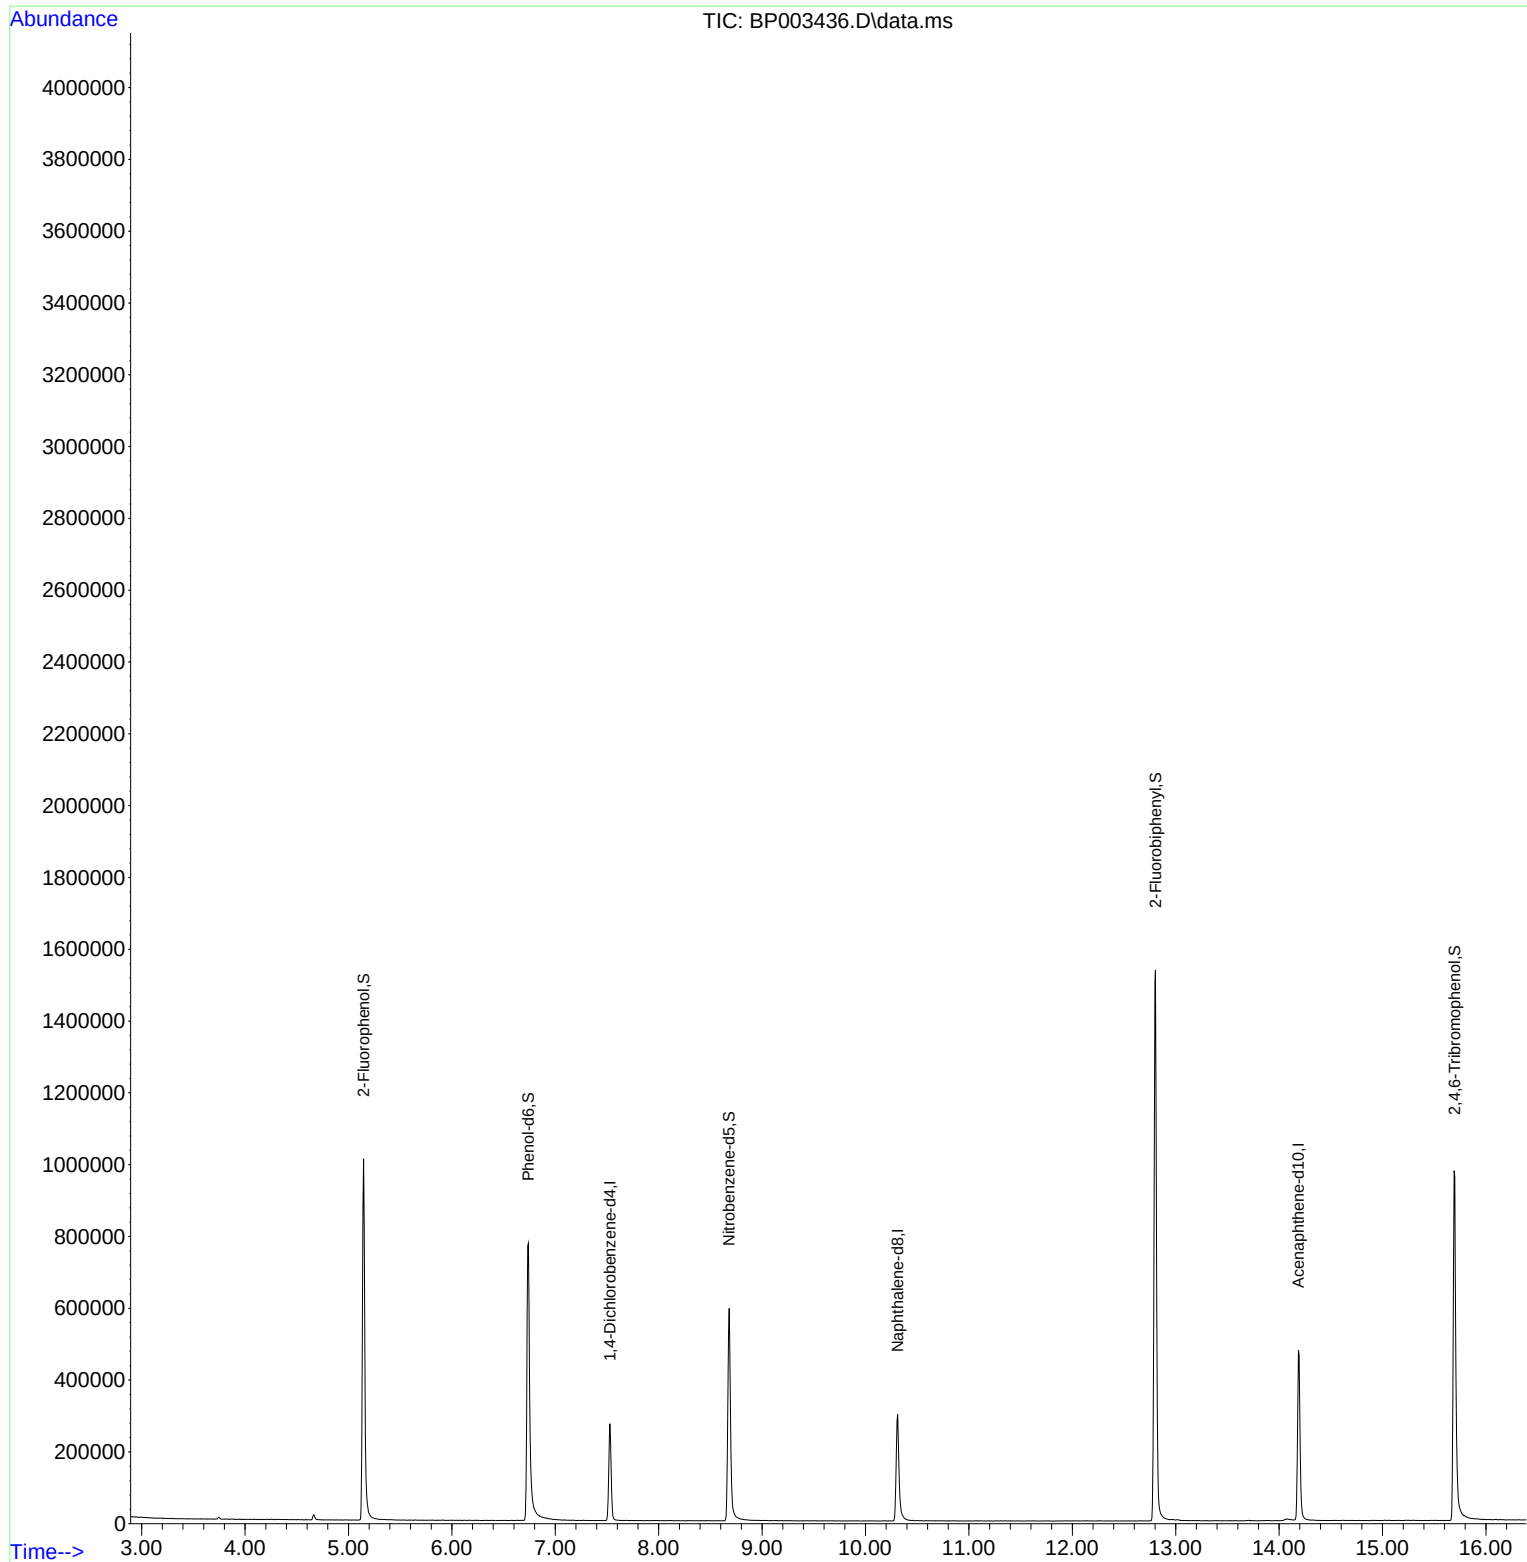


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100120\
Data File : BP003436.D
Acq On : 01 Oct 2020 14:10
Operator : CG/JU
Sample : PB131974BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131974BL

Quant Time: Oct 01 14:47:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 10:05:32 2020
Response via : Initial Calibration




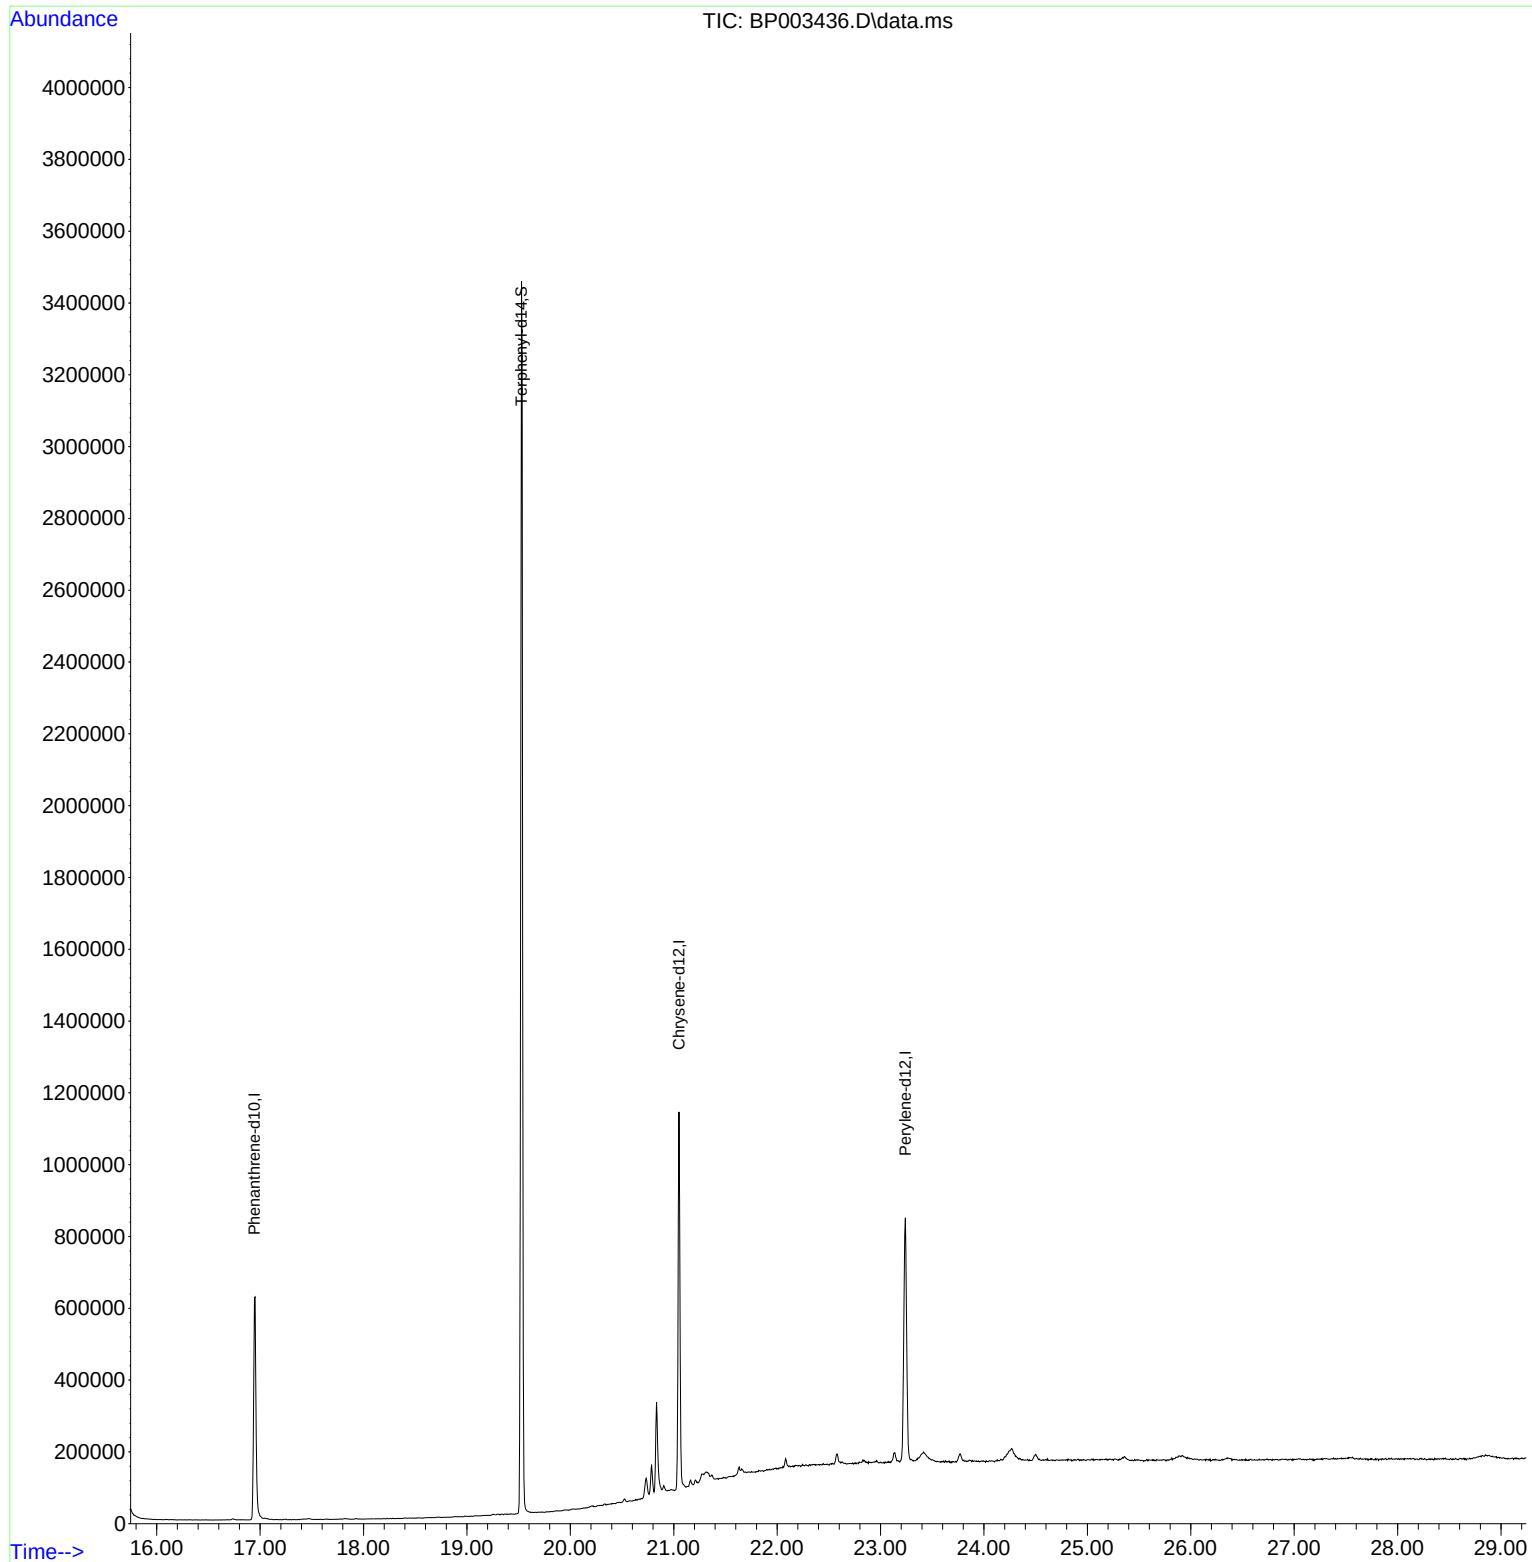


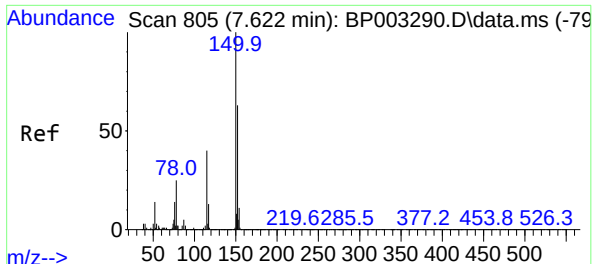

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.528 min Scan# 789
Delta R.T. -0.006 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10




Instrument :
BNA_P
ClientSampleId :
PB131974BL


Tgt Ion:152 Resp: 74781
Ion Ratio Lower Upper
152 100
150 159.9 123.8 185.6
115 65.9 43.8 65.6#

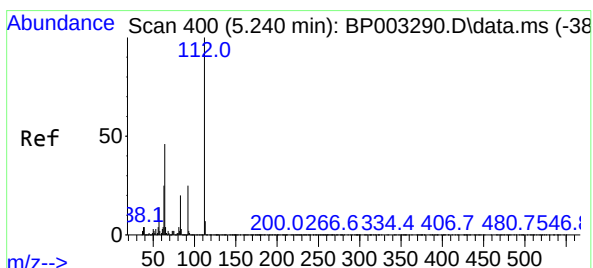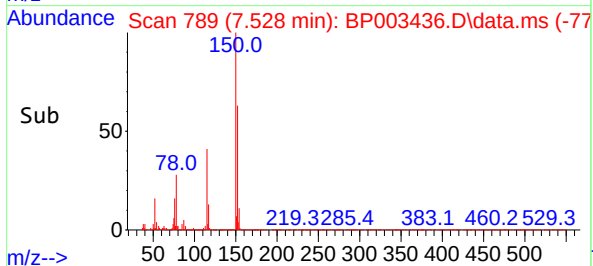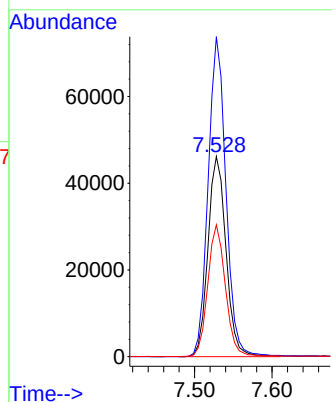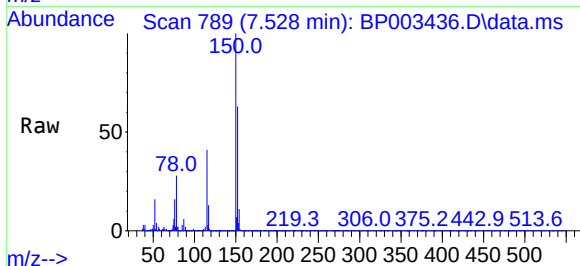

#5
2-Fluorophenol
Concen: 116.33 ng
RT: 5.146 min Scan# 384
Delta R.T. -0.006 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10

Tgt Ion:112 Resp: 498217
Ion Ratio Lower Upper
112 100
64 49.2 32.8 49.2#
63 26.5 17.0 25.4#

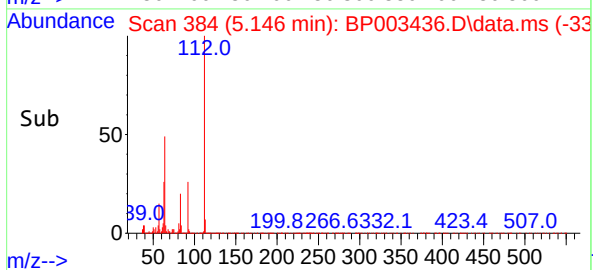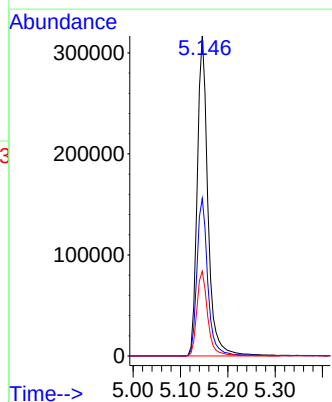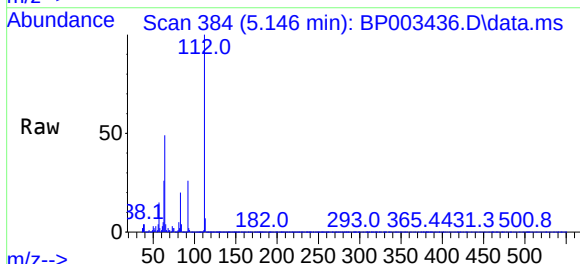




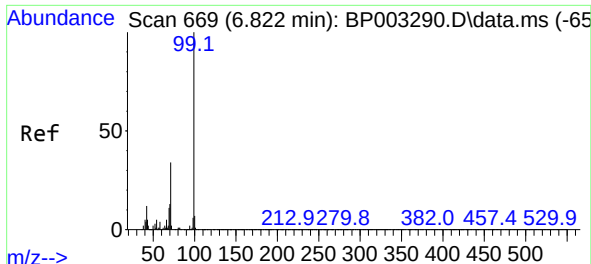


#7
Phenol-d6
Concen: 109.35 ng
RT: 6.740 min Scan# 655
Delta R.T. -0.000 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10

Instrument :
BNA_P
ClientSampleId :
PB131974BL

Tgt Ion: 99 Resp: 624242




Ion	Ratio	Lower	Upper
99	100		
42	12.4	8.6	13.0
71	34.6	23.4	35.2

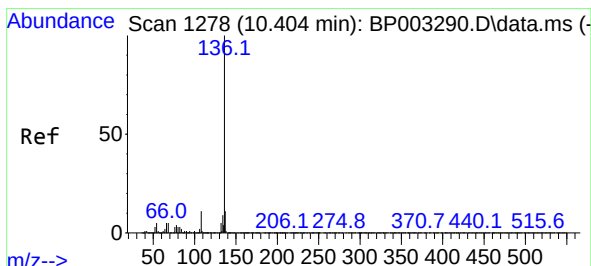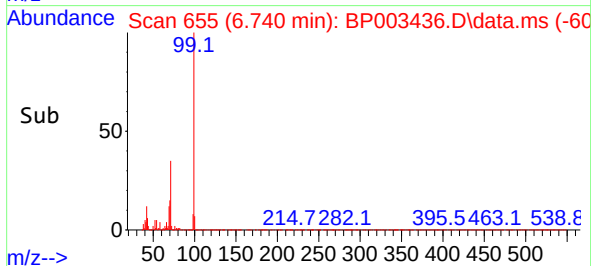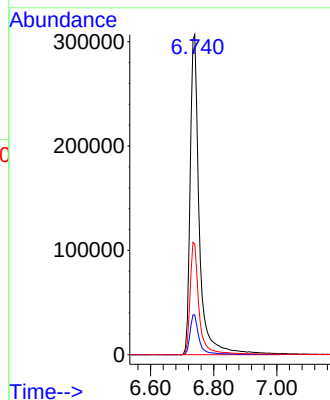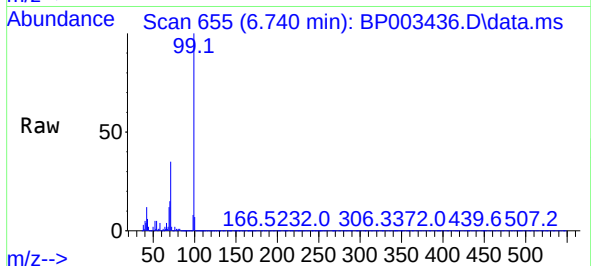


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.310 min Scan# 1262
Delta R.T. -0.000 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10

Tgt Ion: 136 Resp: 293208

Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.6	13.0
54	5.5	3.6	5.4#
68	6.1	3.3	4.9#


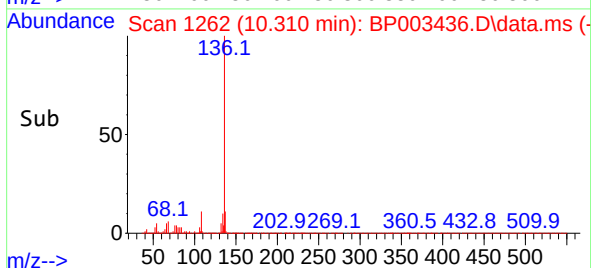
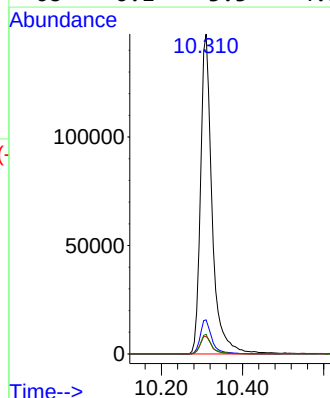
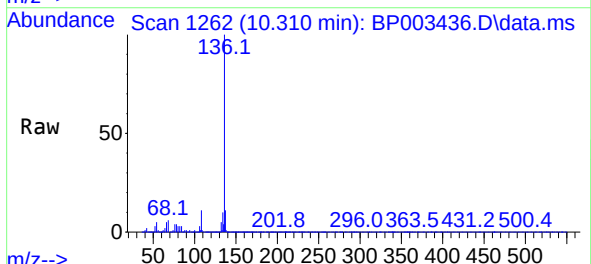


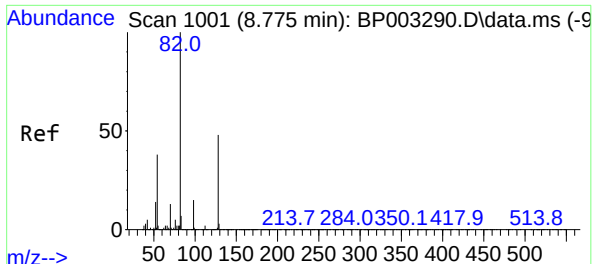

#23
Nitrobenzene-d5
Concen: 83.01 ng
RT: 8.681 min Scan# 985
Delta R.T. -0.006 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10




Instrument :
BNA_P
ClientSampleId :
PB131974BL


Tgt Ion: 82 Resp: 414285
Ion Ratio Lower Upper
82 100
128 43.1 45.6 68.4#
54 37.8 30.1 45.1

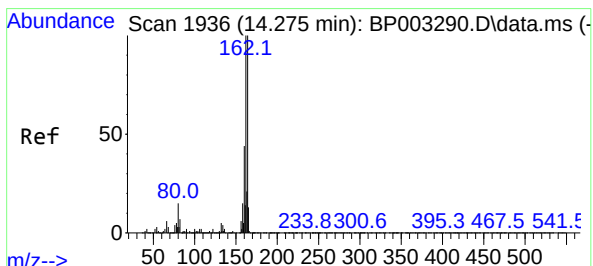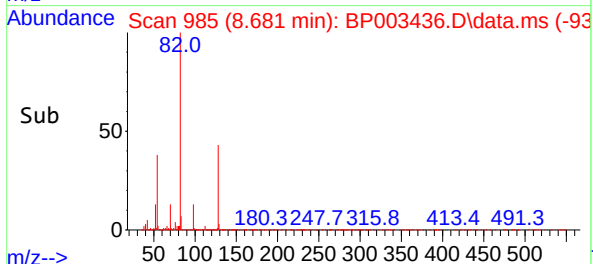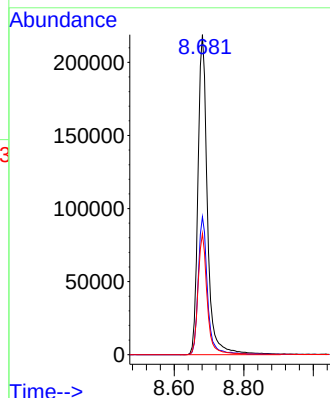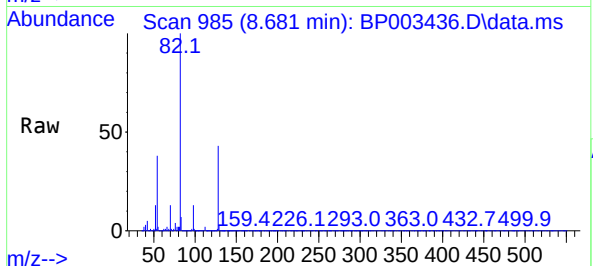

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.187 min Scan# 1921
Delta R.T. -0.006 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10

Tgt Ion:164 Resp: 178470
Ion Ratio Lower Upper
164 100
162 98.9 79.4 119.2
160 44.8 36.1 54.1


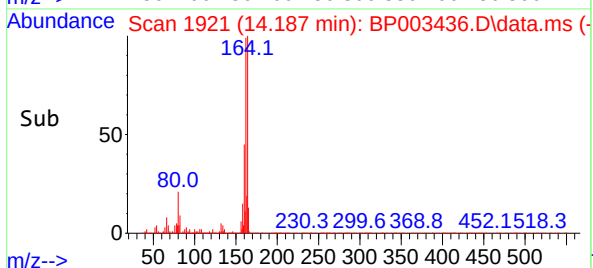
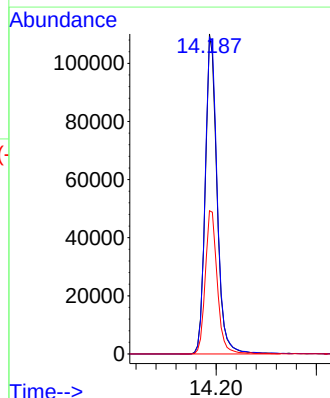
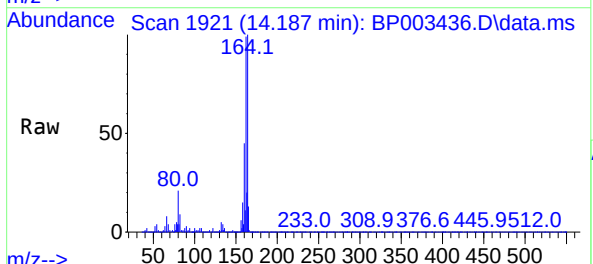


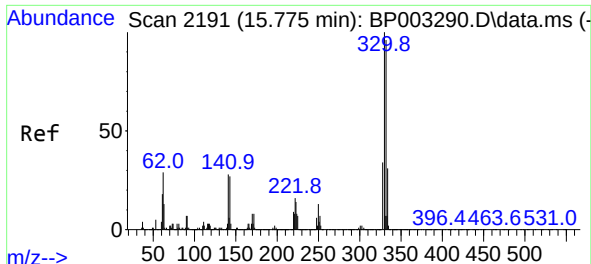

#42
2,4,6-Tribromophenol
Concen: 84.52 ng
RT: 15.698 min Scan# 2178
Delta R.T. 0.006 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10




Instrument :
BNA_P
ClientSampleId :
PB131974BL


Tgt Ion:330 Resp: 230063
Ion Ratio Lower Upper
330 100
332 96.4 77.1 115.7
141 36.9 23.4 35.2#

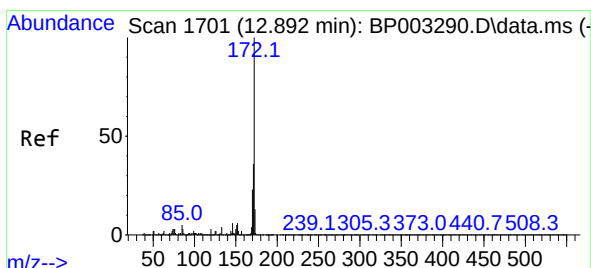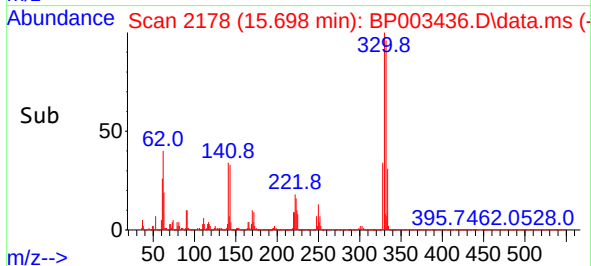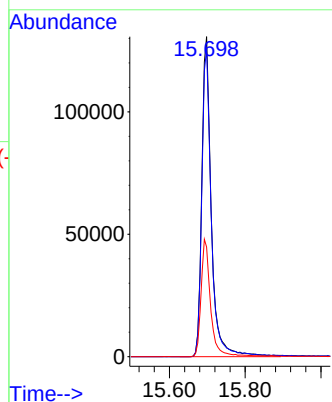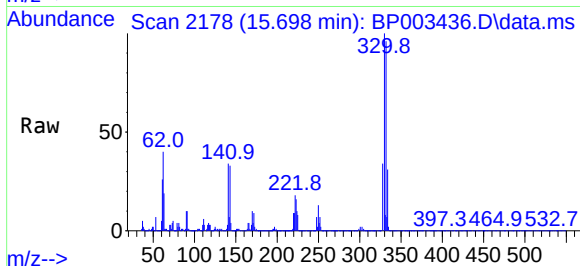

#45
2-Fluorobiphenyl
Concen: 72.69 ng
RT: 12.804 min Scan# 1686
Delta R.T. -0.000 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10

Tgt Ion:172 Resp: 886994
Ion Ratio Lower Upper
172 100
171 35.4 28.5 42.7
170 23.6 19.2 28.8


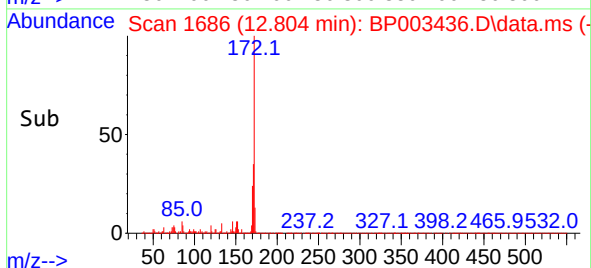
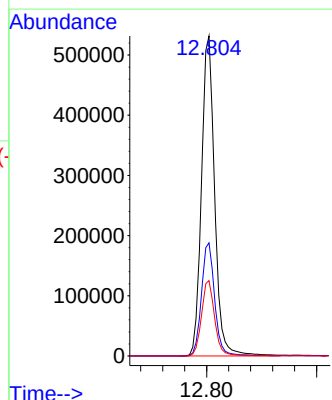
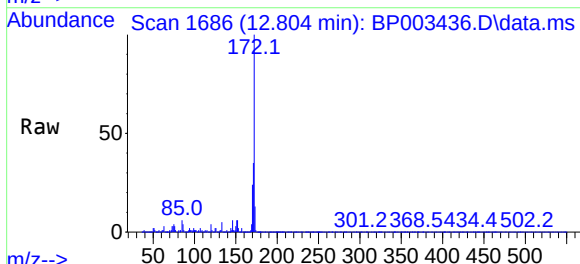


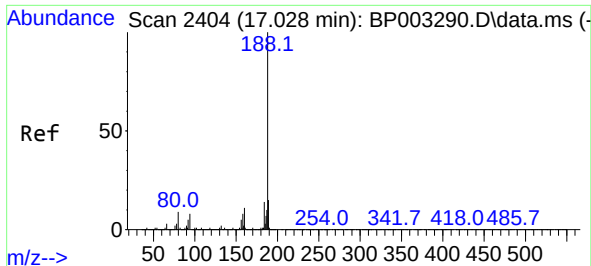

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 16.945 min Scan# 2390
Delta R.T. -0.000 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10




Instrument :
BNA_P
ClientSampleId :
PB131974BL


Tgt Ion:188 Resp: 408826
Ion Ratio Lower Upper
188 100
94 9.6 6.2 9.2#
80 10.6 6.2 9.2#

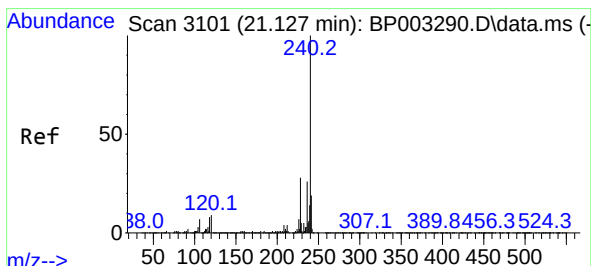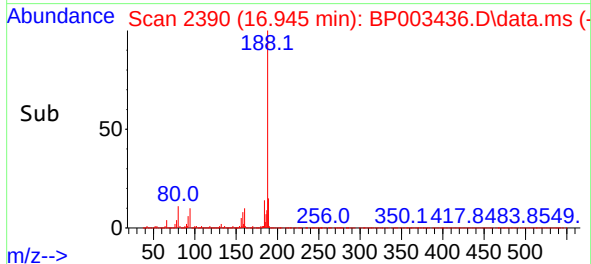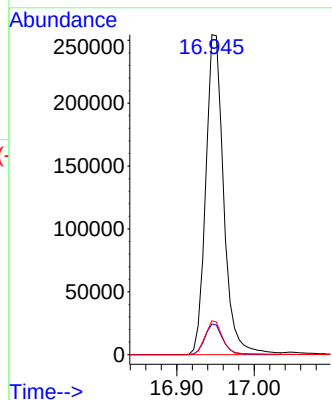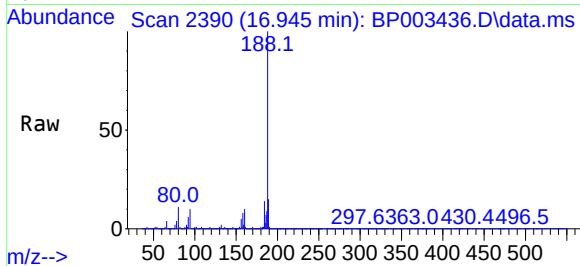

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.051 min Scan# 3088
Delta R.T. -0.012 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10

Tgt Ion:240 Resp: 470294
Ion Ratio Lower Upper
240 100
120 11.0 7.8 11.6
236 25.8 20.8 31.2


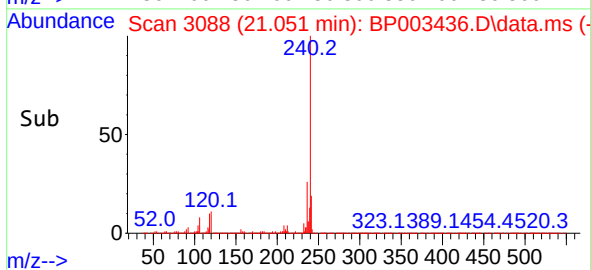
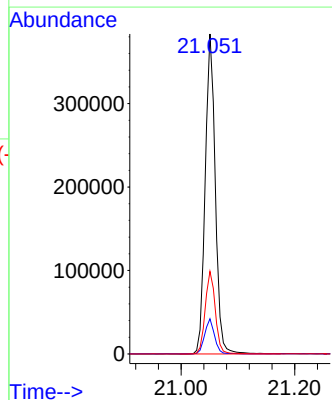
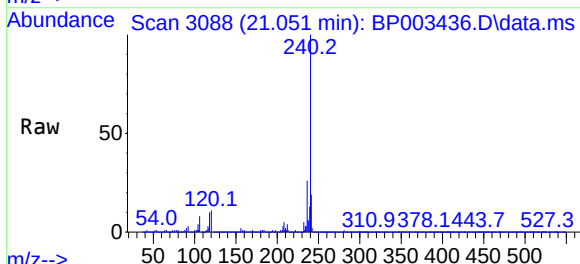


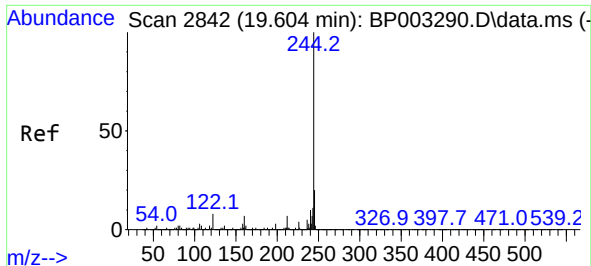

#79
Terphenyl-d14
Concen: 64.78 ng
RT: 19.527 min Scan# 2829
Delta R.T. -0.006 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10

Instrument :
BNA_P
ClientSampleId :
PB131974BL

Tgt Ion:244 Resp: 1462241
Ion Ratio Lower Upper
244 100
212 7.7 5.8 8.6
122 10.2 7.8 11.8

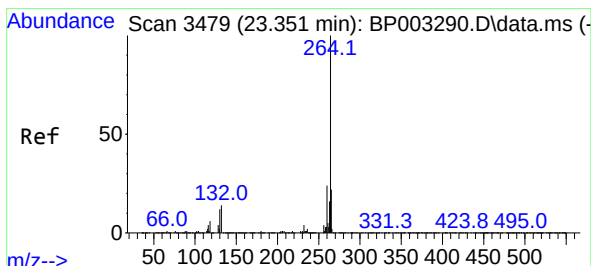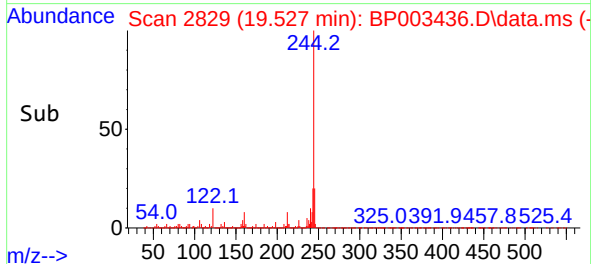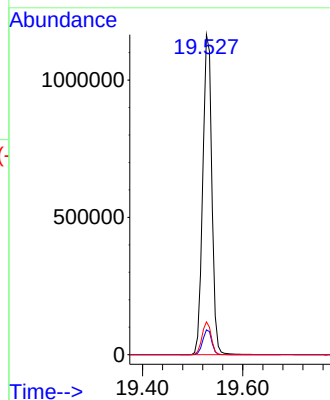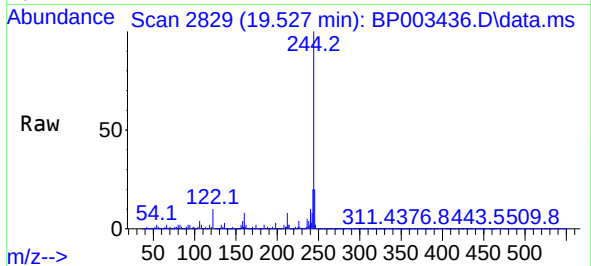

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.239 min Scan# 3460
Delta R.T. -0.018 min
Lab File: BP003436.D
Acq: 01 Oct 2020 14:10

Tgt Ion:264 Resp: 480892
Ion Ratio Lower Upper
264 100
260 24.4 18.8 28.2
265 21.9 17.4 26.2

