

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100120\
 Data File : BP003438.D
 Acq On : 01 Oct 2020 15:18
 Operator : CG/JU
 Sample : PB132022BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132022BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.146	378	384	412	rBV	1388267	2175701	36.95%	8.919%
2	6.734	647	654	692	rBV	1103355	2172505	36.90%	8.906%
3	7.528	782	789	803	rBV	297347	464688	7.89%	1.905%
4	8.681	977	985	1009	rBV	825731	1534195	26.06%	6.289%
5	10.310	1254	1262	1282	rBV	318673	645133	10.96%	2.645%
6	12.798	1678	1685	1709	rBV	2060795	3553962	60.36%	14.569%
7	14.186	1914	1921	1944	rVB2	527150	886049	15.05%	3.632%
8	15.692	2170	2177	2207	rBV	1350439	2523691	42.86%	10.345%
9	16.945	2384	2390	2406	rBV	664781	1117240	18.98%	4.580%
10	19.527	2823	2829	2843	rBV	4567482	5887698	100.00%	24.136%
11	20.733	3029	3034	3038	rBV	52280	89879	1.53%	0.368%
12	20.786	3039	3043	3047	rVV	78801	103686	1.76%	0.425%
13	20.833	3047	3051	3060	rVV	260020	389177	6.61%	1.595%
14	21.051	3083	3088	3099	rBV	1131828	1421419	24.14%	5.827%
15	23.239	3453	3460	3472	rVB2	732992	1429176	24.27%	5.859%




Sum of corrected areas: 24394199

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100120\
Data File : BP003438.D
Acq On : 01 Oct 2020 15:18
Operator : CG/JU
Sample : PB132022BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132022BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

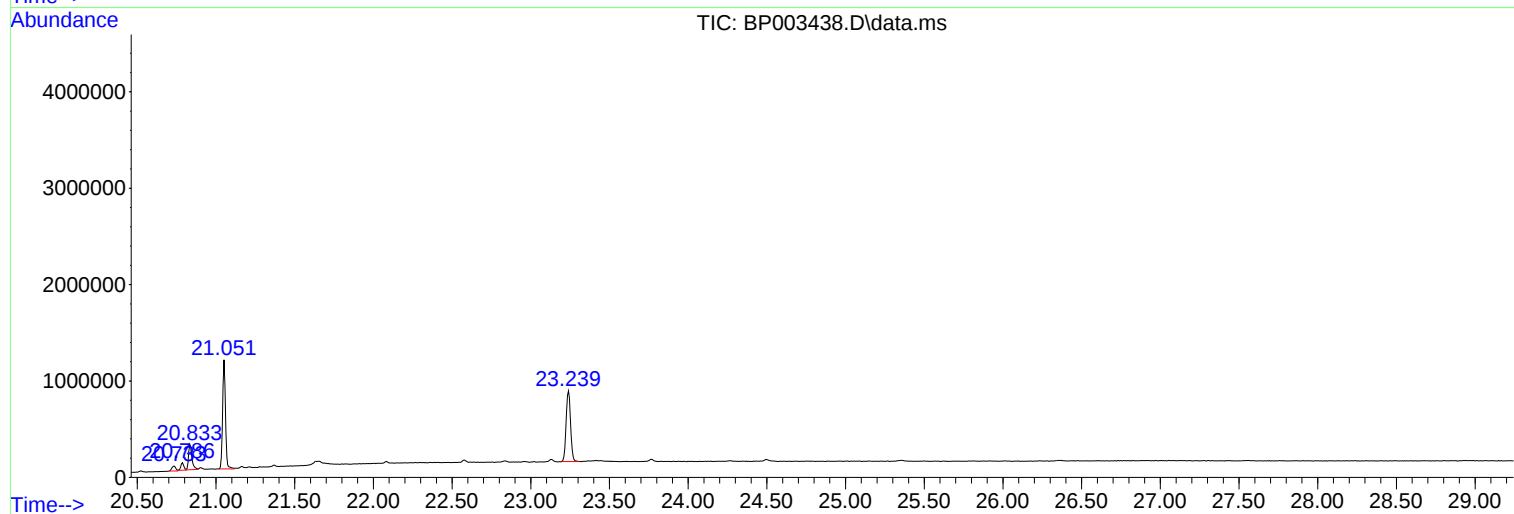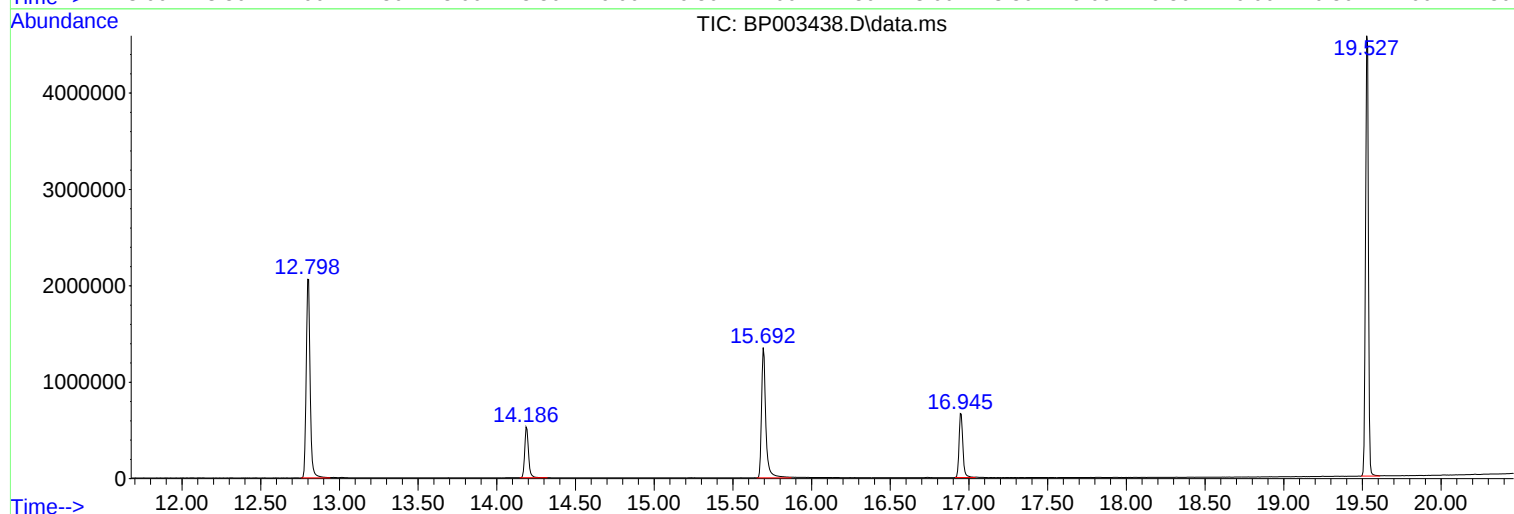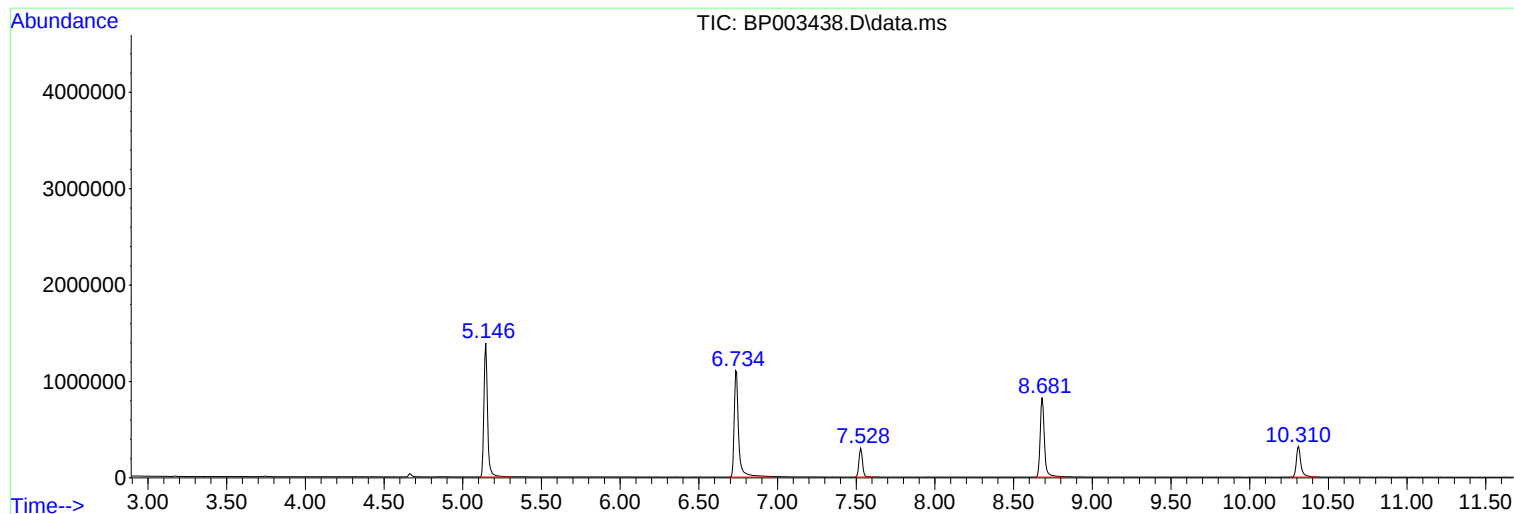

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100120\
Data File : BP003438.D
Acq On : 01 Oct 2020 15:18
Operator : CG/JU
Sample : PB132022BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132022BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethylene glycol dibenzoate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.833	5.48 ng	389177	Chrysene-d12	21.051

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	83
2			Benzoic acid, 2-(3-nitrophenyl)e...	271	C15H13NO4	1000368-22-4	78
3			2,2'-(Ethane-1,2-diylbis(oxy))bi...	358	C20H22O6	1000366-99-4	74
4			2-(2-(2-Methoxyethoxy)ethoxy)eth...	268	C14H20O5	1000366-99-1	74
5			3,6,9,12-Tetraoxatetradecane-1,1...	446	C24H30O8	1000366-97-0	64

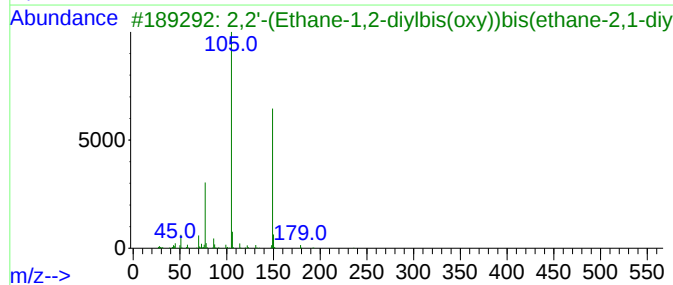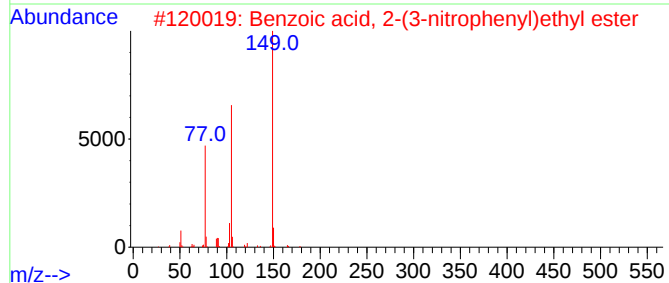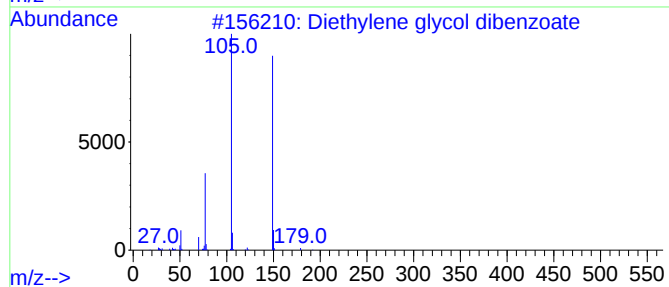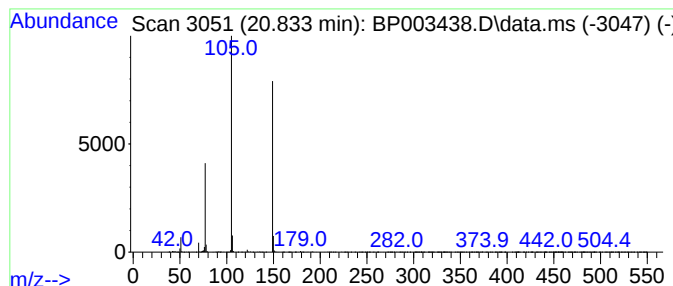

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100120\
Data File : BP003438.D
Acq On : 01 Oct 2020 15:18
Operator : CG/JU
Sample : PB132022BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132022BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethylene glyc...	20.833	5.5	ng	389177	5	21.051	1421420	20.0