


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100120\
 Data File : BP003434.D
 Acq On : 01 Oct 2020 12:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 02 11:17:24 2020

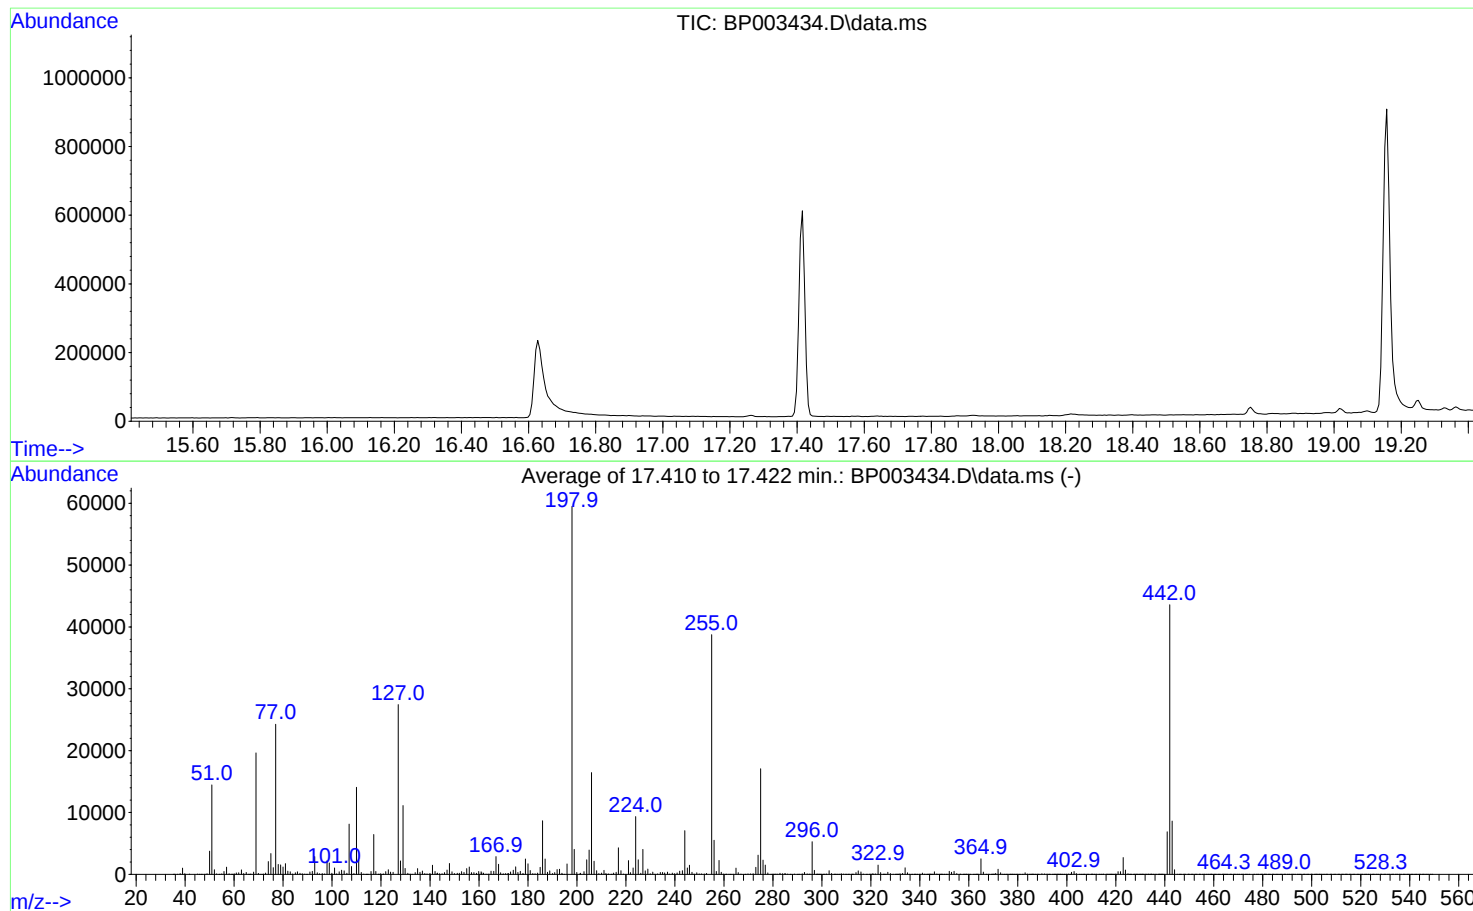

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.3	14450	PASS
68	69	0.00	2	1.9	375	PASS
69	198	0.00	100	33.0	19640	PASS
70	69	0.00	2	0.9	169	PASS
127	198	10	80	46.2	27456	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59475	PASS
199	198	5	9	6.8	4026	PASS
275	198	10	60	28.7	17071	PASS
365	198	1	100	4.2	2512	PASS
441	198	0.01	100	11.6	6877	PASS
442	198	50	100	73.3	43600	PASS
443	442	15	24	19.8	8624	PASS