




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
Data File : BP022136.D
Acq On : 01 Oct 2024 15:10
Operator : RC/JU
Sample : P4010-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AW9

Manual IntegrationsAPPROVED

Quant Time: Oct 01 23:59:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

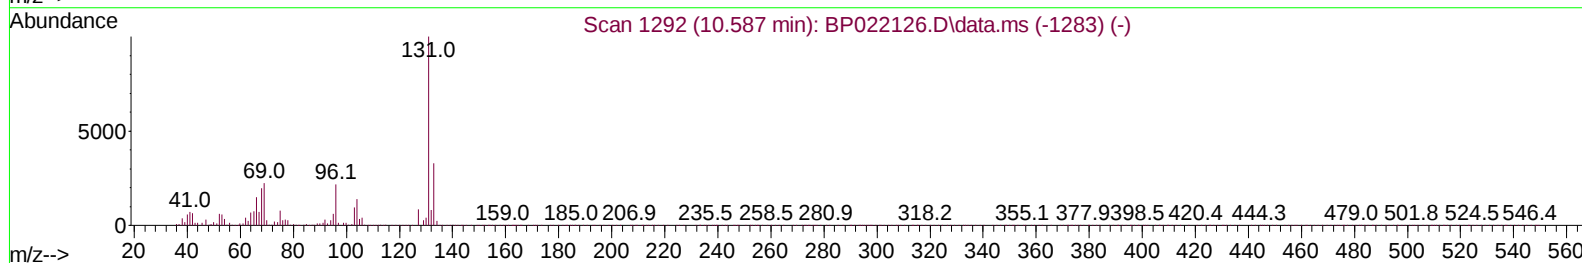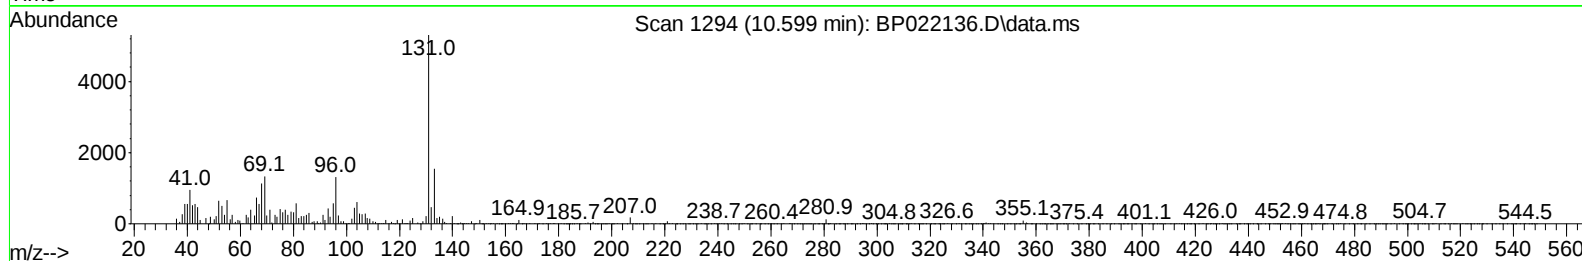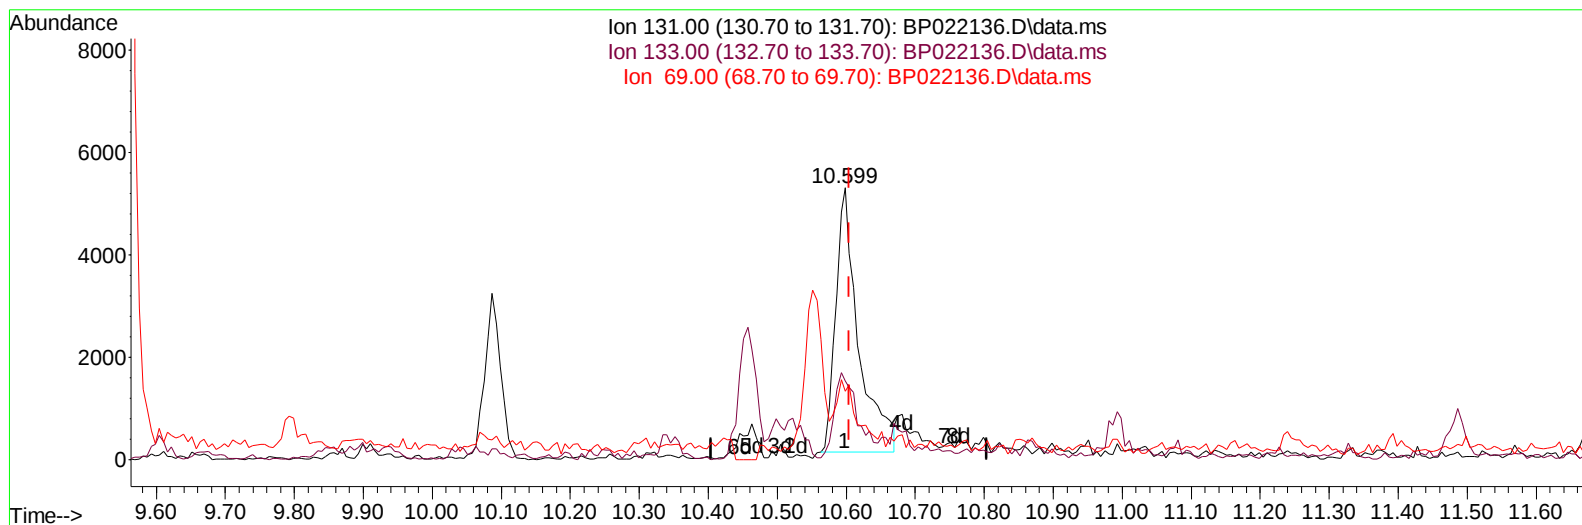

TIC: BP022136.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.599min (-0.006) 0.96 ng/u1

response 11825

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.90	29.00
69.00	22.40	25.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
Data File : BP022136.D
Acq On : 01 Oct 2024 15:10
Operator : RC/JU
Sample : P4010-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AW9

Manual IntegrationsAPPROVED

Quant Time: Oct 01 23:59:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

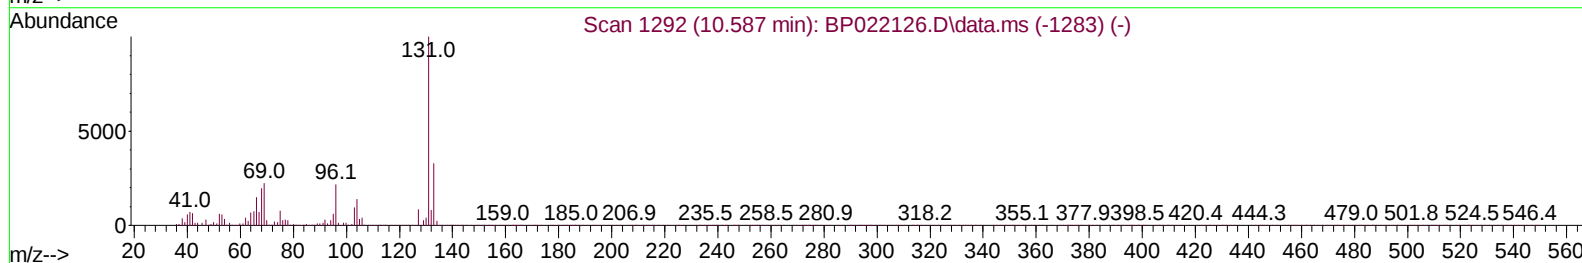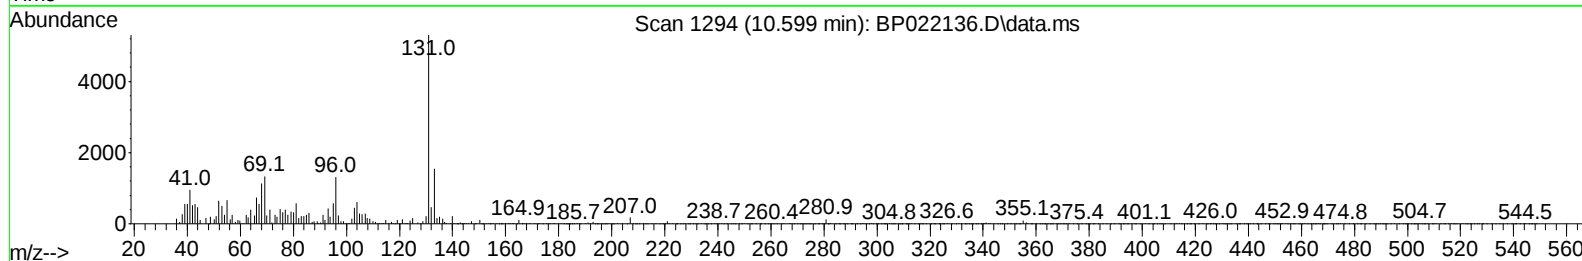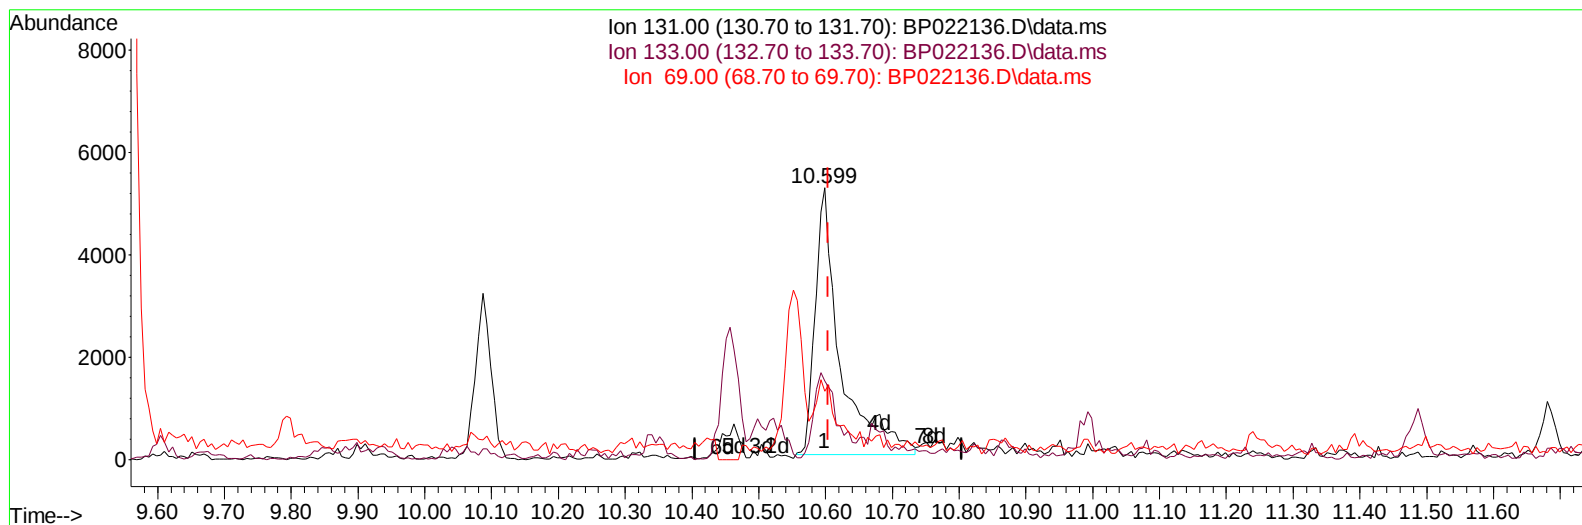

TIC: BP022136.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.599min (-0.006) 1.11 ng/ul m

response 13686

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.90	29.00
69.00	22.40	25.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
Data File : BP022136.D
Acq On : 01 Oct 2024 15:10
Operator : RC/JU
Sample : P4010-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AW9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

Quant Time: Oct 01 23:57:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

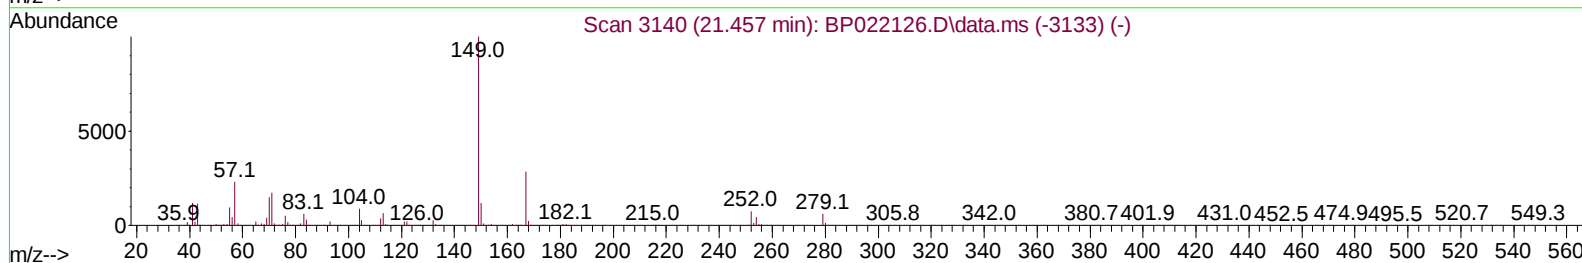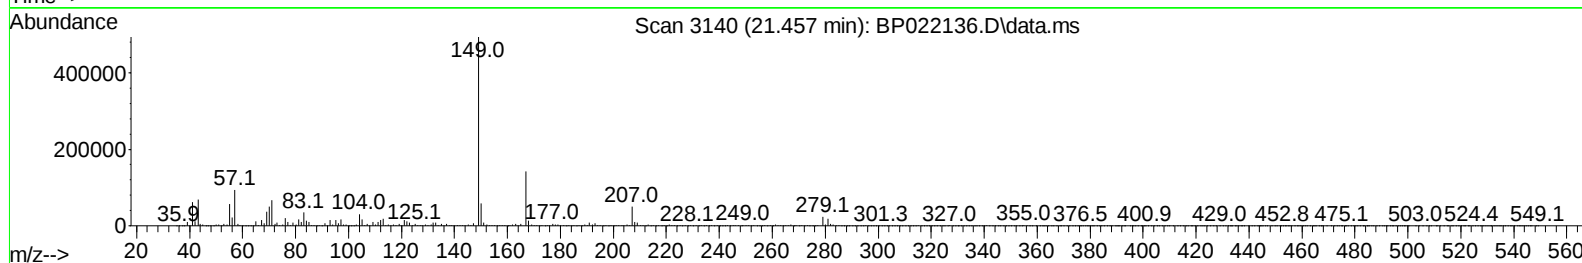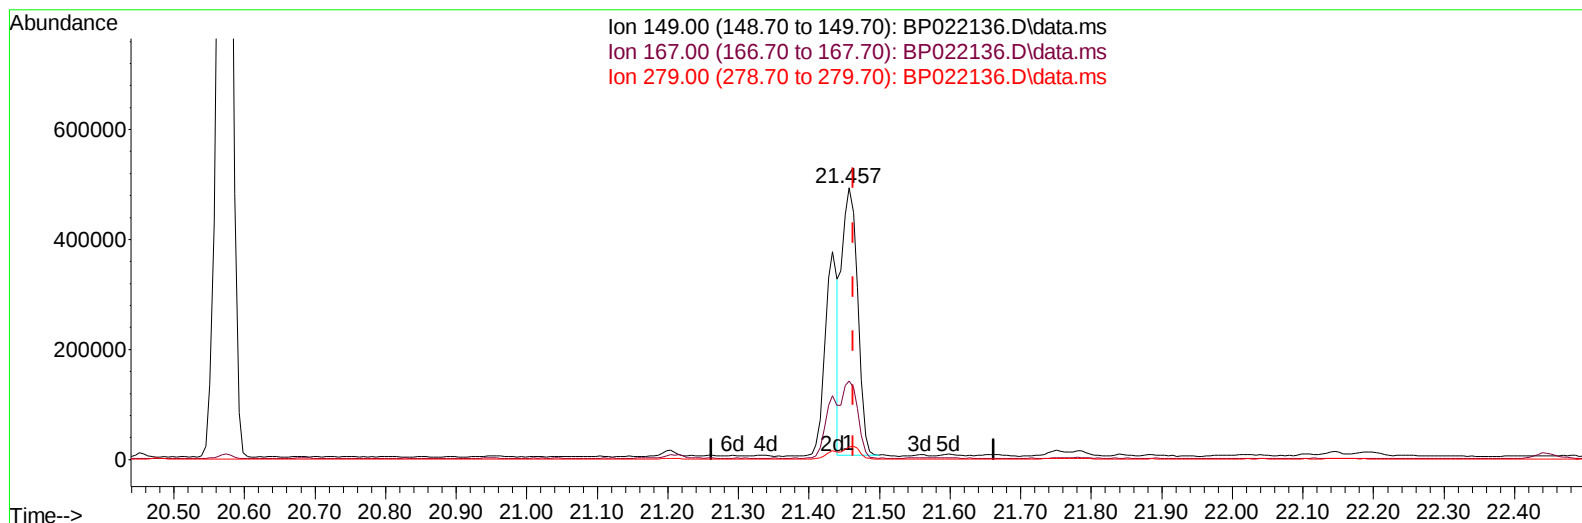

TIC: BP022136.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.457min (-0.006) 24.15 ng/u1

response 770286

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	28.70	28.97
279.00	5.60	4.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
Data File : BP022136.D
Acq On : 01 Oct 2024 15:10
Operator : RC/JU
Sample : P4010-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AW9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

Quant Time: Oct 01 23:57:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

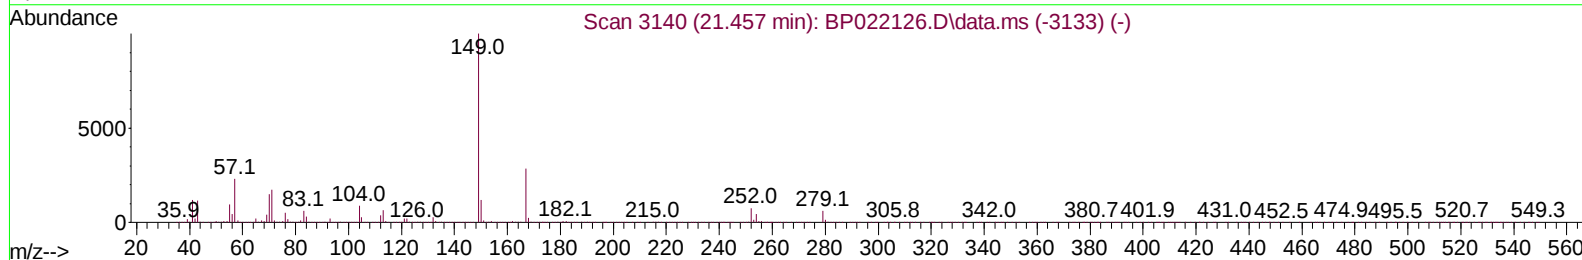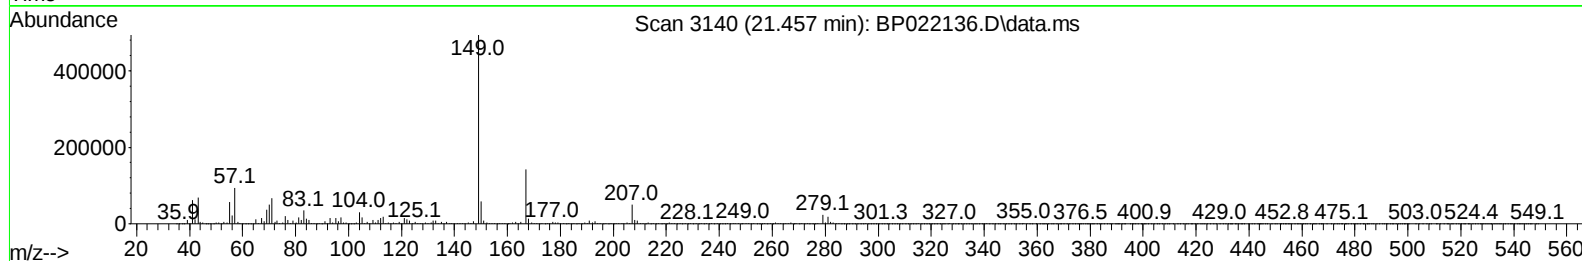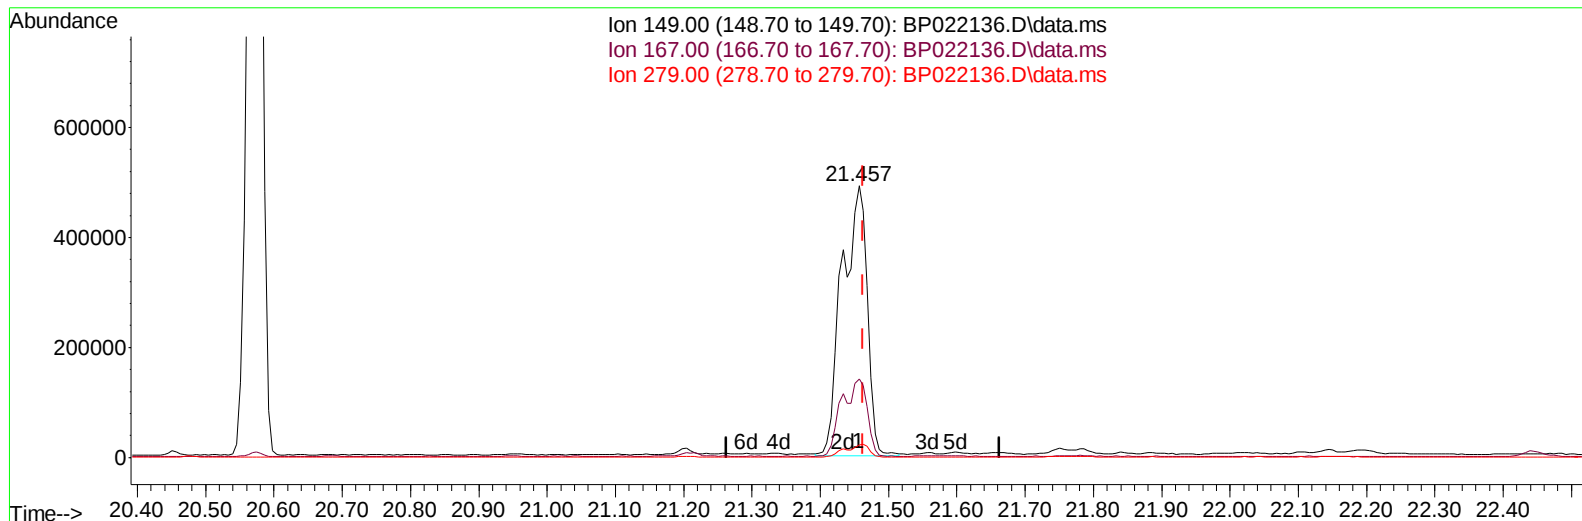

TIC: BP022136.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.457min (-0.006) 39.50 ng/ul m

response 1260069

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	28.70	28.97
279.00	5.60	4.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
 Data File : BP022136.D
 Acq On : 01 Oct 2024 15:10
 Operator : RC/JU
 Sample : P4010-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AW9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/02/2024
 Supervised By :mohammad ahmed 10/04/2024

Quant Time: Oct 02 00:00:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	148931	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.457	136	560031	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.310	164	416389	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.104	188	964437	20.000	ng/ul	-0.01
79) Chrysene-d12	21.539	240	978844	20.000	ng/ul	0.00
88) Perylene-d12	24.827	264	1176606	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	8122	2.136	ng/uL	0.00
4) Pyridine-d5	3.646	84	15167	1.396	ng/ul	0.01
7) Phenol-d5	6.881	99	170825	14.022	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.040	67	103444	13.790	ng/ul	0.00
11) 2-Chlorophenol-d4	7.234	132	134389	15.247	ng/ul	-0.01
15) 4-Methylphenol-d8	8.399	113	120982	12.532	ng/ul	0.00
21) Nitrobenzene-d5	8.840	128	62328	14.870	ng/ul	0.00
24) 2-Nitrophenol-d4	9.552	143	71675	15.081	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.087	165	149407	14.476	ng/ul	0.00
31) 4-Chloroaniline-d4	10.599	131	13686m	1.111	ng/ul	0.00
46) Dimethylphthalate-d6	13.710	166	473713	14.717	ng/ul	-0.01
49) Acenaphthylene-d8	13.998	160	498933	14.641	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143	60727	11.030	ng/ul	-0.01
60) Fluorene-d10	15.316	176	416978	14.645	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.434	200	69622	11.628	ng/ul	-0.01
73) Anthracene-d10	17.198	188	562645	12.497	ng/ul	-0.02
81) Pyrene-d10	19.586	212	733823	14.470	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.610	264	613015	9.906	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.852	77	7562	1.097	ng/ul	94
8) Phenol	6.910	94	22258	1.751	ng/ul	96
16) Acetophenone	8.510	105	95436	5.943	ng/ul	97
78) Di-n-butylphthalate	18.116	149	89268	1.707	ng/ul	98
83) Butylbenzylphthalate	20.574	149	2988786	137.456	ng/ul	92
86) Bis(2-ethylhexyl)phtha...	21.457	149	1260069m	39.498	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
Data File : BP022136.D
Acq On : 01 Oct 2024 15:10
Operator : RC/JU
Sample : P4010-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AW9

Manual IntegrationsAPPROVED

Quant Time: Oct 02 00:00:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

