

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
 Data File : BP022149.D
 Acq On : 02 Oct 2024 00:40
 Operator : RC/JU
 Sample : P4022-08DL 50X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCA6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022149.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.952	161	164	173	rVB2	6472	10838	0.44%	0.084%
2	4.869	313	320	327	rVB4	4111	7257	0.29%	0.057%
3	5.381	404	407	410	rBV5	2565	4289	0.17%	0.033%
4	5.746	464	469	476	rBV7	3452	6051	0.25%	0.047%
5	6.622	614	618	625	rVB6	4102	6789	0.28%	0.053%
6	6.699	625	631	636	rBV3	3194	5999	0.24%	0.047%
7	6.805	642	649	654	rBV	11705	18288	0.74%	0.142%
8	6.863	654	659	667	rVV5	9819	18926	0.77%	0.147%
9	6.934	667	671	677	rVB2	9907	15910	0.65%	0.124%
10	7.040	684	689	694	rBV	5276	8825	0.36%	0.069%
11	7.099	694	699	702	rVV2	9576	16327	0.66%	0.127%
12	7.134	702	705	711	rVB2	13609	20474	0.83%	0.160%
13	7.228	715	721	727	rBV3	18137	33116	1.34%	0.258%
14	7.352	734	742	750	rVB	26948	45448	1.84%	0.354%
15	7.699	794	801	807	rBV	379867	605090	24.56%	4.715%
16	7.763	807	812	817	rVV	53860	82884	3.36%	0.646%
17	7.810	817	820	827	rVV4	13790	23601	0.96%	0.184%
18	7.928	835	840	844	rBV6	4129	7081	0.29%	0.055%
19	8.058	857	862	868	rBV8	2058	3964	0.16%	0.031%
20	8.122	868	873	877	rVV5	2662	4082	0.17%	0.032%
21	8.175	877	882	888	rVV7	5020	10159	0.41%	0.079%
22	8.240	888	893	897	rVV3	3732	6215	0.25%	0.048%
23	8.328	900	908	913	rBV3	9421	15770	0.64%	0.123%
24	8.405	913	921	928	rVV5	4803	11982	0.49%	0.093%
25	8.493	932	936	944	rVB4	5398	10572	0.43%	0.082%
26	8.634	955	960	965	rBV2	6519	9824	0.40%	0.077%
27	8.687	965	969	976	rVB4	7083	11089	0.45%	0.086%
28	8.793	981	987	991	rBV4	6392	11368	0.46%	0.089%
29	8.852	991	997	1003	rBV6	4697	10809	0.44%	0.084%
30	8.969	1011	1017	1022	rVB7	4079	6850	0.28%	0.053%
31	9.110	1034	1041	1047	rBV4	16829	26413	1.07%	0.206%
32	9.175	1047	1052	1056	rBV7	2601	4275	0.17%	0.033%
33	9.357	1079	1083	1089	rBV4	3596	7131	0.29%	0.056%
34	9.475	1096	1103	1110	rVB9	4738	10099	0.41%	0.079%
35	9.557	1110	1117	1122	rBV10	5447	12992	0.53%	0.101%
36	9.622	1122	1128	1134	rVB2	9504	18157	0.74%	0.141%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
 Data File : BP022149.D
 Acq On : 02 Oct 2024 00:40
 Operator : RC/JU
 Sample : P4022-08DL 50X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCA6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	9.716	1140	1144	1149	rVB6	2541	4379	0.18%	0.034%
38	9.857	1162	1168	1176	rBV6	4209	9839	0.40%	0.077%
39	10.099	1203	1209	1215	rVV5	7827	14988	0.61%	0.117%
40	10.152	1215	1218	1225	rVB9	3169	6100	0.25%	0.048%
41	10.457	1263	1270	1277	rBV	501592	822589	33.39%	6.410%
42	10.575	1285	1290	1298	rVB10	8221	15486	0.63%	0.121%
43	10.769	1319	1323	1328	rVB7	3431	6693	0.27%	0.052%
44	10.834	1328	1334	1341	rBV	21439	33822	1.37%	0.264%
45	10.904	1341	1346	1348	rBV6	2432	3720	0.15%	0.029%
46	10.963	1352	1356	1362	rVB8	2486	4185	0.17%	0.033%
47	11.310	1411	1415	1418	rVV6	2152	3885	0.16%	0.030%
48	11.346	1418	1421	1428	rVB8	4249	6810	0.28%	0.053%
49	11.546	1452	1455	1462	rVB4	4230	7789	0.32%	0.061%
50	11.722	1475	1485	1490	rVB4	5977	14257	0.58%	0.111%
51	11.869	1506	1510	1514	rBV6	5407	8749	0.36%	0.068%
52	11.916	1514	1518	1524	rVV2	10405	16616	0.67%	0.129%
53	11.987	1524	1530	1532	rVV5	3253	5582	0.23%	0.043%
54	12.057	1540	1542	1546	rVV5	3259	4725	0.19%	0.037%
55	12.116	1546	1552	1564	rVB5	12569	26685	1.08%	0.208%
56	12.298	1577	1583	1586	rBV7	3477	7699	0.31%	0.060%
57	12.334	1586	1589	1596	rVB2	7813	12083	0.49%	0.094%
58	12.534	1617	1623	1633	rVB3	13674	25436	1.03%	0.198%
59	12.716	1649	1654	1660	rBV7	3540	5748	0.23%	0.045%
60	12.875	1676	1681	1686	rVB3	6145	9541	0.39%	0.074%
61	13.045	1703	1710	1716	rBV4	7338	11336	0.46%	0.088%
62	13.128	1719	1724	1726	rBV6	3342	4242	0.17%	0.033%
63	13.257	1741	1746	1750	rBV4	4064	5793	0.24%	0.045%
64	13.351	1757	1762	1767	rVB7	5626	10192	0.41%	0.079%
65	13.475	1775	1783	1784	rBV8	4800	7932	0.32%	0.062%
66	13.563	1793	1798	1803	rBV4	8154	12213	0.50%	0.095%
67	13.616	1803	1807	1810	rVV5	5037	8584	0.35%	0.067%
68	13.657	1810	1814	1820	rVV4	15860	27950	1.13%	0.218%
69	13.716	1820	1824	1833	rVB	15762	26806	1.09%	0.209%
70	13.998	1867	1872	1876	rBV	16328	27420	1.11%	0.214%
71	14.040	1876	1879	1883	rVB2	6487	9092	0.37%	0.071%
72	14.216	1904	1909	1912	rVB7	4935	7616	0.31%	0.059%
73	14.310	1918	1925	1932	rBV	785887	1177741	47.81%	9.177%
74	14.616	1973	1977	1982	rBV5	4960	8934	0.36%	0.070%
75	14.692	1984	1990	1995	rVV10	6284	12272	0.50%	0.096%
76	14.763	1997	2002	2005	rVB7	3439	4703	0.19%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
 Data File : BP022149.D
 Acq On : 02 Oct 2024 00:40
 Operator : RC/JU
 Sample : P4022-08DL 50X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCA6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

77	14.857	2014	2018	2023	rBV9	5123	7624	0.31%	0.059%
78	14.945	2023	2033	2047	rVV	190770	319777	12.98%	2.492%
79	15.081	2051	2056	2059	rVV7	6028	10025	0.41%	0.078%
80	15.128	2060	2064	2070	rVV3	7369	12976	0.53%	0.101%
81	15.175	2070	2072	2078	rVB7	3974	5638	0.23%	0.044%
82	15.239	2080	2083	2088	rVB7	3166	4435	0.18%	0.035%
83	15.322	2088	2097	2104	rBV3	26708	49155	2.00%	0.383%
84	15.434	2110	2116	2120	rBV	12533	21437	0.87%	0.167%
85	15.698	2155	2161	2170	rVV5	9232	17609	0.71%	0.137%
86	16.157	2235	2239	2242	rBV5	6646	7583	0.31%	0.059%
87	16.263	2252	2257	2261	rBV8	1792	3944	0.16%	0.031%
88	16.604	2311	2315	2318	rVB4	6120	7979	0.32%	0.062%
89	16.757	2334	2341	2356	rBV	1574699	2463595	100.00%	19.196%
90	17.110	2393	2401	2411	rBV	1007728	1615239	65.56%	12.586%
91	17.210	2413	2418	2428	rVB	35885	64098	2.60%	0.499%
92	17.716	2500	2504	2506	rVB5	4969	6713	0.27%	0.052%
93	18.045	2557	2560	2565	rBV7	7414	13137	0.53%	0.102%
94	18.692	2666	2670	2674	rBV4	9539	12803	0.52%	0.100%
95	18.828	2691	2693	2697	rBV4	4111	4077	0.17%	0.032%
96	19.580	2817	2821	2832	rVB	45994	71935	2.92%	0.561%
97	20.257	2933	2936	2939	rBV3	24992	26750	1.09%	0.208%
98	20.927	3046	3050	3055	rBV3	45298	78857	3.20%	0.614%
99	21.539	3148	3154	3161	rVB2	1239384	2096653	85.11%	16.337%
100	24.827	3705	3713	3727	rVB	892906	2342652	95.09%	18.254%




Sum of corrected areas: 12833867

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
Data File : BP022149.D
Acq On : 02 Oct 2024 00:40
Operator : RC/JU
Sample : P4022-08DL 50X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCA6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

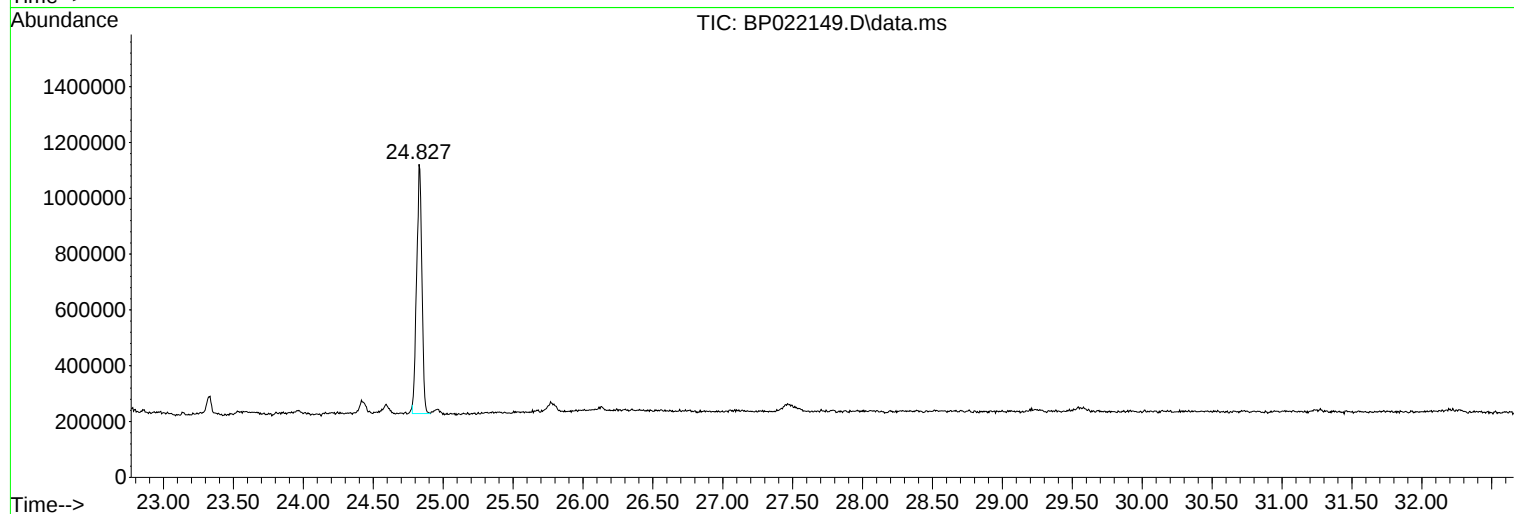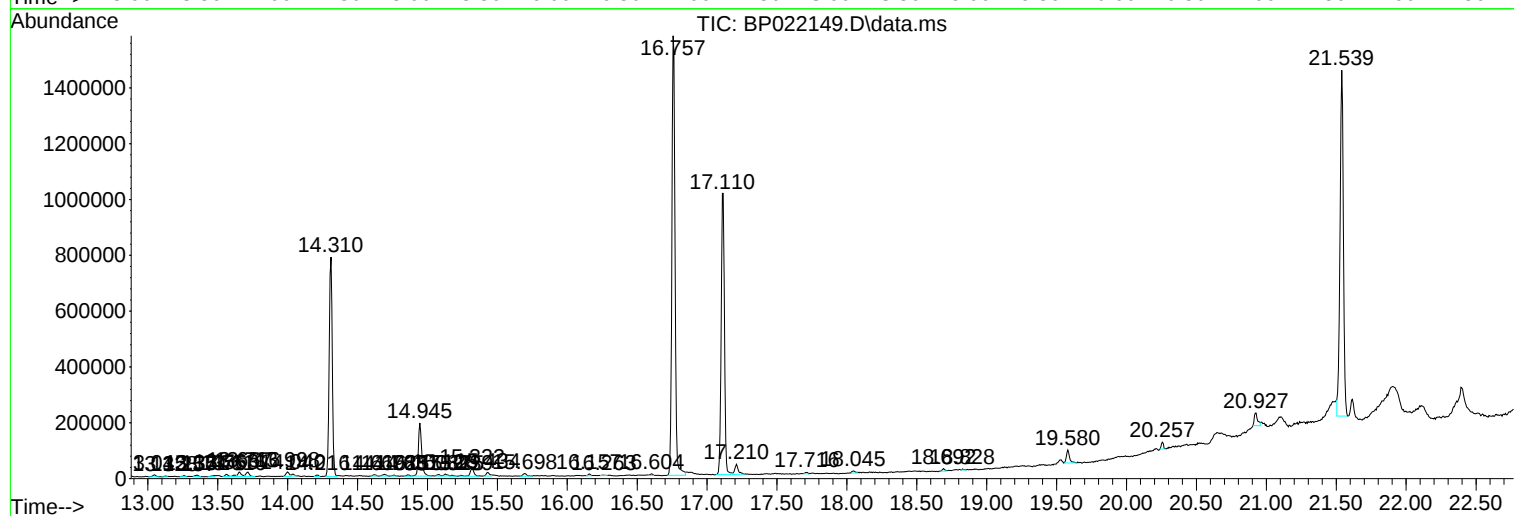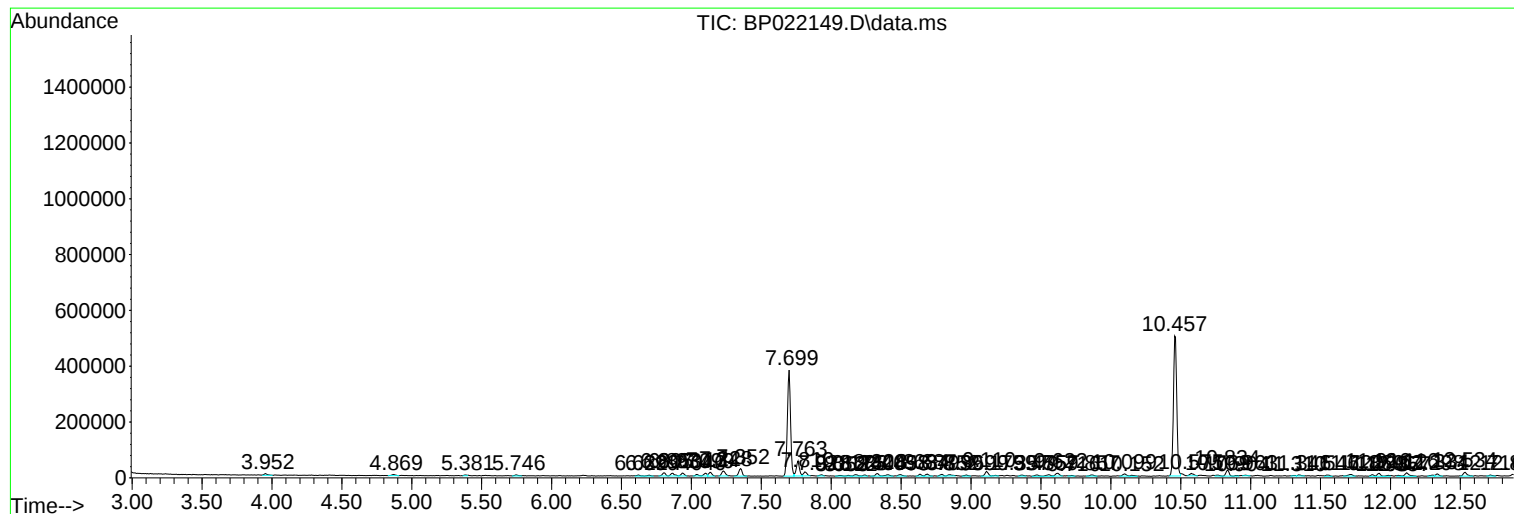

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
Data File : BP022149.D
Acq On : 02 Oct 2024 00:40
Operator : RC/JU
Sample : P4022-08DL 50X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCA6DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Propyl-1-pentanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.763	2.74 ng/ul	82884	1,4-Dichlorobenzene-d4	7.699

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Propyl-1-pentanol			130	C8H18O	058175-57-8	64
2	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	64
3	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	64
4	2-Propyl-1-pentanol			130	C8H18O	058175-57-8	53
5	Pentadecafluorooctanoic acid, 2-...			526	C16H17F15O2	1000406-80-9	50

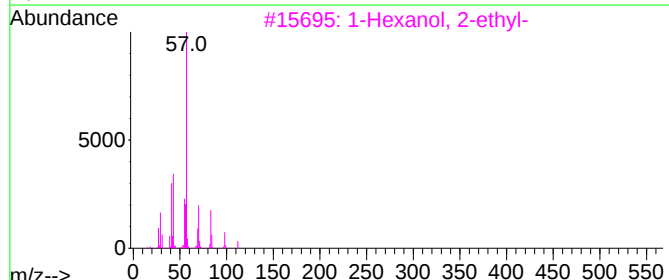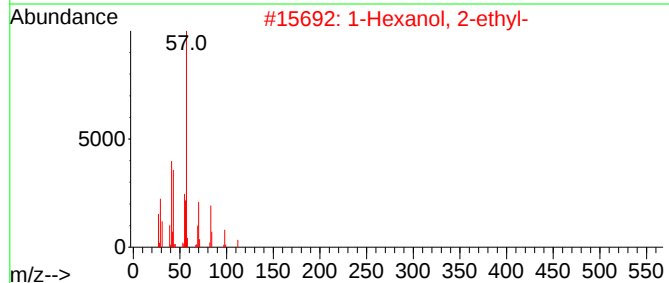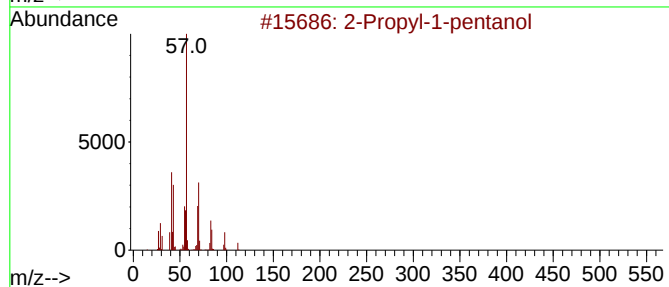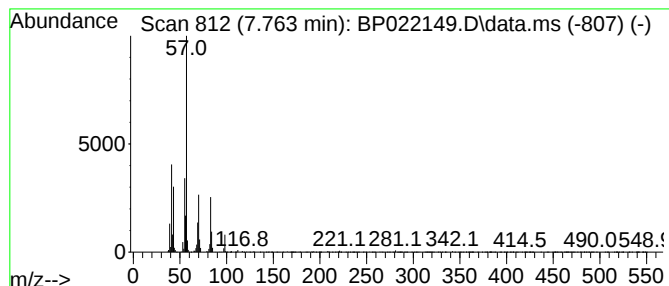

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100124\
Data File : BP022149.D
Acq On : 02 Oct 2024 00:40
Operator : RC/JU
Sample : P4022-08DL 50X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCA6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Propyl-1-pent...	7.763	2.7	ng/u1	82884	1	7.699	605090	20.0