

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
 Data File : BP003467.D
 Acq On : 02 Oct 2020 19:13
 Operator : CG/JU
 Sample : L3863-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HD-02-093020

Quant Time: Oct 03 02:35:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 02 11:17:24 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.522	152	111035	20.00	ng	0.00
21) Naphthalene-d8	10.304	136	450152	20.00	ng	# 0.00
39) Acenaphthene-d10	14.187	164	270820	20.00	ng	0.00
64) Phenanthrene-d10	16.951	188	581419	20.00	ng	# 0.01
76) Chrysene-d12	21.051	240	640760	20.00	ng	0.00
86) Perylene-d12	23.239	264	618897	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.146	112	882292	138.75	ng	0.00
7) Phenol-d6	6.734	99	1000728	118.07	ng	0.00
23) Nitrobenzene-d5	8.681	82	847524	110.61	ng	0.00
42) 2,4,6-Tribromophenol	15.692	330	479219	116.02	ng	0.00
45) 2-Fluorobiphenyl	12.798	172	1727309	93.28	ng	0.00
79) Terphenyl-d14	19.527	244	2491226	81.01	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.657	163	44711	2.07	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003467.D
Acq On : 02 Oct 2020 19:13
Operator : CG/JU
Sample : L3863-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HD-02-093020

Quant Time: Oct 03 02:35:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

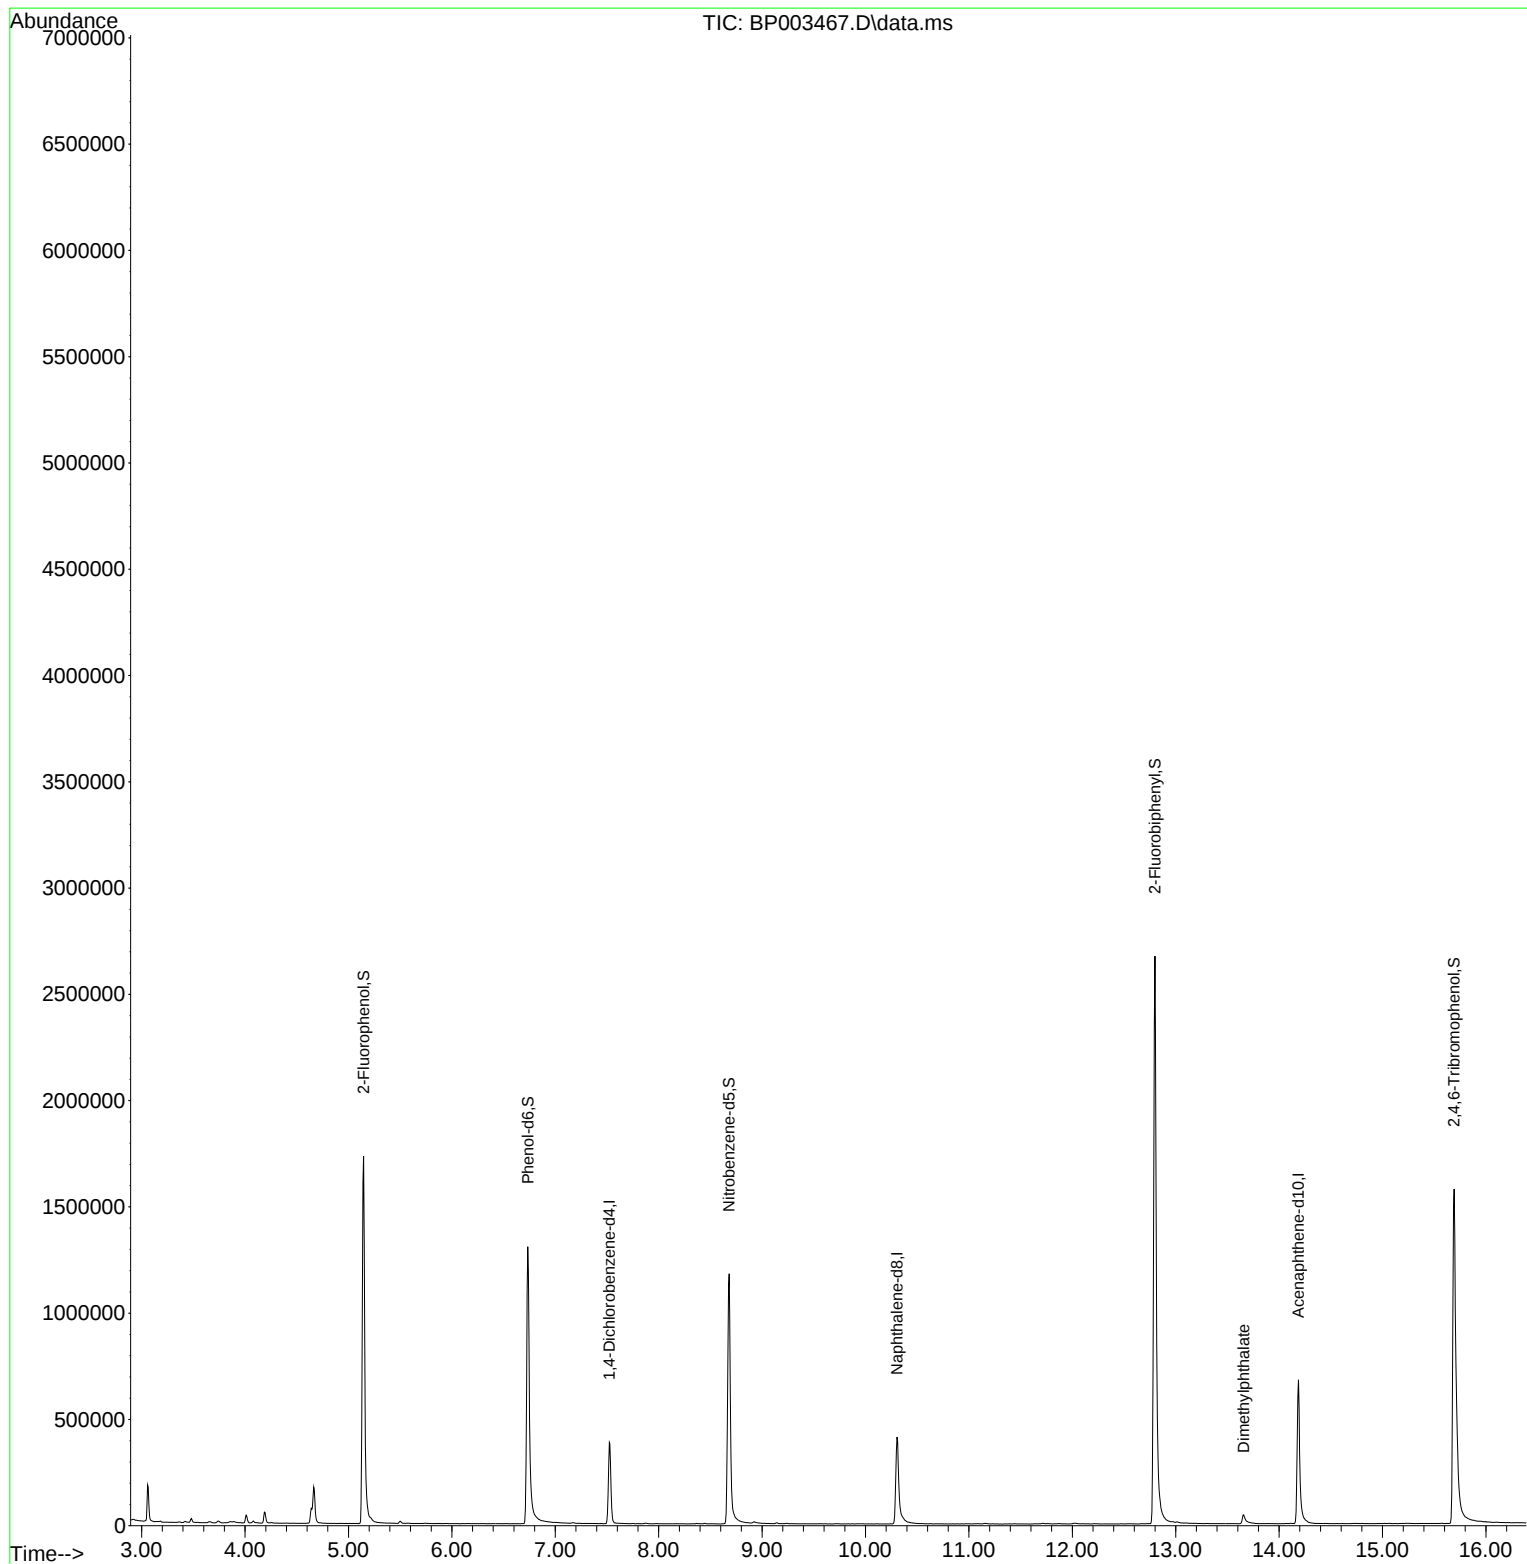

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003467.D
Acq On : 02 Oct 2020 19:13
Operator : CG/JU
Sample : L3863-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HD-02-093020

Quant Time: Oct 03 02:35:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

