

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
 Data File : BP003469.D
 Acq On : 02 Oct 2020 20:21
 Operator : CG/JU
 Sample : L3865-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 NB-07-093020

Quant Time: Oct 03 02:36:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 02 11:17:24 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.528	152	119155	20.00	ng	0.00
21) Naphthalene-d8	10.304	136	487464	20.00	ng	# 0.00
39) Acenaphthene-d10	14.187	164	299191	20.00	ng	0.00
64) Phenanthrene-d10	16.951	188	650183	20.00	ng	# 0.01
76) Chrysene-d12	21.051	240	678809	20.00	ng	0.00
86) Perylene-d12	23.233	264	603472	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.146	112	245685	36.00	ng	0.00
7) Phenol-d6	6.740	99	263102	28.93	ng	0.00
23) Nitrobenzene-d5	8.681	82	244898	29.51	ng	0.00
42) 2,4,6-Tribromophenol	15.698	330	130927	28.69	ng	0.00
45) 2-Fluorobiphenyl	12.804	172	549853	26.88	ng	0.00
79) Terphenyl-d14	19.527	244	868479	26.66	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003469.D
Acq On : 02 Oct 2020 20:21
Operator : CG/JU
Sample : L3865-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
NB-07-093020

Quant Time: Oct 03 02:36:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

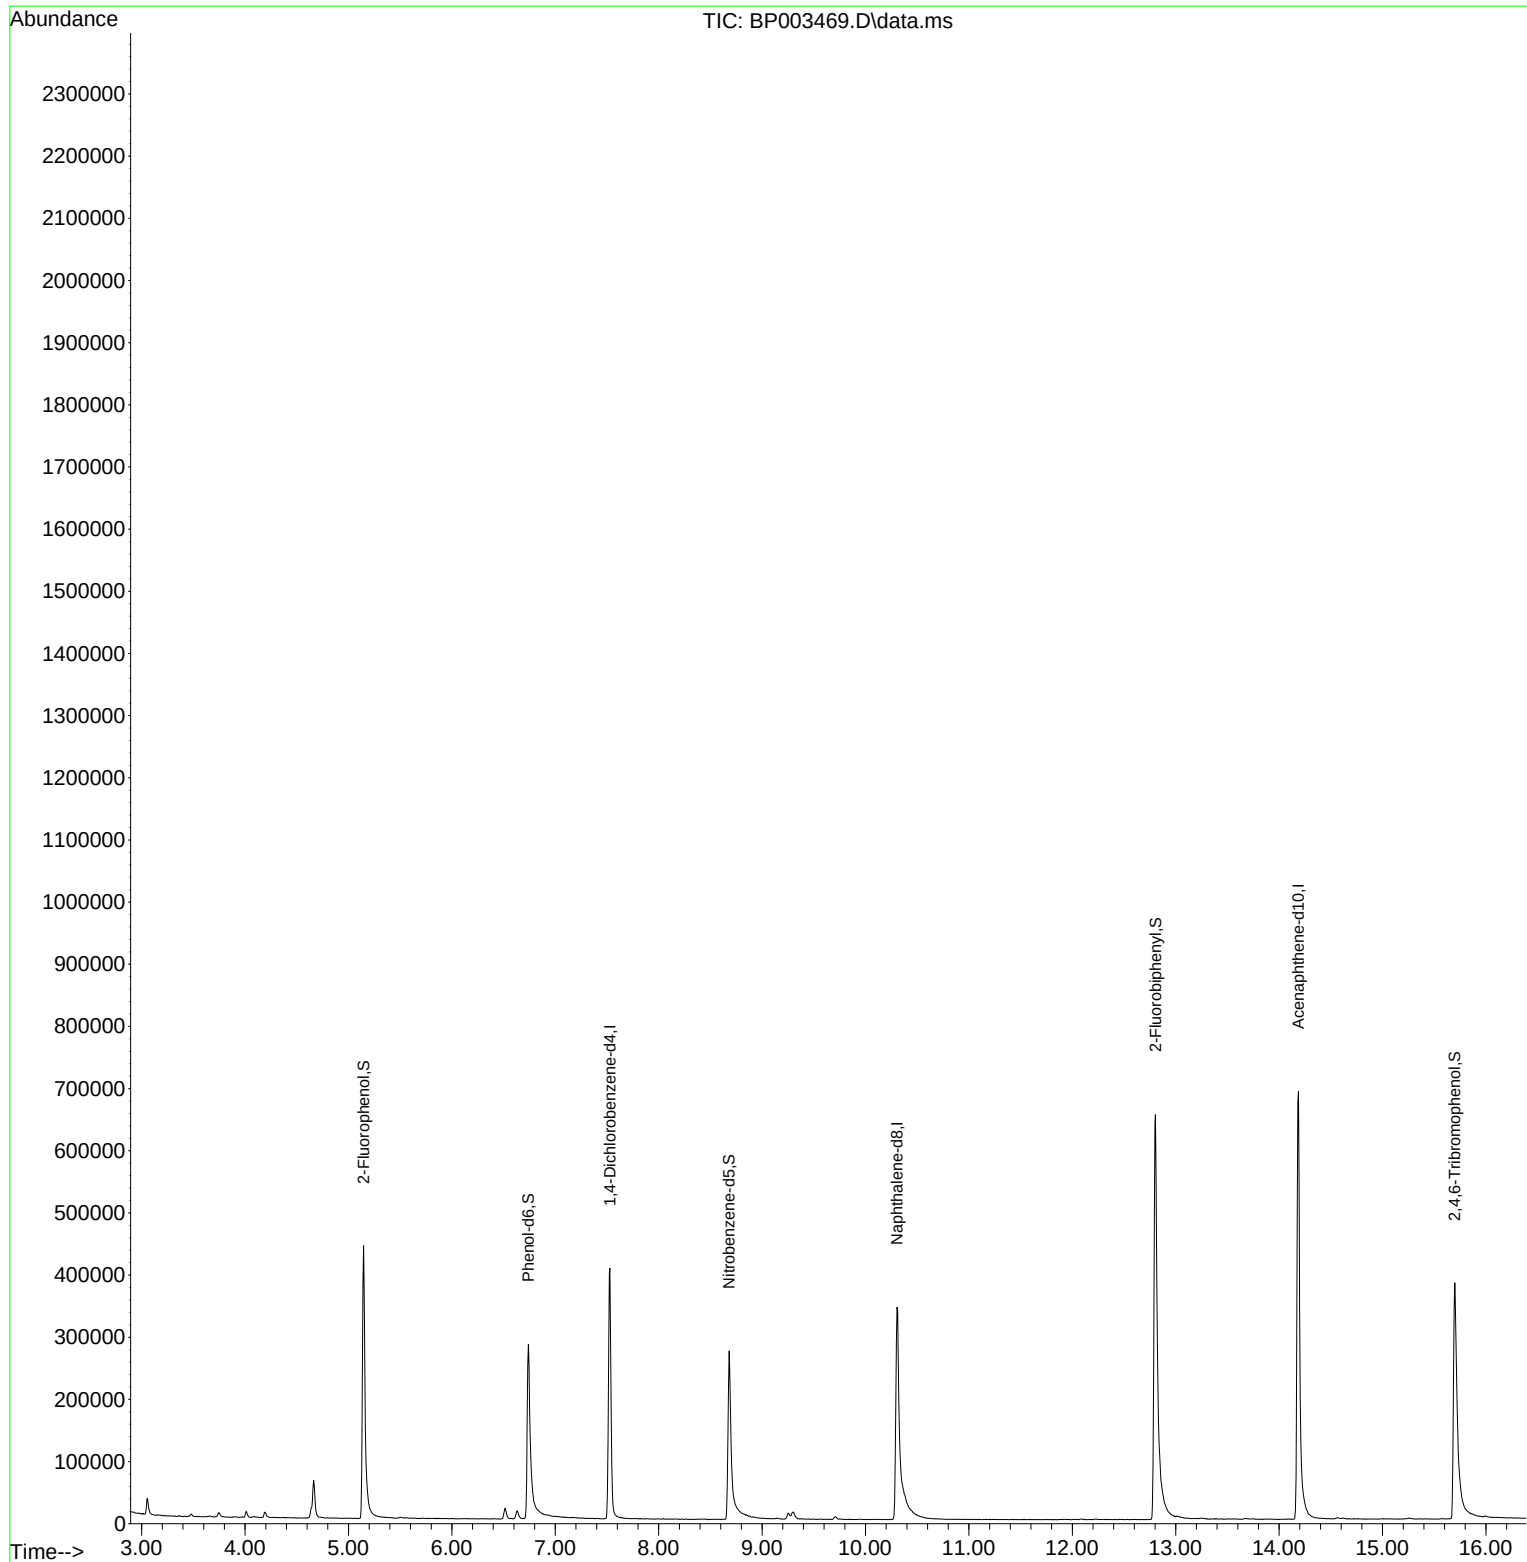

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003469.D
Acq On : 02 Oct 2020 20:21
Operator : CG/JU
Sample : L3865-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
NB-07-093020

Quant Time: Oct 03 02:36:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

