

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
 Data File : BP003470.D
 Acq On : 02 Oct 2020 20:56
 Operator : CG/JU
 Sample : L3870-20
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SU-03-093020

Quant Time: Oct 03 02:36:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 02 11:17:24 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.528	152	98490	20.00	ng	0.00
21) Naphthalene-d8	10.304	136	401342	20.00	ng	# 0.00
39) Acenaphthene-d10	14.187	164	245545	20.00	ng	0.00
64) Phenanthrene-d10	16.951	188	529781	20.00	ng	# 0.01
76) Chrysene-d12	21.051	240	607713	20.00	ng	0.00
86) Perylene-d12	23.239	264	609708	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.146	112	809010	143.43	ng	0.00
7) Phenol-d6	6.734	99	955573	127.10	ng	0.00
23) Nitrobenzene-d5	8.681	82	768282	112.46	ng	0.00
42) 2,4,6-Tribromophenol	15.692	330	434887	116.12	ng	0.00
45) 2-Fluorobiphenyl	12.798	172	1645041	97.98	ng	0.00
79) Terphenyl-d14	19.527	244	2359120	80.88	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.657	163	41813	2.13	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003470.D
Acq On : 02 Oct 2020 20:56
Operator : CG/JU
Sample : L3870-20
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SU-03-093020

Quant Time: Oct 03 02:36:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

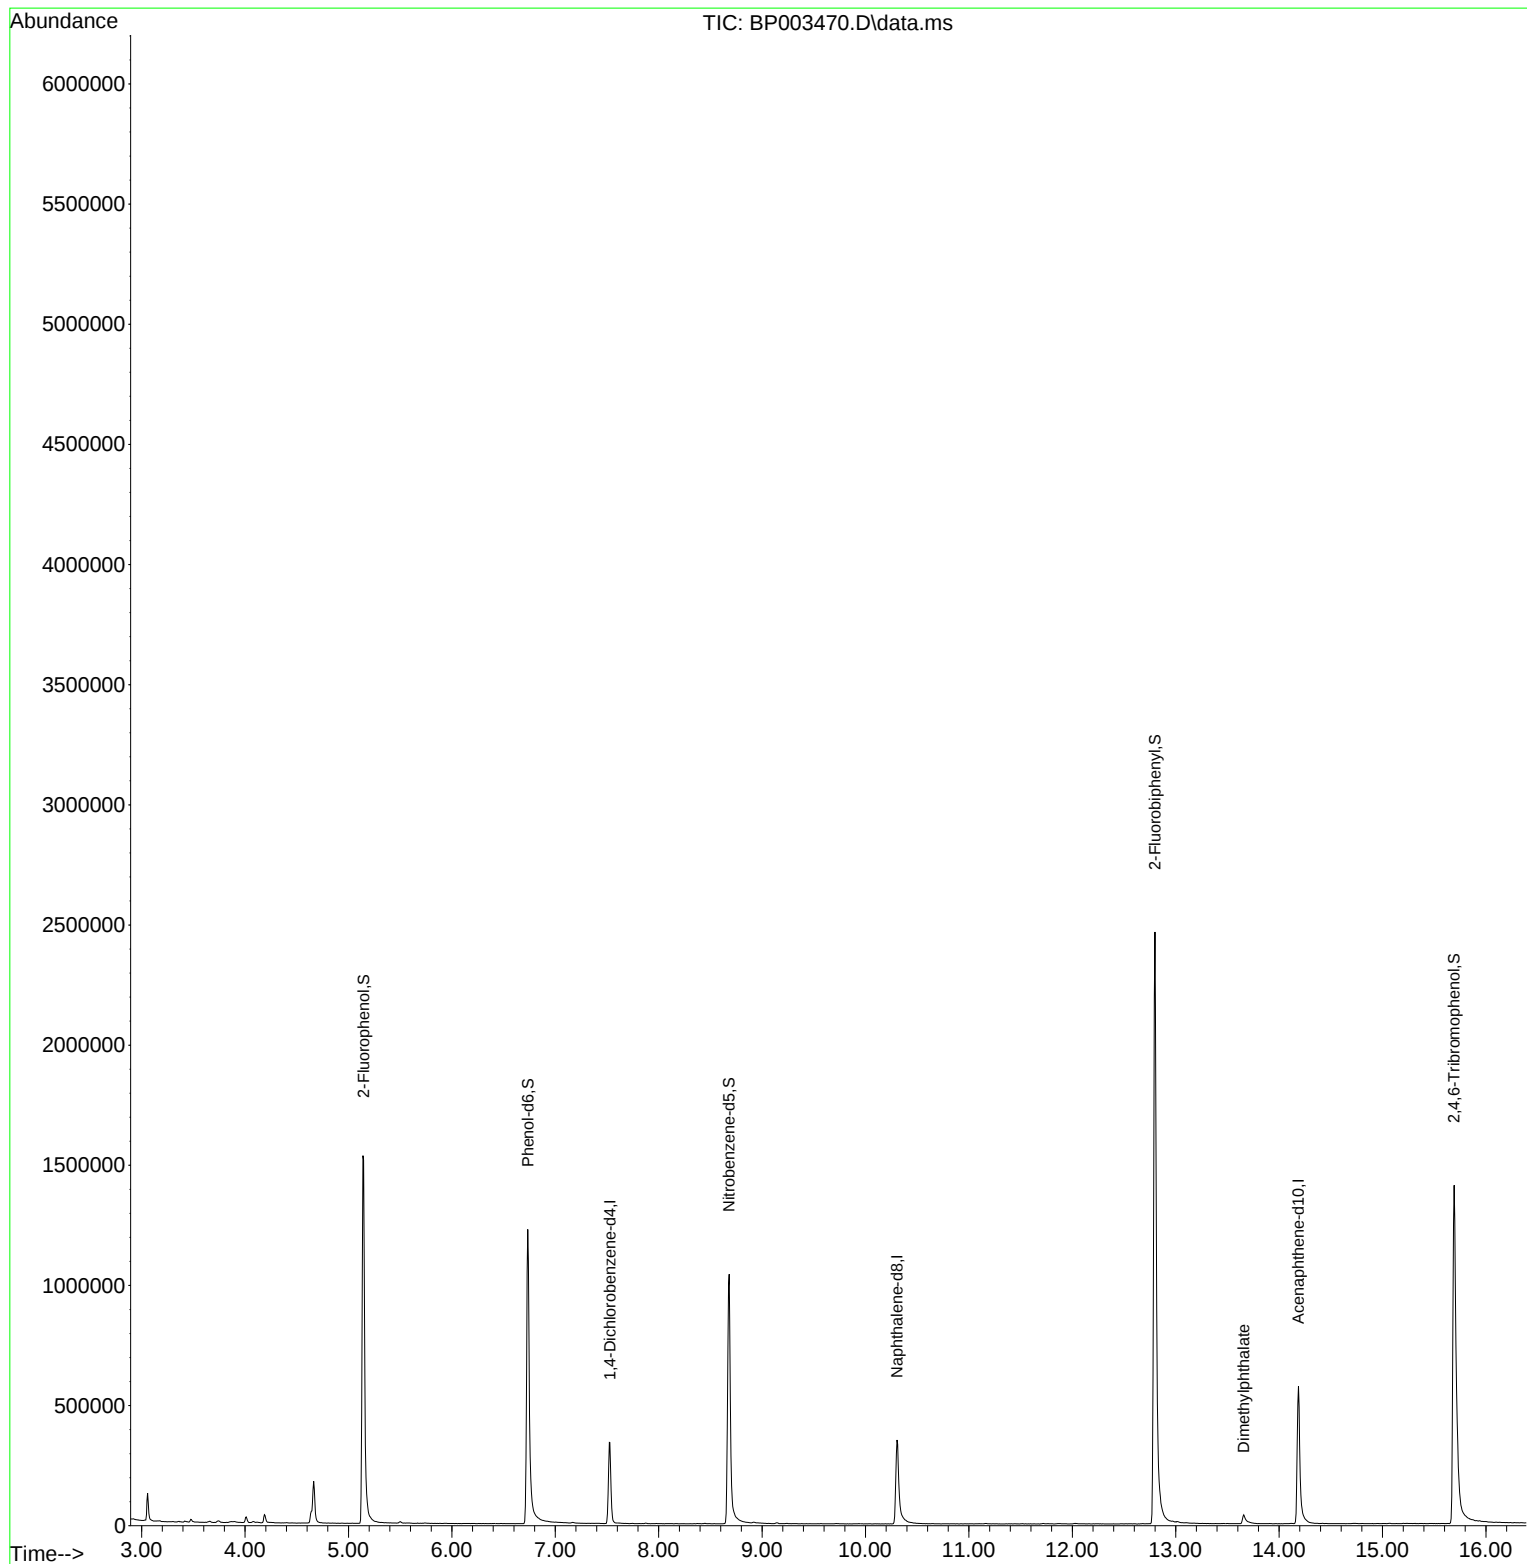

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003470.D
Acq On : 02 Oct 2020 20:56
Operator : CG/JU
Sample : L3870-20
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SU-03-093020

Quant Time: Oct 03 02:36:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

