

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
 Data File : BP003478.D
 Acq On : 03 Oct 2020 04:34
 Operator : CG/JU
 Sample : L4198-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RO-25

Quant Time: Oct 03 06:23:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 02 11:17:24 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.528	152	107800	20.00	ng	0.00
21) Naphthalene-d8	10.304	136	434336	20.00	ng	# 0.00
39) Acenaphthene-d10	14.187	164	268800	20.00	ng	0.00
64) Phenanthrene-d10	16.951	188	598418	20.00	ng	# 0.01
76) Chrysene-d12	21.051	240	652444	20.00	ng	0.00
86) Perylene-d12	23.239	264	599348	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.146	112	829572	134.37	ng	0.00
7) Phenol-d6	6.734	99	942638	114.55	ng	0.00
23) Nitrobenzene-d5	8.681	82	827638	111.95	ng	0.00
42) 2,4,6-Tribromophenol	15.692	330	472231	115.18	ng	0.00
45) 2-Fluorobiphenyl	12.798	172	1707707	92.92	ng	0.00
79) Terphenyl-d14	19.527	244	2646827	84.53	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003478.D
Acq On : 03 Oct 2020 04:34
Operator : CG/JU
Sample : L4198-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-25

Quant Time: Oct 03 06:23:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

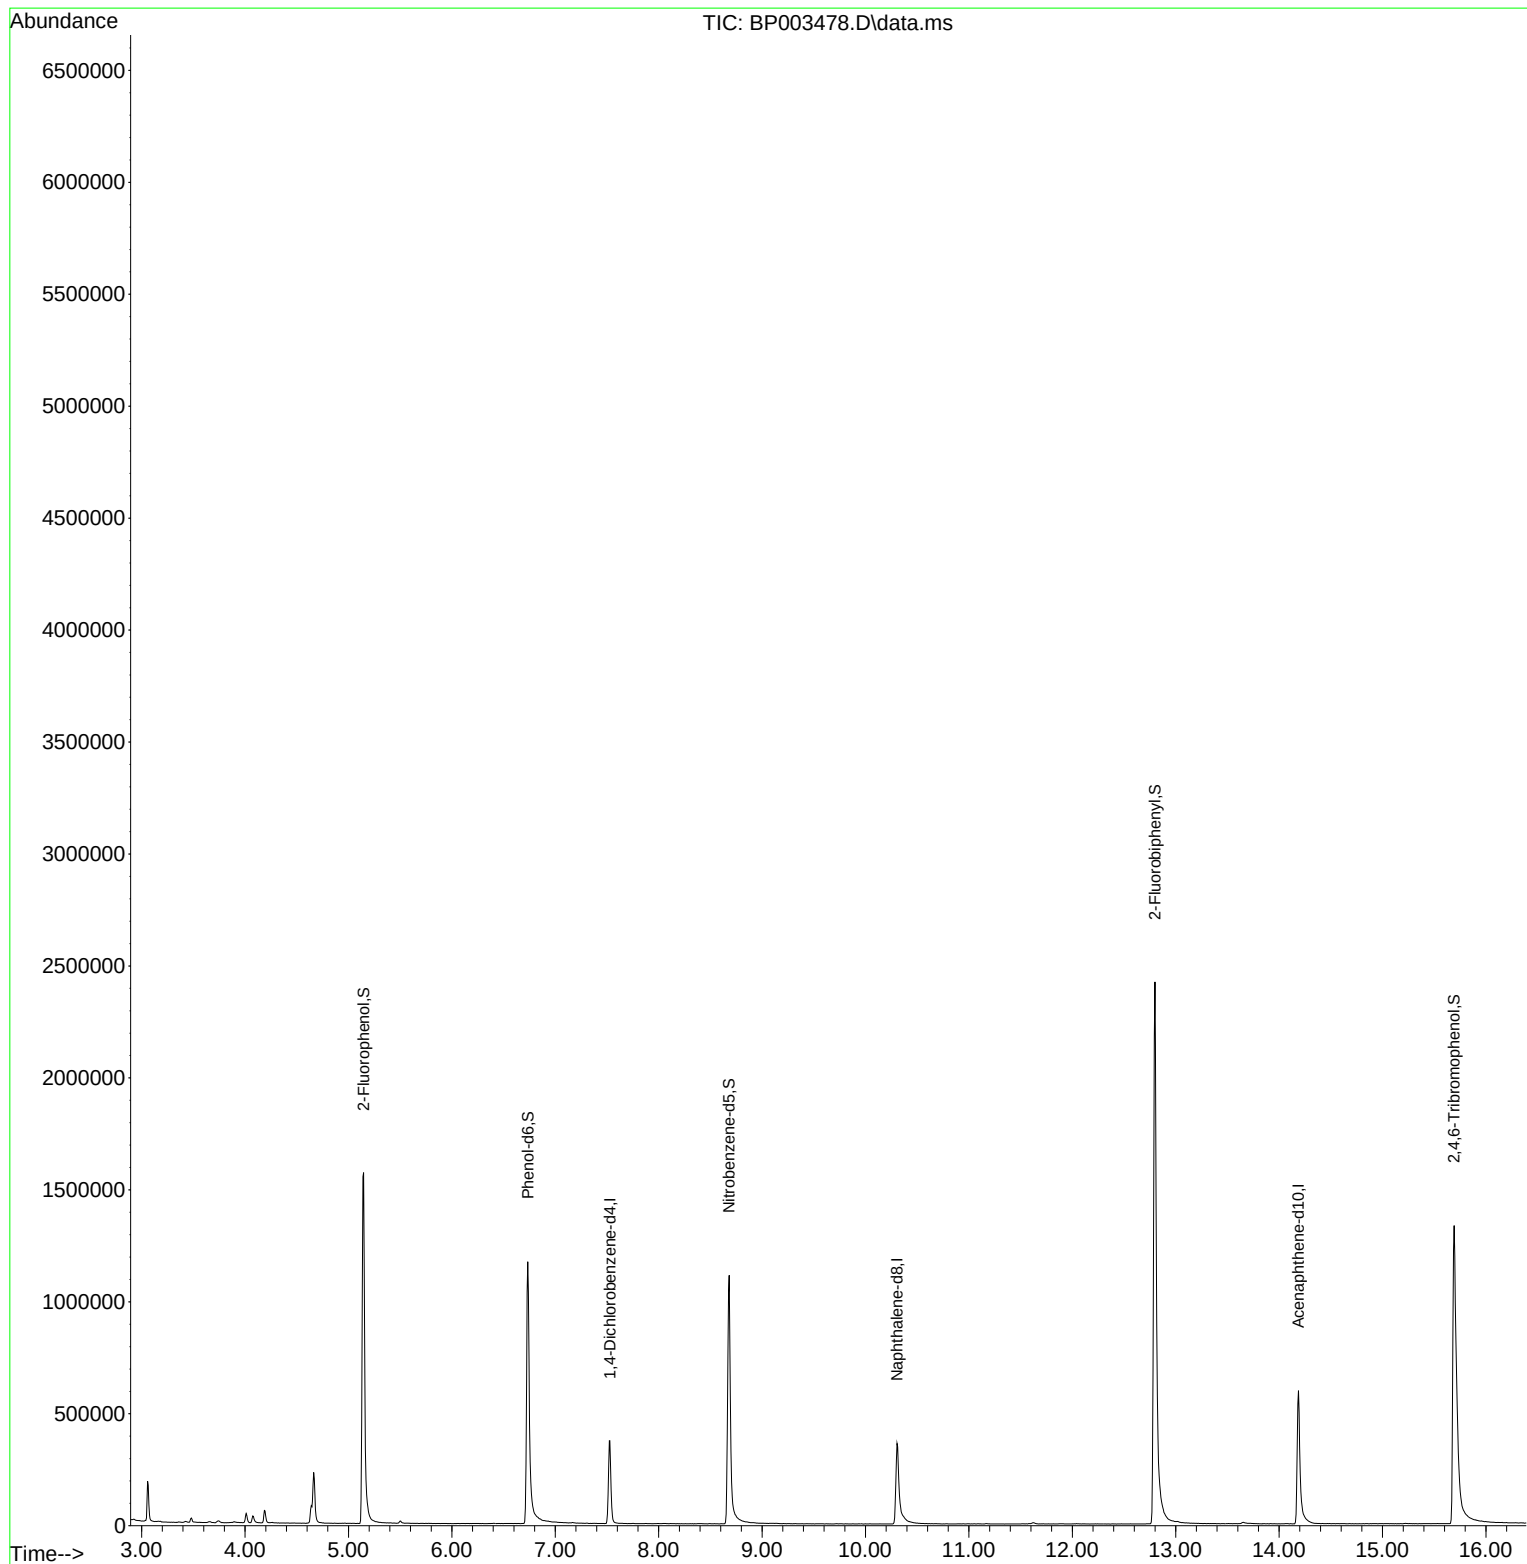

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003478.D
Acq On : 03 Oct 2020 04:34
Operator : CG/JU
Sample : L4198-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-25

Quant Time: Oct 03 06:23:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

