

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
 Data File : BP003480.D
 Acq On : 03 Oct 2020 05:42
 Operator : CG/JU
 Sample : L4198-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RO-10

Quant Time: Oct 03 06:24:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 02 11:17:24 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.528	152	116395	20.00	ng	0.00
21) Naphthalene-d8	10.304	136	469147	20.00	ng	# 0.00
39) Acenaphthene-d10	14.186	164	282969	20.00	ng	0.00
64) Phenanthrene-d10	16.951	188	622158	20.00	ng	# 0.01
76) Chrysene-d12	21.057	240	626321	20.00	ng	0.00
86) Perylene-d12	23.245	264	541899	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.146	112	966185	144.95	ng	0.00
7) Phenol-d6	6.734	99	1145754	128.95	ng	0.00
23) Nitrobenzene-d5	8.681	82	903831	113.18	ng	0.00
42) 2,4,6-Tribromophenol	15.692	330	494136	114.49	ng	0.00
45) 2-Fluorobiphenyl	12.798	172	1844500	95.33	ng	0.00
79) Terphenyl-d14	19.527	244	2700330	89.83	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003480.D
Acq On : 03 Oct 2020 05:42
Operator : CG/JU
Sample : L4198-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-10

Quant Time: Oct 03 06:24:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

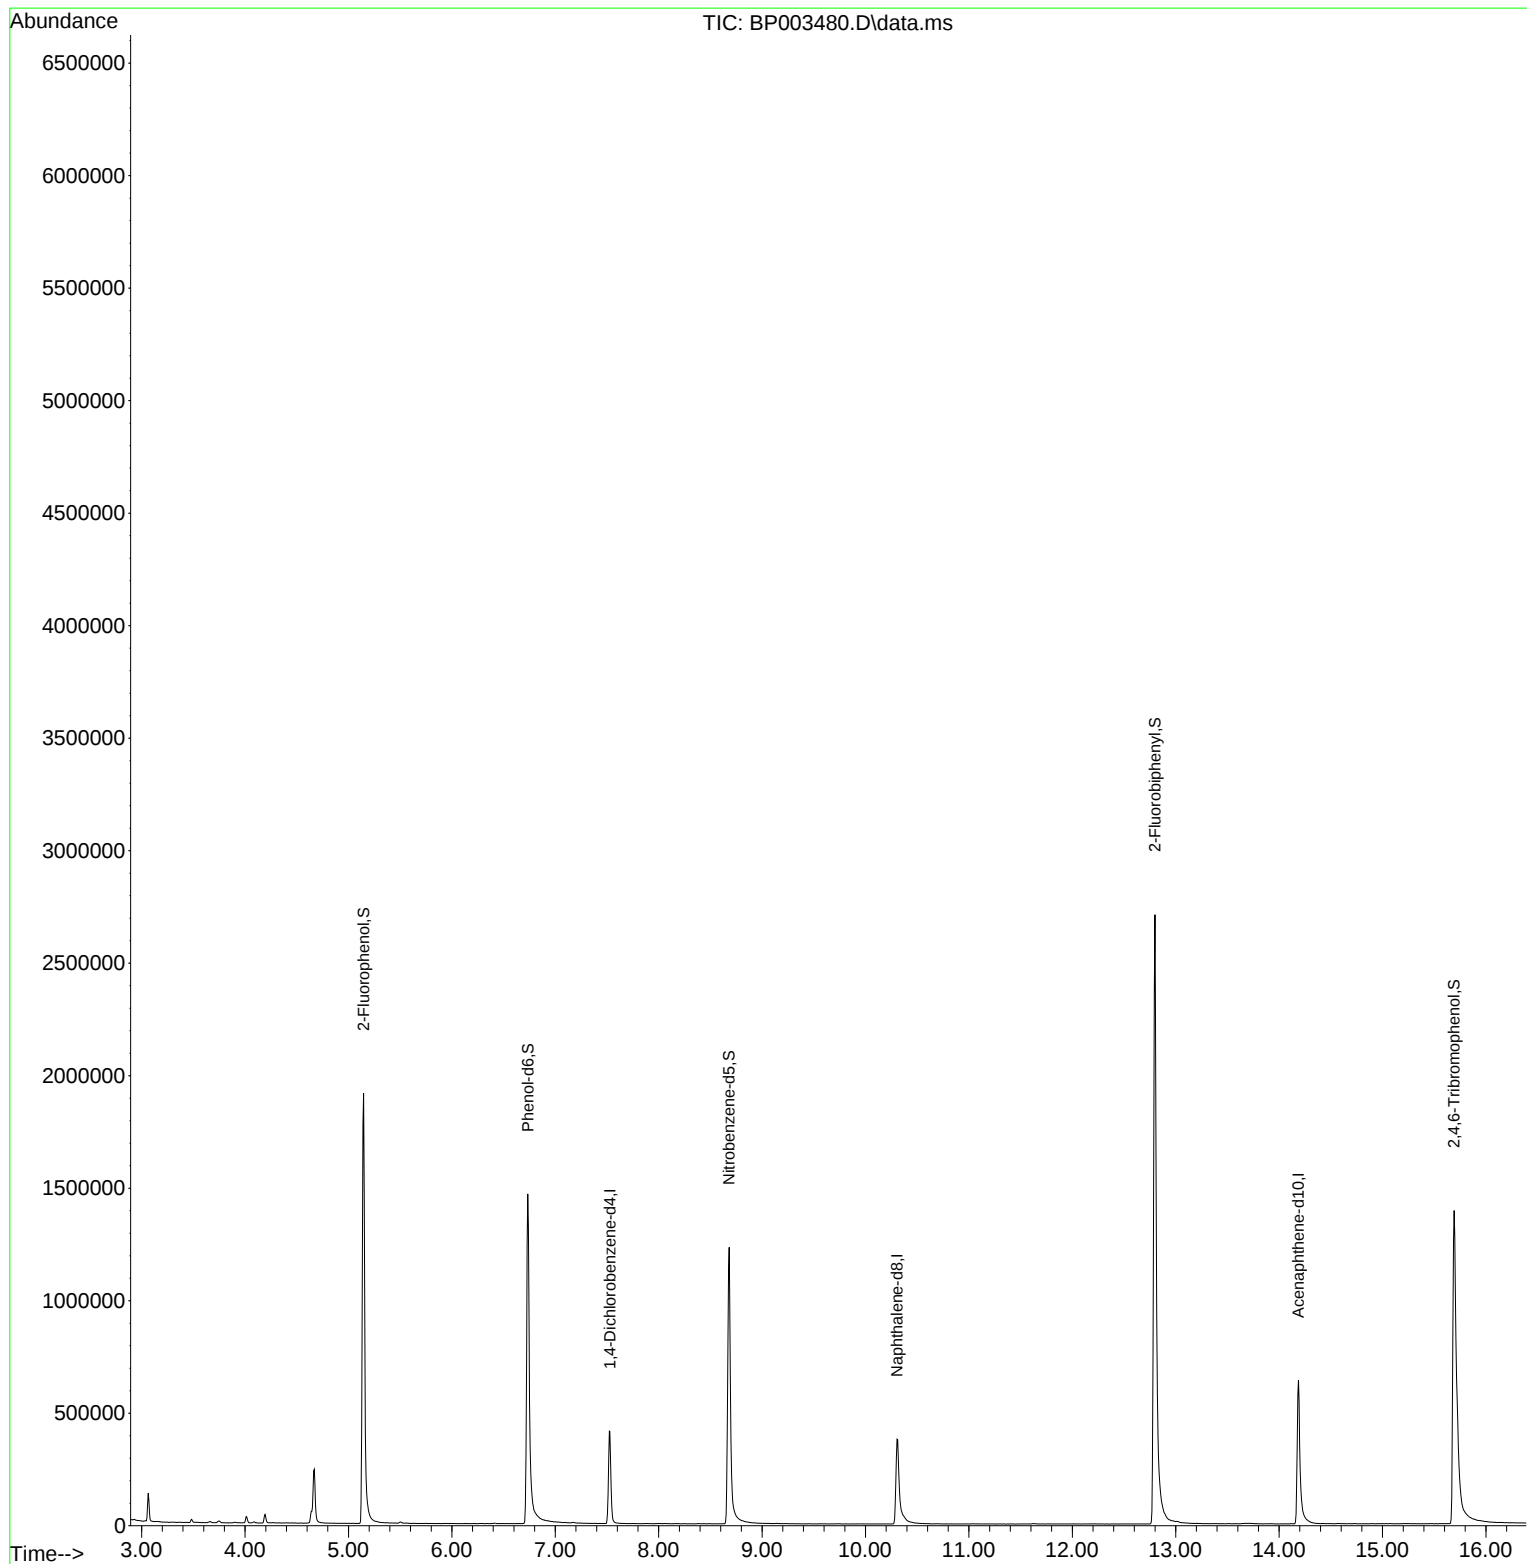

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003480.D
Acq On : 03 Oct 2020 05:42
Operator : CG/JU
Sample : L4198-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-10

Quant Time: Oct 03 06:24:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

