
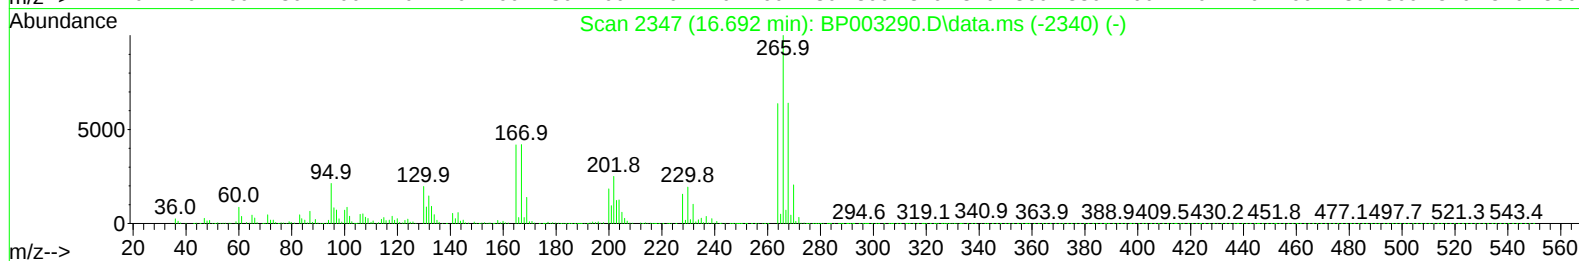
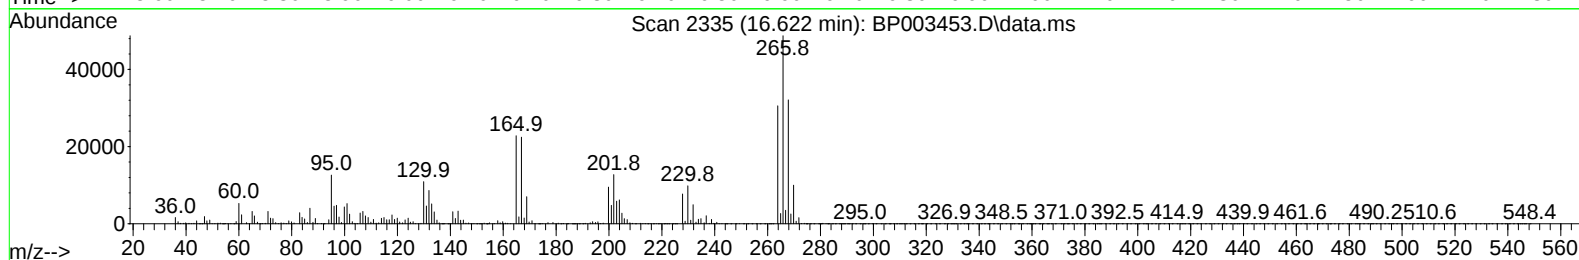


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003453.D
Acq On : 02 Oct 2020 10:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 05:23:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

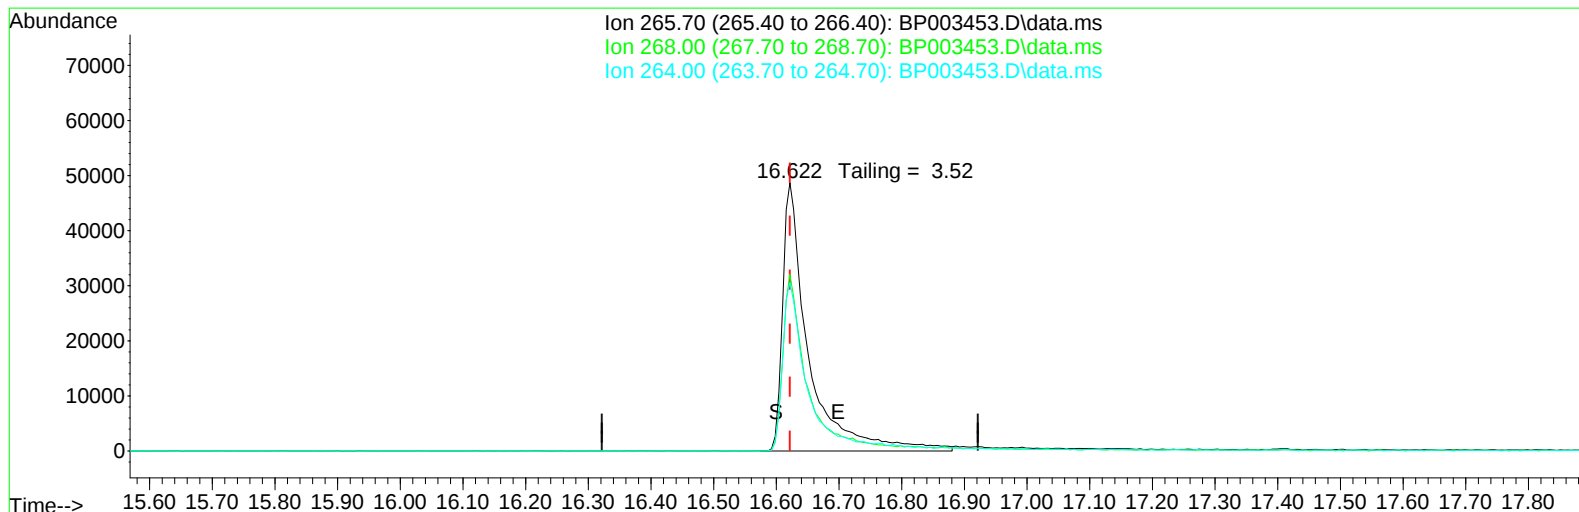

TIC: BP003453.D\data.ms

(70) Pentachlorophenol (C)




16.622min (+ 0.000) 1090973.57 ng

response 139581

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.83
264.00	63.30	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003453.D
Acq On : 02 Oct 2020 10:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 05:23:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 11:17:24 2020
Response via : Initial Calibration

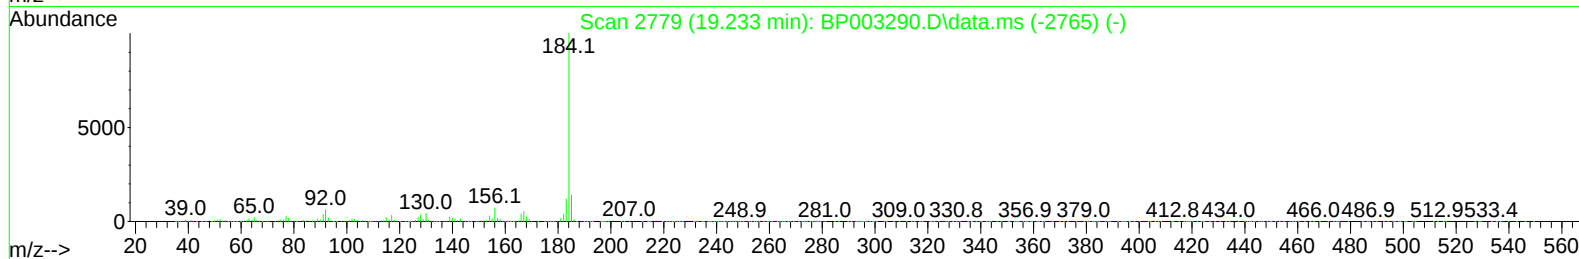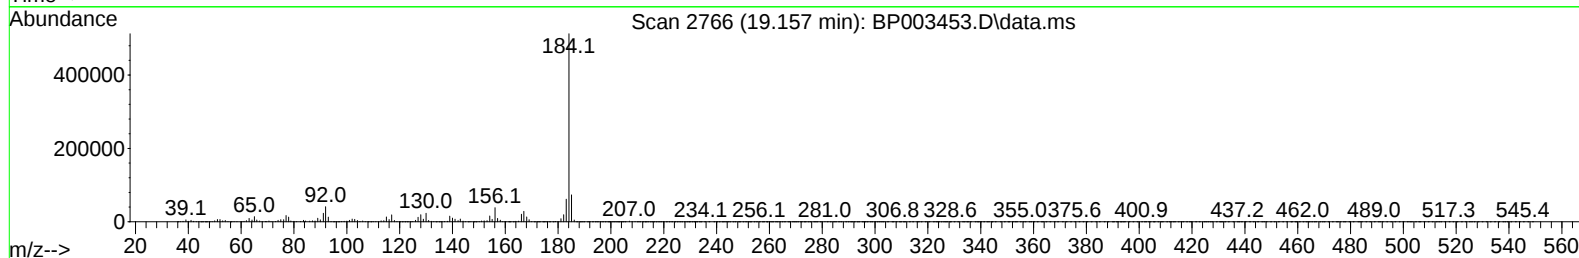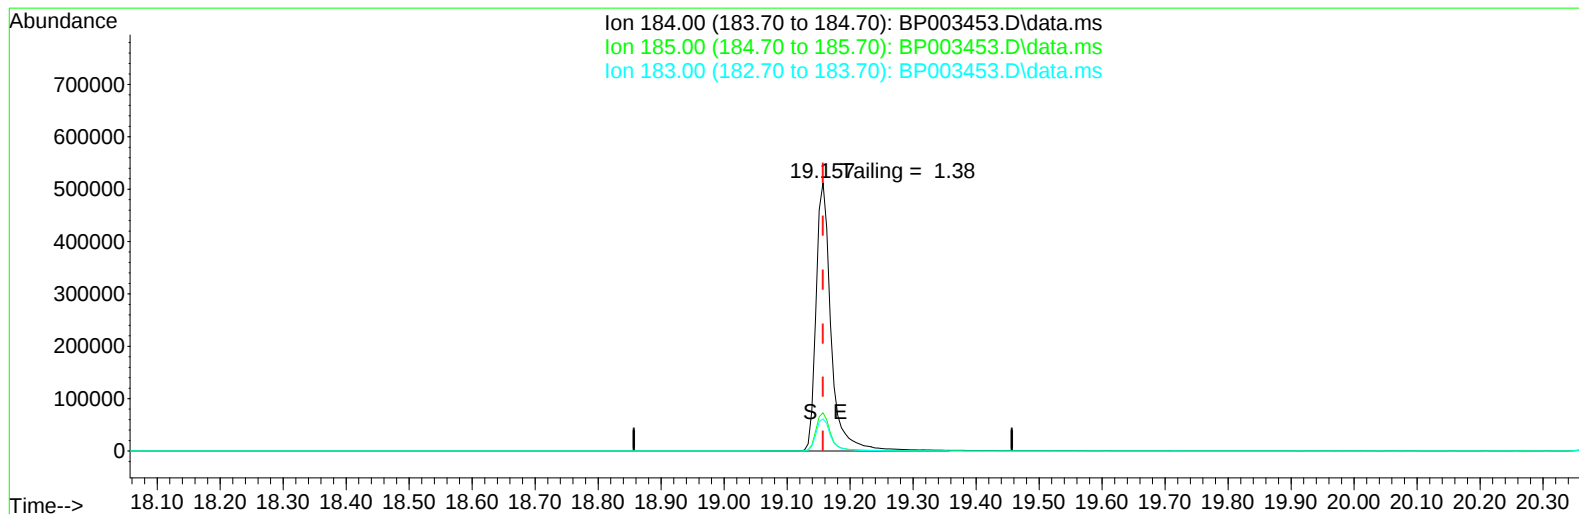

TIC: BP003453.D\data.ms

(77) Benzidine**19.157min (+ 0.000) 163907.12 ng****response 853871**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.29
183.00	12.00	12.03
0.00	0.00	0.00