

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
 Data File : BP003465.D
 Acq On : 02 Oct 2020 18:05
 Operator : CG/JU
 Sample : L4195-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RBR-251673

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.140	377	383	413	rBV	1230994	2104023	61.24%	8.443%
2	6.734	647	654	679	rBV	1058478	2056939	59.87%	8.254%
3	7.522	782	788	800	rBV	410413	684086	19.91%	2.745%
4	8.681	976	985	1012	rBV	722009	1487077	43.28%	5.968%
5	10.305	1252	1261	1300	rBV	416732	975792	28.40%	3.916%
6	12.799	1678	1685	1712	rBV	1355056	2803030	81.58%	11.248%
7	13.651	1824	1830	1857	rBV	156632	330014	9.60%	1.324%
8	14.187	1914	1921	1941	rBV2	708292	1295030	37.69%	5.197%
9	15.693	2169	2177	2212	rBV	986320	2251142	65.52%	9.034%
10	16.945	2383	2390	2405	rBV	877092	1620505	47.16%	6.503%
11	17.875	2544	2548	2555	rVB	22235	37683	1.10%	0.151%
12	18.010	2567	2571	2575	rBV2	23622	40856	1.19%	0.164%
13	18.722	2687	2692	2696	rBV	21822	34461	1.00%	0.138%
14	18.975	2730	2735	2742	rBV	195667	271657	7.91%	1.090%
15	19.322	2786	2794	2804	rBV	191830	322894	9.40%	1.296%
16	19.528	2823	2829	2844	rVB	2597538	3435875	100.00%	13.788%
17	19.651	2845	2850	2857	rVB3	15985	36986	1.08%	0.148%
18	19.969	2900	2904	2910	rBV2	25417	36593	1.07%	0.147%
19	20.775	3037	3041	3047	rVV3	229617	380690	11.08%	1.528%
20	20.833	3047	3051	3060	rVB	124948	199333	5.80%	0.800%
21	21.051	3081	3088	3092	rBV	1391950	2044998	59.52%	8.207%
22	21.204	3111	3114	3118	rVB3	36935	40866	1.19%	0.164%
23	22.198	3279	3283	3294	rVB	86081	133900	3.90%	0.537%
24	22.580	3343	3348	3353	rBV	103852	230447	6.71%	0.925%
25	23.045	3423	3427	3434	rVB	56499	93569	2.72%	0.375%
26	23.139	3439	3443	3451	rVV	90844	169980	4.95%	0.682%
27	23.233	3452	3459	3477	rVB2	908250	1800744	52.41%	7.226%




Sum of corrected areas: 24919170

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003465.D
Acq On : 02 Oct 2020 18:05
Operator : CG/JU
Sample : L4195-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RBR-251673

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

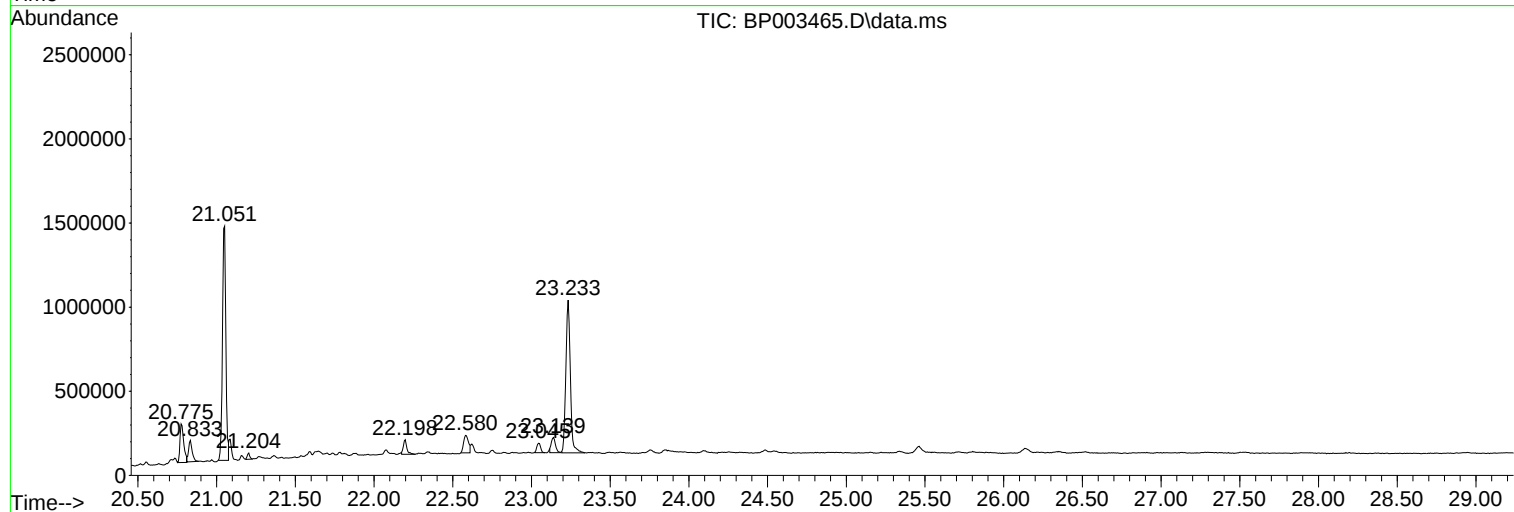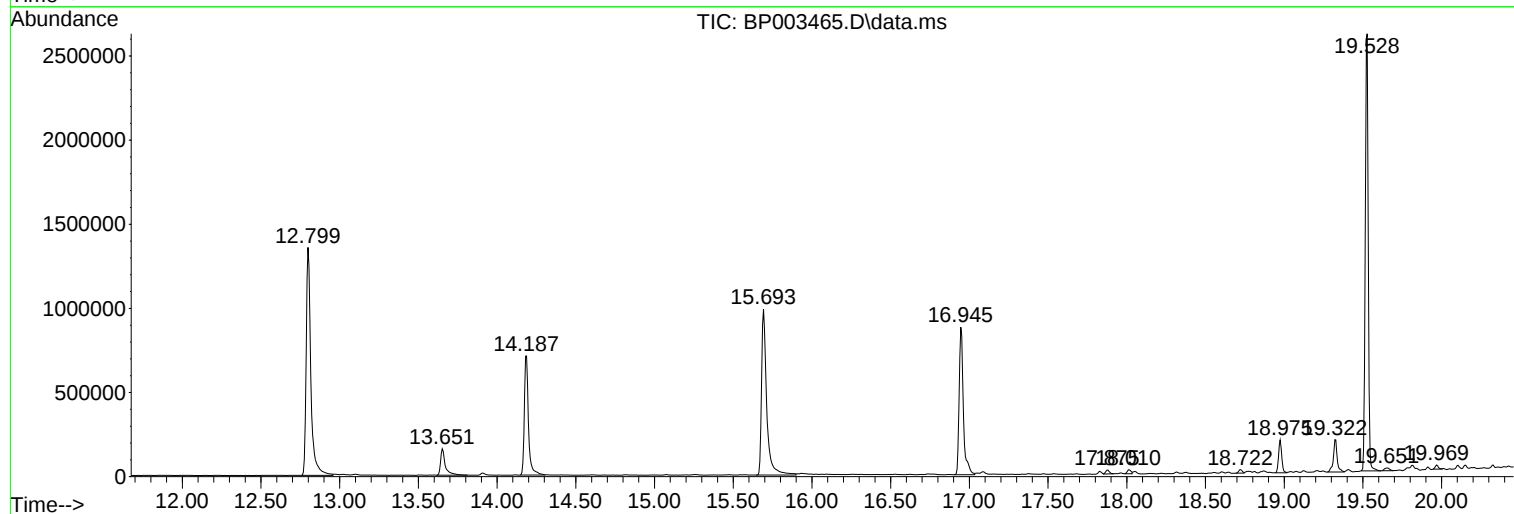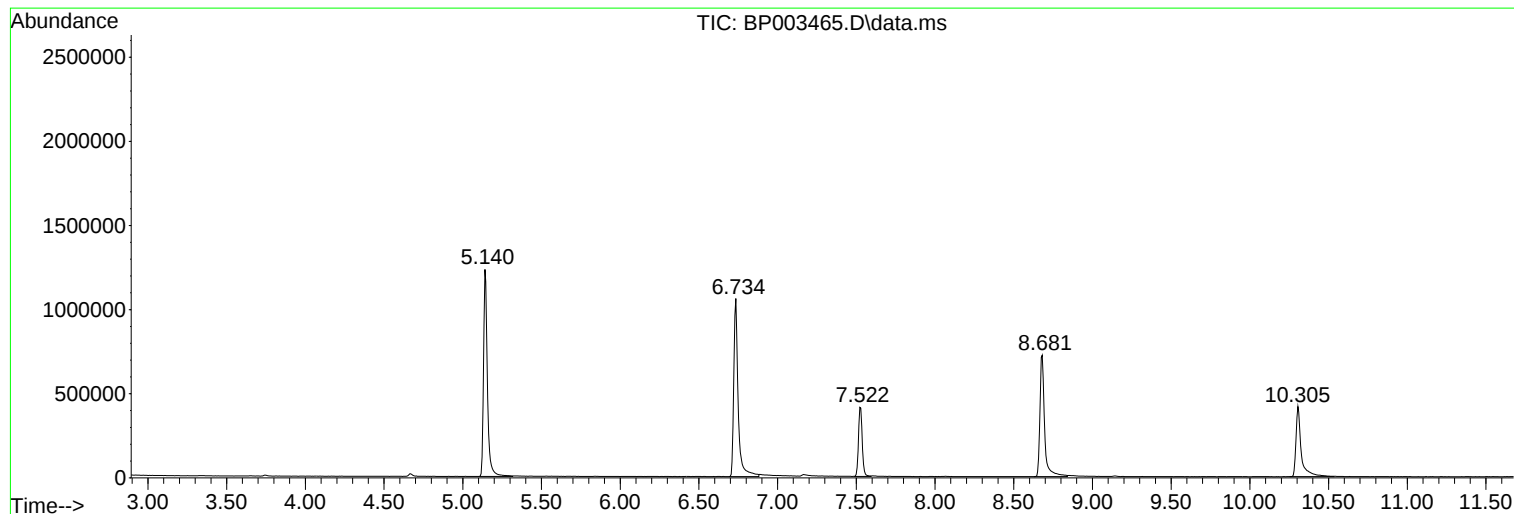

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003465.D
Acq On : 02 Oct 2020 18:05
Operator : CG/JU
Sample : L4195-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RBR-251673










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclohexadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.775	3.72 ng	380690	Chrysene-d12	21.051

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexadecane	224	C16H32	000295-65-8	94
2			Behenic alcohol	326	C22H46O	000661-19-8	93
3			5-Octadecene, (E)-	252	C18H36	007206-21-5	93
4			n-Nonadecanol-1	284	C19H40O	001454-84-8	91
5			1-Octadecene	252	C18H36	000112-88-9	90

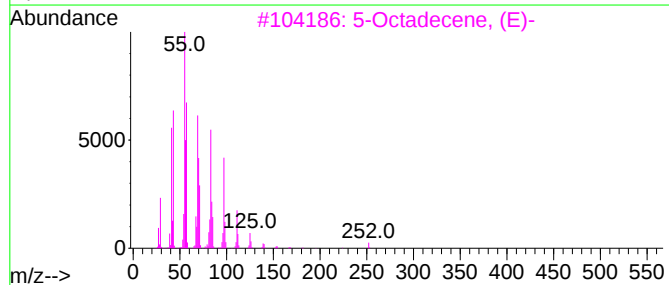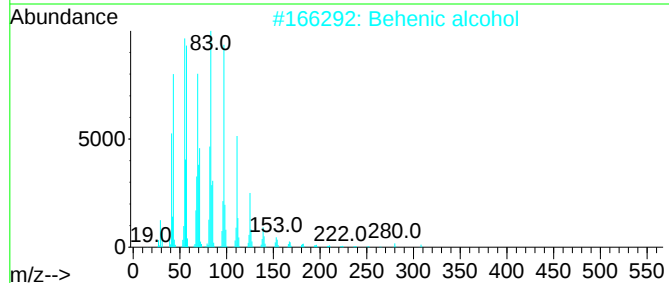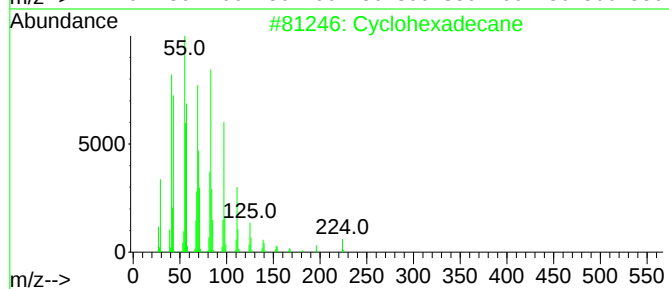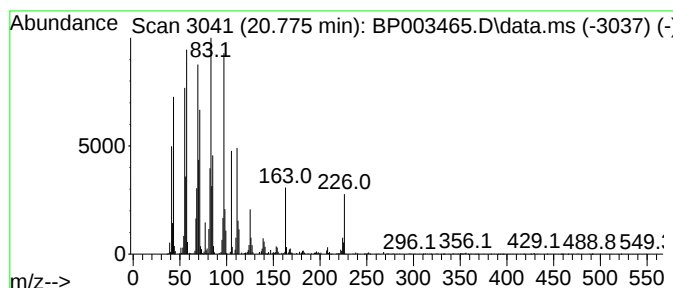

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
Data File : BP003465.D
Acq On : 02 Oct 2020 18:05
Operator : CG/JU
Sample : L4195-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RBR-251673

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclohexadecane	20.775	3.7	ng	380690	5	21.051	2045000	20.0