
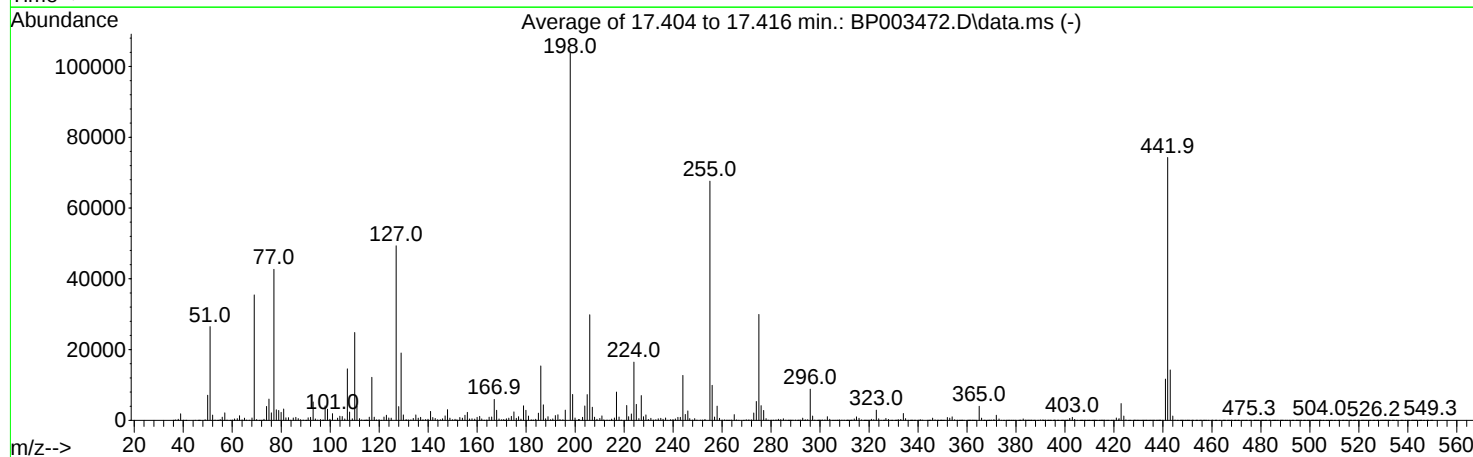


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100220\
 Data File : BP003472.D
 Acq On : 03 Oct 2020 00:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 02 11:17:24 2020

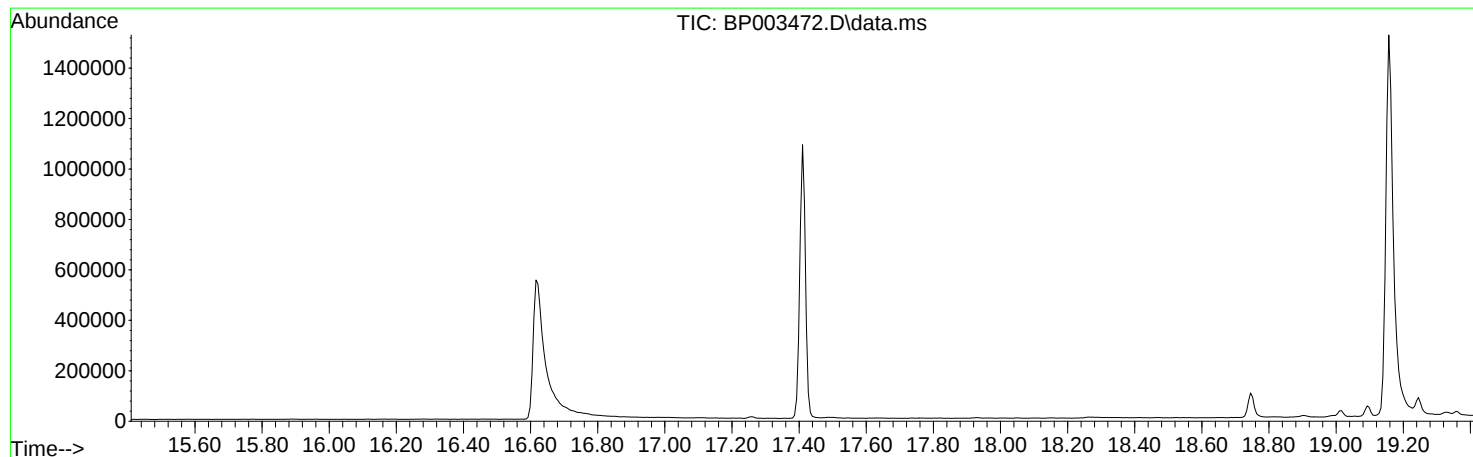

Spectrum Information: Average of 17.404 to 17.416 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	26487	PASS
68	69	0.00	2	1.9	675	PASS
69	198	0.00	100	34.1	35441	PASS
70	69	0.00	2	0.7	250	PASS
127	198	10	80	47.5	49323	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	103944	PASS
199	198	5	9	7.0	7324	PASS
275	198	10	60	28.8	29925	PASS
365	198	1	100	3.8	3996	PASS
441	198	0.01	100	11.2	11676	PASS
442	198	50	100	71.5	74280	PASS
443	442	15	24	19.2	14234	PASS